

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
 Data File : BM017041.D
 Acq On : 05 Oct 2018 18:38
 Operator : MJ/SJ
 Sample : PB113579BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.869	654	660	670	rVB	797448	1240579	22.10%	2.331%
2	7.040	683	689	697	rVB	671094	993315	17.69%	1.867%
3	7.228	715	721	731	rVB	809578	1290876	22.99%	2.426%
4	7.698	794	801	811	rVB	679513	1081980	19.27%	2.033%
5	8.398	913	920	933	rVB	1037926	1632178	29.07%	3.067%
6	8.845	989	996	1009	rVB	825039	1343983	23.94%	2.525%
7	9.563	1111	1118	1128	rBV	648105	1026842	18.29%	1.930%
8	10.092	1201	1208	1220	rBV	1053171	1717808	30.60%	3.228%
9	10.475	1263	1273	1281	rVB	973341	1604949	28.59%	3.016%
10	10.610	1288	1296	1308	rBV	1078834	1882494	33.53%	3.537%
11	12.069	1539	1544	1550	rVB2	16915	27908	0.50%	0.052%
12	13.751	1823	1830	1842	rBV	2215947	2995954	53.36%	5.630%
13	14.027	1870	1877	1887	rBV	2530182	3587073	63.89%	6.740%
14	14.333	1923	1929	1937	rBV2	1354493	2103957	37.47%	3.953%
15	14.539	1956	1964	1980	rBV	929136	1299906	23.15%	2.443%
16	15.333	2092	2099	2108	rBV	3286259	4574938	81.49%	8.597%
17	15.451	2113	2119	2128	rBV	745123	997213	17.76%	1.874%
18	15.568	2135	2139	2146	rBV2	30095	41269	0.74%	0.078%
19	16.868	2355	2360	2364	rBV3	4483	7250	0.13%	0.014%
20	17.080	2390	2396	2403	rBV2	1665812	2349439	41.85%	4.415%
21	17.180	2406	2413	2427	rBV2	3443838	4883254	86.98%	9.176%
22	19.115	2737	2742	2747	rBV	31898	44728	0.80%	0.084%
23	19.362	2781	2784	2789	rBV	21584	27776	0.49%	0.052%
24	19.480	2797	2804	2812	rBV	4172017	5357733	95.43%	10.068%
25	21.268	3103	3108	3115	rBV	2127039	2604022	46.38%	4.893%
26	23.356	3456	3463	3478	rBV	2920832	5614327	100.00%	10.550%
27	23.491	3480	3486	3498	rVB2	1403392	2658484	47.35%	4.995%
28	24.033	3574	3578	3586	rVB2	126398	227533	4.05%	0.428%


Sum of corrected areas: 53217768

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
Data File : BM017041.D
Acq On : 05 Oct 2018 18:38
Operator : MJ/SJ
Sample : PB113579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

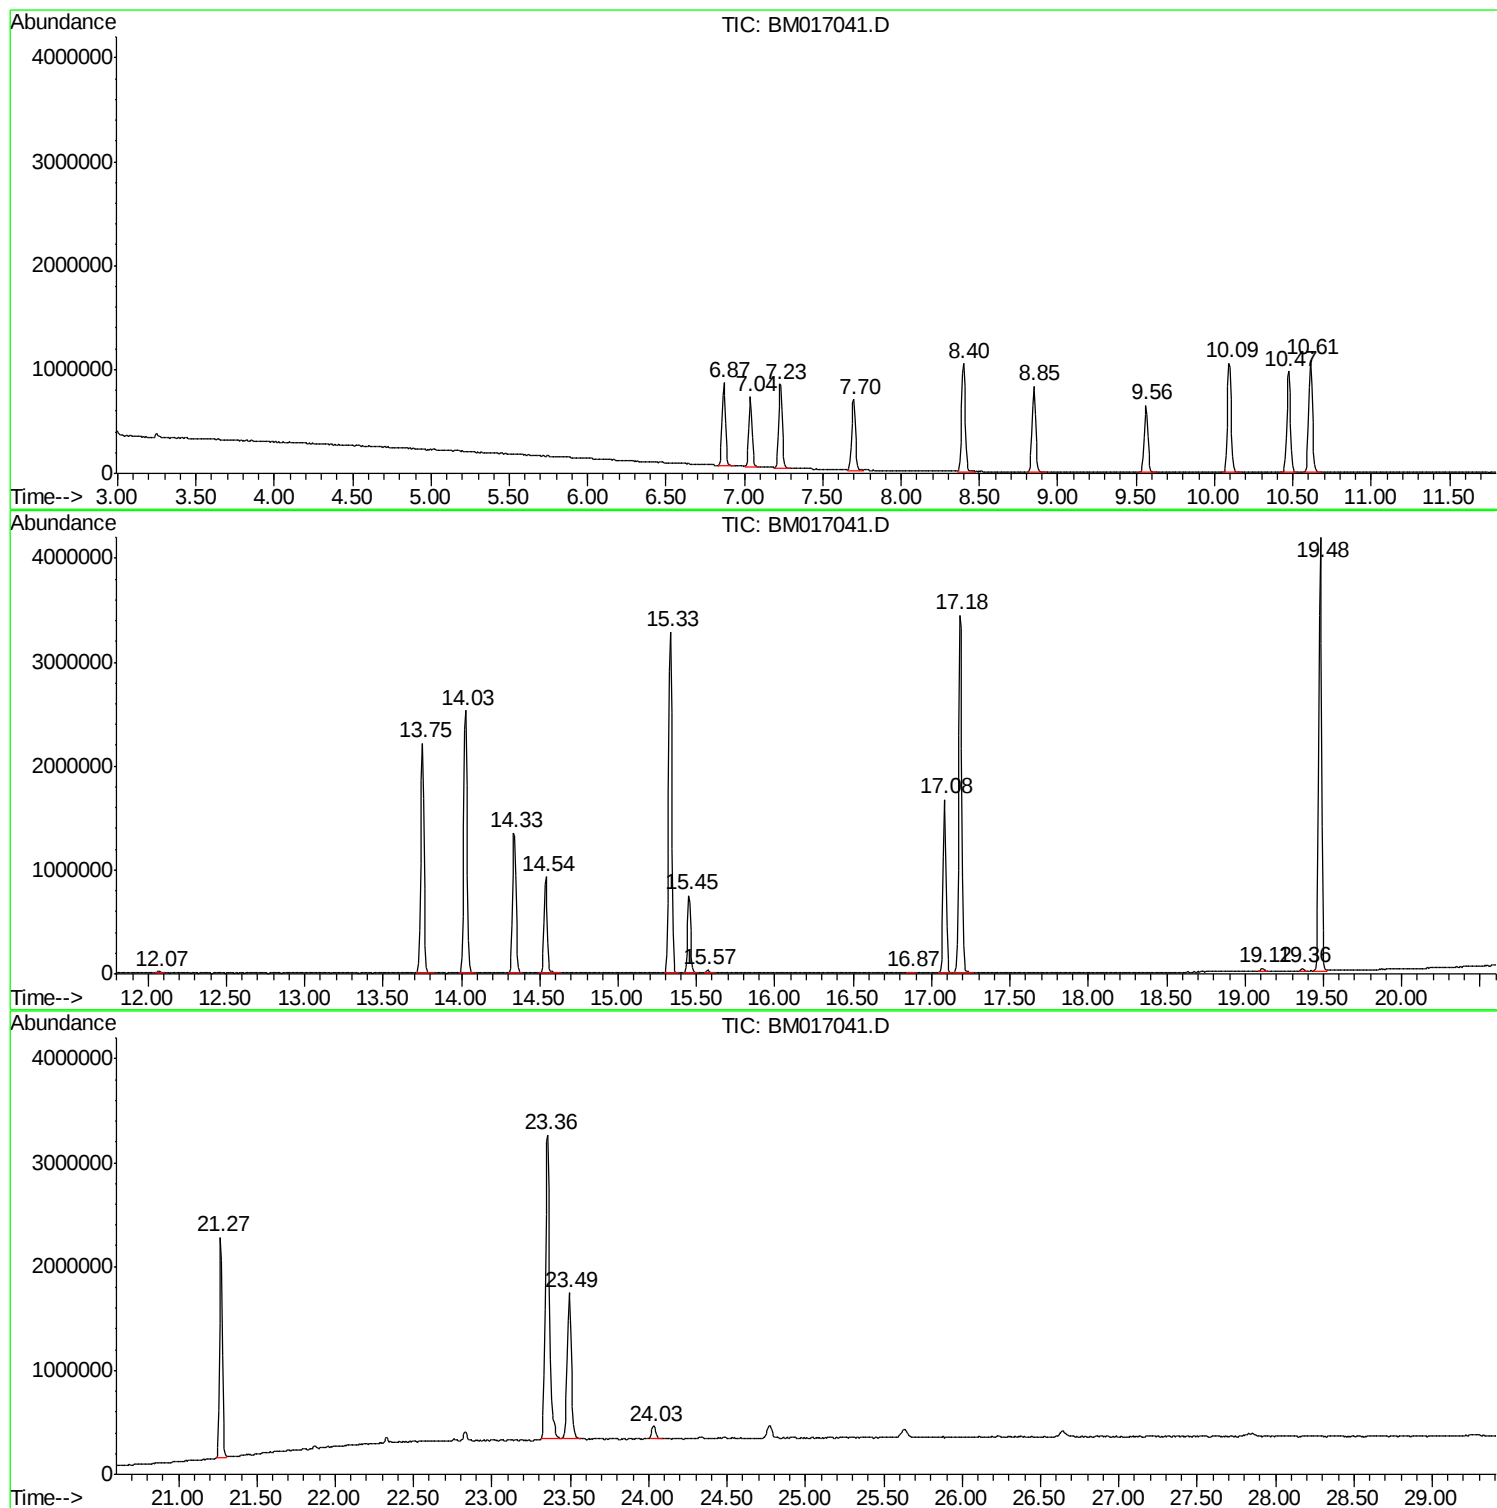

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
Data File : BM017041.D
Acq On : 05 Oct 2018 18:38
Operator : MJ/SJ
Sample : PB113579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
Data File : BM017041.D
Acq On : 05 Oct 2018 18:38
Operator : MJ/SJ
Sample : PB113579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc