

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
 Data File : BM017044.D
 Acq On : 05 Oct 2018 20:27
 Operator : MJ/SJ
 Sample : J5298-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E62W2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.869	655	660	671	rVB2	210376	370836	6.75%	0.720%
2	7.040	683	689	697	rVB	729399	1096270	19.96%	2.129%
3	7.228	715	721	728	rVB	757475	1192357	21.71%	2.315%
4	7.699	794	801	808	rVB	750511	1204232	21.92%	2.338%
5	7.757	808	811	820	rVB4	10122	23394	0.43%	0.045%
6	8.399	913	920	929	rVV	583986	916764	16.69%	1.780%
7	8.475	929	933	936	rVB2	4932	7134	0.13%	0.014%
8	8.757	977	981	986	rBV3	21187	33902	0.62%	0.066%
9	8.846	989	996	1004	rVB	898407	1471841	26.79%	2.858%
10	9.046	1027	1030	1036	rVB6	7807	12263	0.22%	0.024%
11	9.110	1038	1041	1044	rVV3	6198	7881	0.14%	0.015%
12	9.157	1044	1049	1053	rVV4	7473	13330	0.24%	0.026%
13	9.228	1055	1061	1072	rVB3	31477	65523	1.19%	0.127%
14	9.563	1111	1118	1129	rVB	702799	1107839	20.17%	2.151%
15	9.728	1142	1146	1151	rVB6	5956	9821	0.18%	0.019%
16	9.851	1163	1167	1171	rVB3	4858	6281	0.11%	0.012%
17	10.093	1202	1208	1220	rBV	1091516	1817822	33.09%	3.530%
18	10.304	1240	1244	1249	rBV5	6475	8156	0.15%	0.016%
19	10.375	1252	1256	1261	rBV6	8411	13755	0.25%	0.027%
20	10.475	1261	1273	1280	rVV	1105148	1817663	33.09%	3.529%
21	10.540	1280	1284	1286	rVV4	10791	18467	0.34%	0.036%
22	10.563	1286	1288	1292	rVV5	9210	16168	0.29%	0.031%
23	10.622	1292	1298	1306	rVB3	70522	137070	2.50%	0.266%
24	10.910	1345	1347	1353	rVB5	3515	5911	0.11%	0.011%
25	11.069	1369	1374	1379	rVB5	9607	15602	0.28%	0.030%
26	11.234	1396	1402	1408	rVB5	3715	8345	0.15%	0.016%
27	11.592	1459	1463	1468	rVB4	5015	6778	0.12%	0.013%
28	11.681	1473	1478	1482	rBV5	7722	13250	0.24%	0.026%
29	11.757	1487	1491	1495	rVB5	9355	14203	0.26%	0.028%
30	11.887	1509	1513	1518	rBV3	8467	12550	0.23%	0.024%
31	12.063	1539	1543	1554	rBV	18464	36640	0.67%	0.071%
32	12.187	1560	1564	1568	rVB3	12073	15861	0.29%	0.031%
33	12.481	1609	1614	1619	rVB2	20445	29120	0.53%	0.057%
34	12.563	1625	1628	1631	rBV4	4418	5766	0.10%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
 Data File : BM017044.D
 Acq On : 05 Oct 2018 20:27
 Operator : MJ/SJ
 Sample : J5298-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E62W2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

35	12.681	1642	1648	1653	rBV4	42654	72728	1.32%	0.141%
36	12.734	1653	1657	1664	rVB3	29438	52426	0.95%	0.102%
37	12.834	1669	1674	1681	rVB8	5129	12414	0.23%	0.024%
38	12.928	1685	1690	1691	rBV3	5901	7613	0.14%	0.015%
39	13.204	1732	1737	1740	rBV5	4512	6548	0.12%	0.013%
40	13.234	1740	1742	1746	rVV3	6237	8352	0.15%	0.016%
41	13.275	1746	1749	1751	rVV	11260	13085	0.24%	0.025%
42	13.304	1751	1754	1760	rVB4	9916	14239	0.26%	0.028%
43	13.575	1796	1800	1802	rBV5	12068	16475	0.30%	0.032%
44	13.598	1802	1804	1808	rVB3	7059	7838	0.14%	0.015%
45	13.686	1813	1819	1822	rBV4	26089	44741	0.81%	0.087%
46	13.751	1822	1830	1835	rVV	2090804	2803682	51.04%	5.444%
47	13.798	1835	1838	1842	rVV	134627	180178	3.28%	0.350%
48	13.839	1842	1845	1854	rVB3	48645	95605	1.74%	0.186%
49	14.028	1869	1877	1886	rBV	2449572	3534946	64.35%	6.864%
50	14.086	1886	1887	1895	rVB5	4405	5518	0.10%	0.011%
51	14.157	1895	1899	1902	rBV4	7883	12127	0.22%	0.024%
52	14.333	1923	1929	1940	rBV2	1530315	2403317	43.75%	4.666%
53	14.422	1940	1944	1953	rVB5	18652	38212	0.70%	0.074%
54	14.539	1955	1964	1970	rBV	137031	230717	4.20%	0.448%
55	14.639	1977	1981	1982	rBV3	7843	9660	0.18%	0.019%
56	15.139	2060	2066	2071	rBV5	6135	14083	0.26%	0.027%
57	15.227	2078	2081	2084	rBV4	5486	7218	0.13%	0.014%
58	15.333	2092	2099	2105	rVB	3149642	4368675	79.53%	8.482%
59	15.451	2113	2119	2126	rBV	657947	912111	16.60%	1.771%
60	15.510	2126	2129	2133	rVV5	11751	21863	0.40%	0.042%
61	15.569	2133	2139	2149	rVB3	37232	79712	1.45%	0.155%
62	15.763	2167	2172	2174	rBV4	4765	8575	0.16%	0.017%
63	15.863	2185	2189	2191	rBV4	5082	6689	0.12%	0.013%
64	15.969	2203	2207	2212	rBV6	6780	13270	0.24%	0.026%
65	16.016	2212	2215	2218	rVV4	6882	8573	0.16%	0.017%
66	16.086	2225	2227	2230	rVB4	5493	5954	0.11%	0.012%
67	16.163	2236	2240	2245	rBV6	8191	14340	0.26%	0.028%
68	16.210	2245	2248	2249	rBV3	5381	5624	0.10%	0.011%
69	16.286	2259	2261	2264	rVB4	5672	6006	0.11%	0.012%
70	16.327	2264	2268	2271	rBV6	4985	6884	0.13%	0.013%
71	16.386	2274	2278	2281	rBV6	13473	22571	0.41%	0.044%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
 Data File : BM017044.D
 Acq On : 05 Oct 2018 20:27
 Operator : MJ/SJ
 Sample : J5298-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E62W2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

72	16.486	2291	2295	2298	rBV5	3582	5713	0.10%	0.011%
73	16.539	2300	2304	2305	rVV3	6058	6989	0.13%	0.014%
74	16.645	2319	2322	2325	rBV5	7386	11448	0.21%	0.022%
75	16.757	2338	2341	2349	rVB6	8030	16442	0.30%	0.032%
76	16.816	2349	2351	2355	rBV5	6008	7945	0.14%	0.015%
77	16.869	2355	2360	2365	rVB3	11575	19712	0.36%	0.038%
78	16.969	2372	2377	2379	rBV6	6998	7441	0.14%	0.014%
79	17.086	2390	2397	2403	rBV2	1888732	2750205	50.07%	5.340%
80	17.180	2407	2413	2424	rVV2	3202620	4579176	83.36%	8.891%
81	17.280	2428	2430	2433	rVB4	7417	7067	0.13%	0.014%
82	17.463	2457	2461	2465	rBV5	9422	15687	0.29%	0.030%
83	17.986	2545	2550	2555	rBV2	103736	148144	2.70%	0.288%
84	18.286	2597	2601	2605	rBV7	5173	7690	0.14%	0.015%
85	18.839	2693	2695	2700	rVB5	6091	7049	0.13%	0.014%
86	19.033	2726	2728	2731	rBV3	6043	5543	0.10%	0.011%
87	19.110	2737	2741	2745	rVV	38880	54150	0.99%	0.105%
88	19.268	2764	2768	2775	rBV4	44061	68503	1.25%	0.133%
89	19.363	2781	2784	2790	rVB	27792	38237	0.70%	0.074%
90	19.480	2798	2804	2810	rBV	3925149	5114820	93.11%	9.931%
91	19.715	2842	2844	2848	rVB5	10134	8285	0.15%	0.016%
92	20.998	3058	3062	3069	rBV4	79074	130708	2.38%	0.254%
93	21.268	3103	3108	3116	rBV	2366508	3184179	57.97%	6.183%
94	23.356	3456	3463	3475	rVB	2865487	5493124	100.00%	10.666%
95	23.498	3480	3487	3500	rVB	1633455	3209420	58.43%	6.232%


Sum of corrected areas: 51503041

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
Data File : BM017044.D
Acq On : 05 Oct 2018 20:27
Operator : MJ/SJ
Sample : J5298-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E62W2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

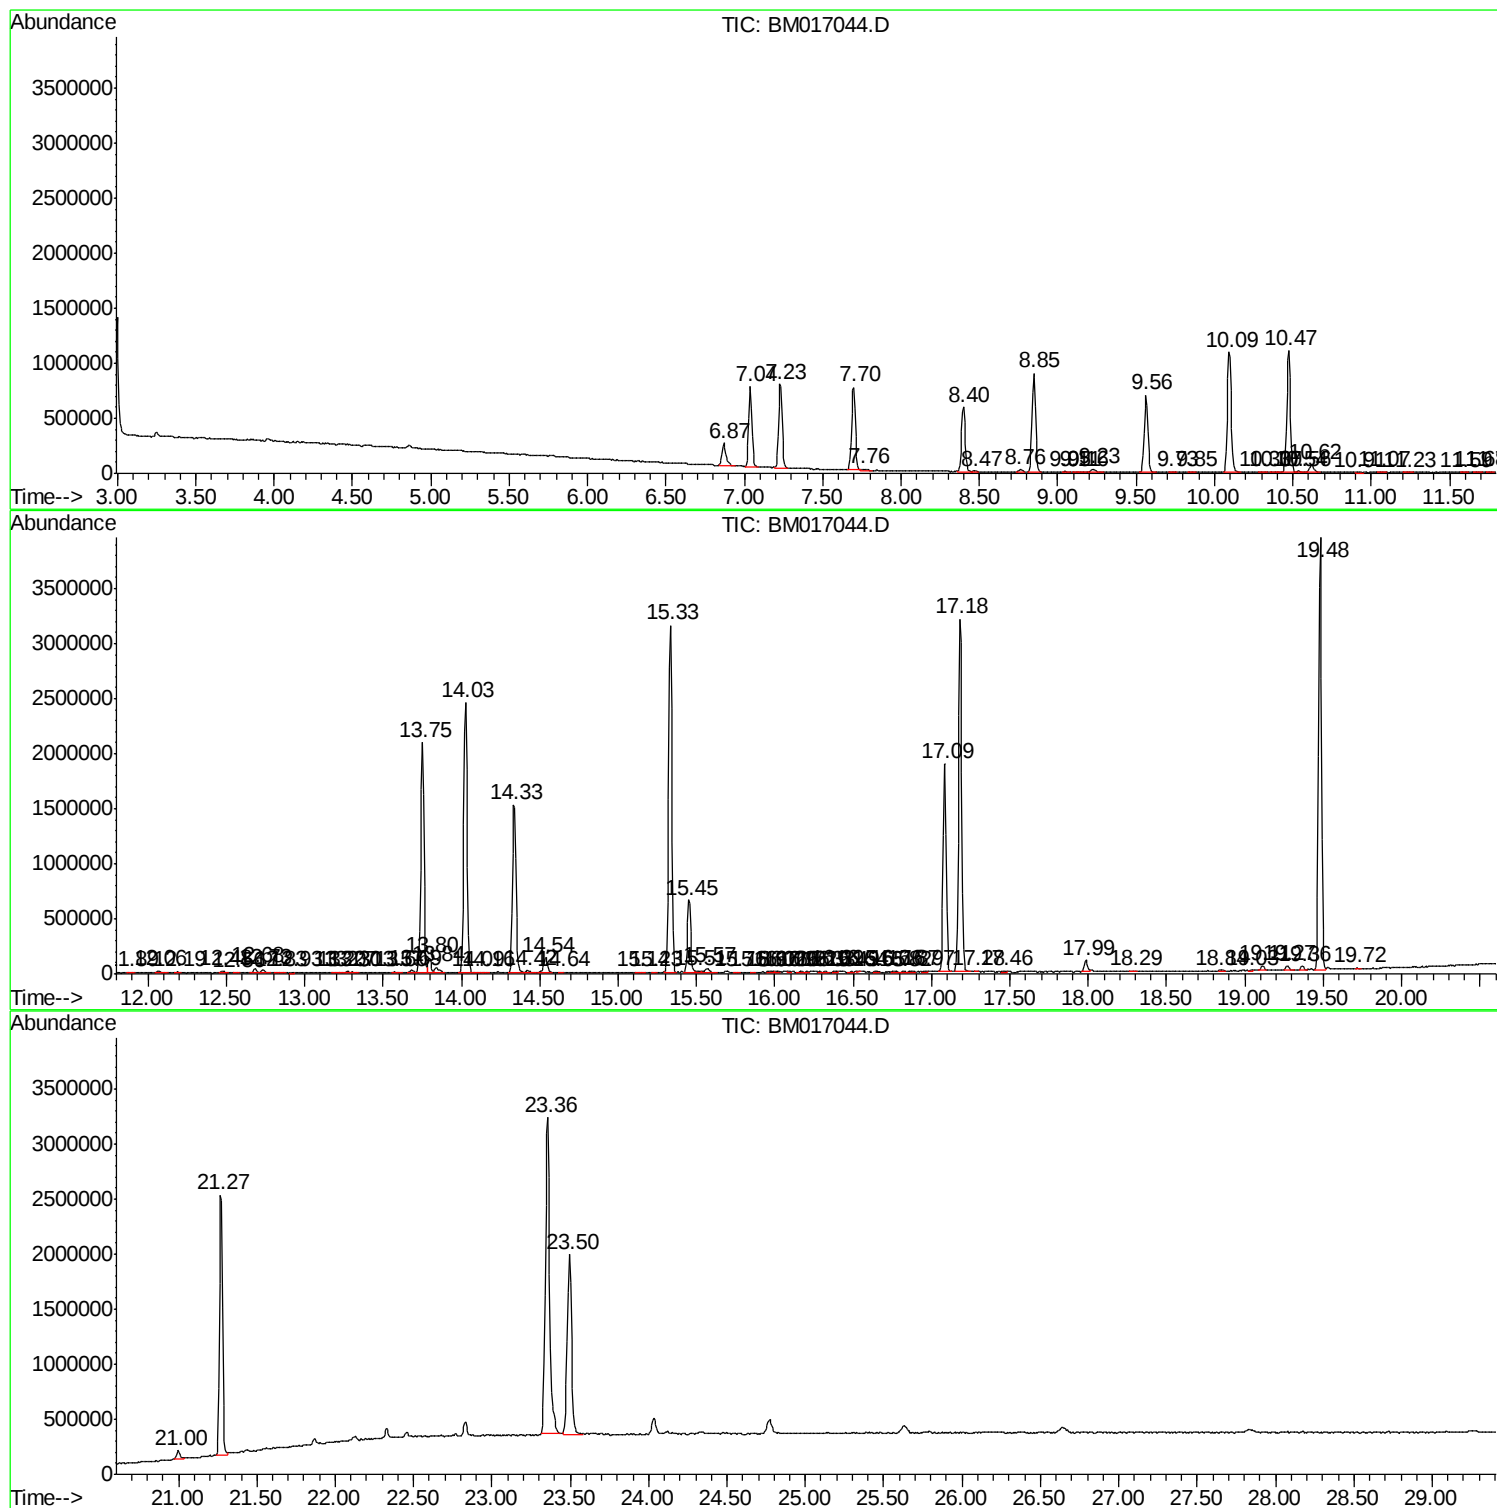

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
Data File : BM017044.D
Acq On : 05 Oct 2018 20:27
Operator : MJ/SJ
Sample : J5298-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E62W2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100518\
Data File : BM017044.D
Acq On : 05 Oct 2018 20:27
Operator : MJ/SJ
Sample : J5298-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E62W2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
