

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100719\
 Data File : BM023033.D
 Acq On : 07 Oct 2019 15:43
 Operator : JU
 Sample : K5056-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAD8

Quant Time: Oct 07 16:57:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 07 01:10:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	145820	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	593704	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.42	164	350349	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.16	188	704173	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	713350	20.00	ng/ul	0.00
86) Perylene-d12	23.60	264	839010	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	30986	9.19	ng/uL	0.00
5) Phenol-d5	6.95	99	606886	47.11	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.11	67	354557	50.28	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.31	132	506040	48.77	ng/ul	-0.01
13) 4-Methylphenol-d8	8.48	113	496396	47.06	ng/ul	-0.02
19) Nitrobenzene-d5	8.93	128	246878	53.88	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.65	143	270378	54.04	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.19	165	502874	50.48	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.70	131	691577	57.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.83	166	1487177	54.69	ng/ul	0.00
47) Acenaphthylene-d8	14.11	160	1761208	56.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.61	143	144838	26.96	ng/ul	-0.01
58) Fluorene-d10	15.41	176	1267307	54.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	93950	20.50	ng/ul	-0.01
71) Anthracene-d10	17.26	188	1893569	55.07	ng/ul	0.00
79) Pyrene-d10	19.55	212	2157213	56.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.46	264	2475000	57.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.87	163	264663	9.475	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100719\
Data File : BM023033.D
Acq On : 07 Oct 2019 15:43
Operator : JU
Sample : K5056-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAD8

Quant Time: Oct 07 16:57:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 07 01:10:23 2019
Response via : Initial Calibration

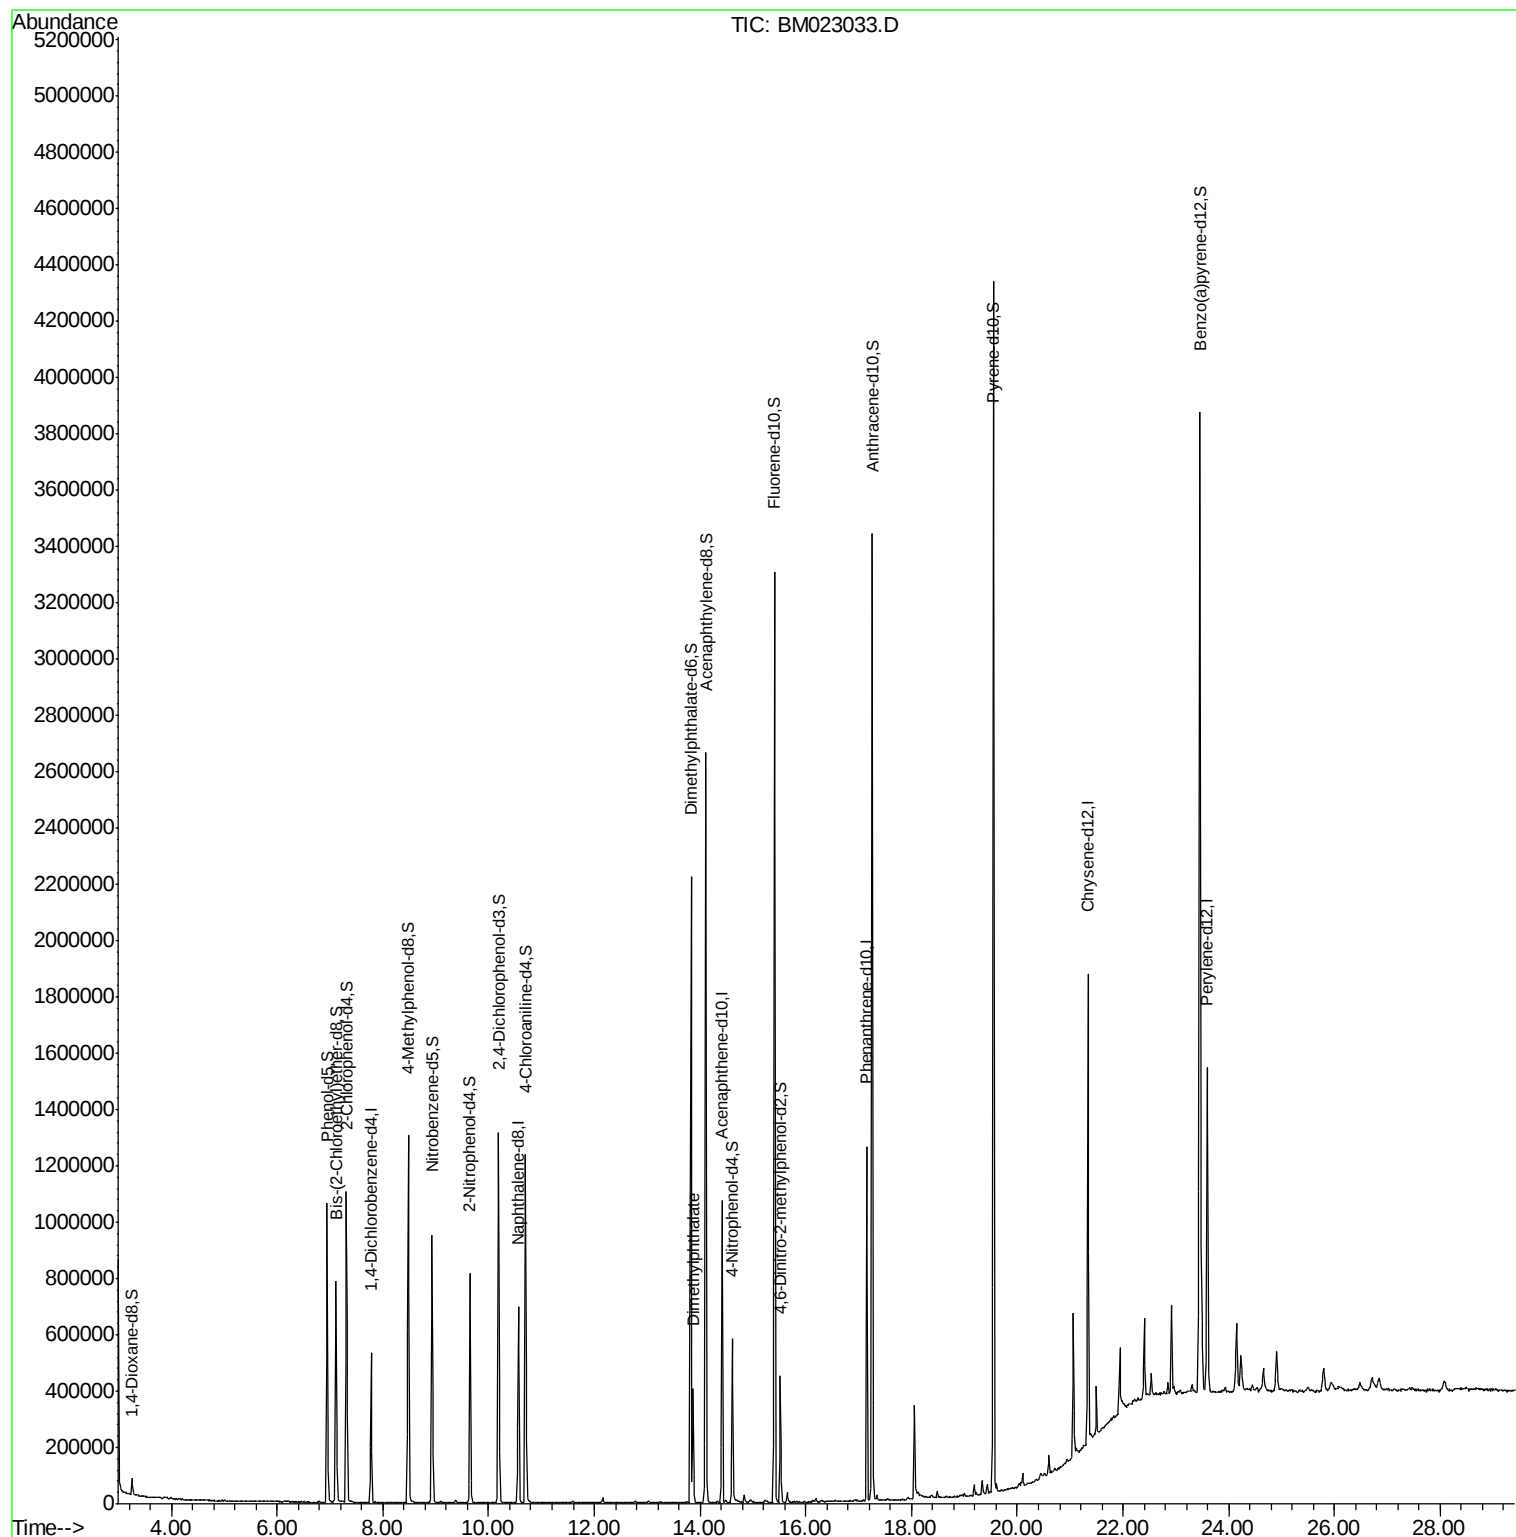

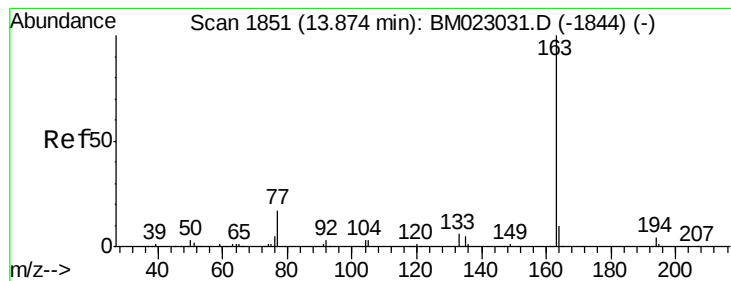

#45
 Dimethylphthalate
 Concen: 9.475 ng/ul
 RT: 13.87 min Scan# 1851
 Delta R.T. -0.01 min
 Lab File: BM023033.D
 Acq: 07 Oct 2019 15:43

Instrument :
 BNA_M
 ClientSampleId :
 DBAD8

Tgt Ion:	163	Resp:	264663
Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.0
164	10.1	8.1	12.1

