

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100818\
 Data File : BM017073.D
 Acq On : 08 Oct 2018 19:27
 Operator : MJ/SJ
 Sample : J5234-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AL6

Quant Time: Oct 09 04:14:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 09 04:00:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	201171	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	885621	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	480544	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1035743	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1087141	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	1135974	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	21236	5.25	ng/uL	0.00
5) Phenol-d5	6.87	99	105953	6.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	278439	27.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	321754	23.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	191896	14.56	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	181640	28.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	173361	26.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	349621	25.80	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.75	166	1082184	28.38	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	1369801	28.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	15901	2.21	ng/ul	0.00
58) Fluorene-d10	15.33	176	987887	29.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	86594	14.18	ng/ul	0.00
71) Anthracene-d10	17.18	188	1421543	28.74	ng/ul	0.00
79) Pyrene-d10	19.47	212	1539703	31.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	1693750	29.12	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.79	163	327616	8.678	ng/ul 99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100818\
Data File : BM017073.D
Acq On : 08 Oct 2018 19:27
Operator : MJ/SJ
Sample : J5234-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AL6

Quant Time: Oct 09 04:14:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 09 04:00:09 2018
Response via : Initial Calibration

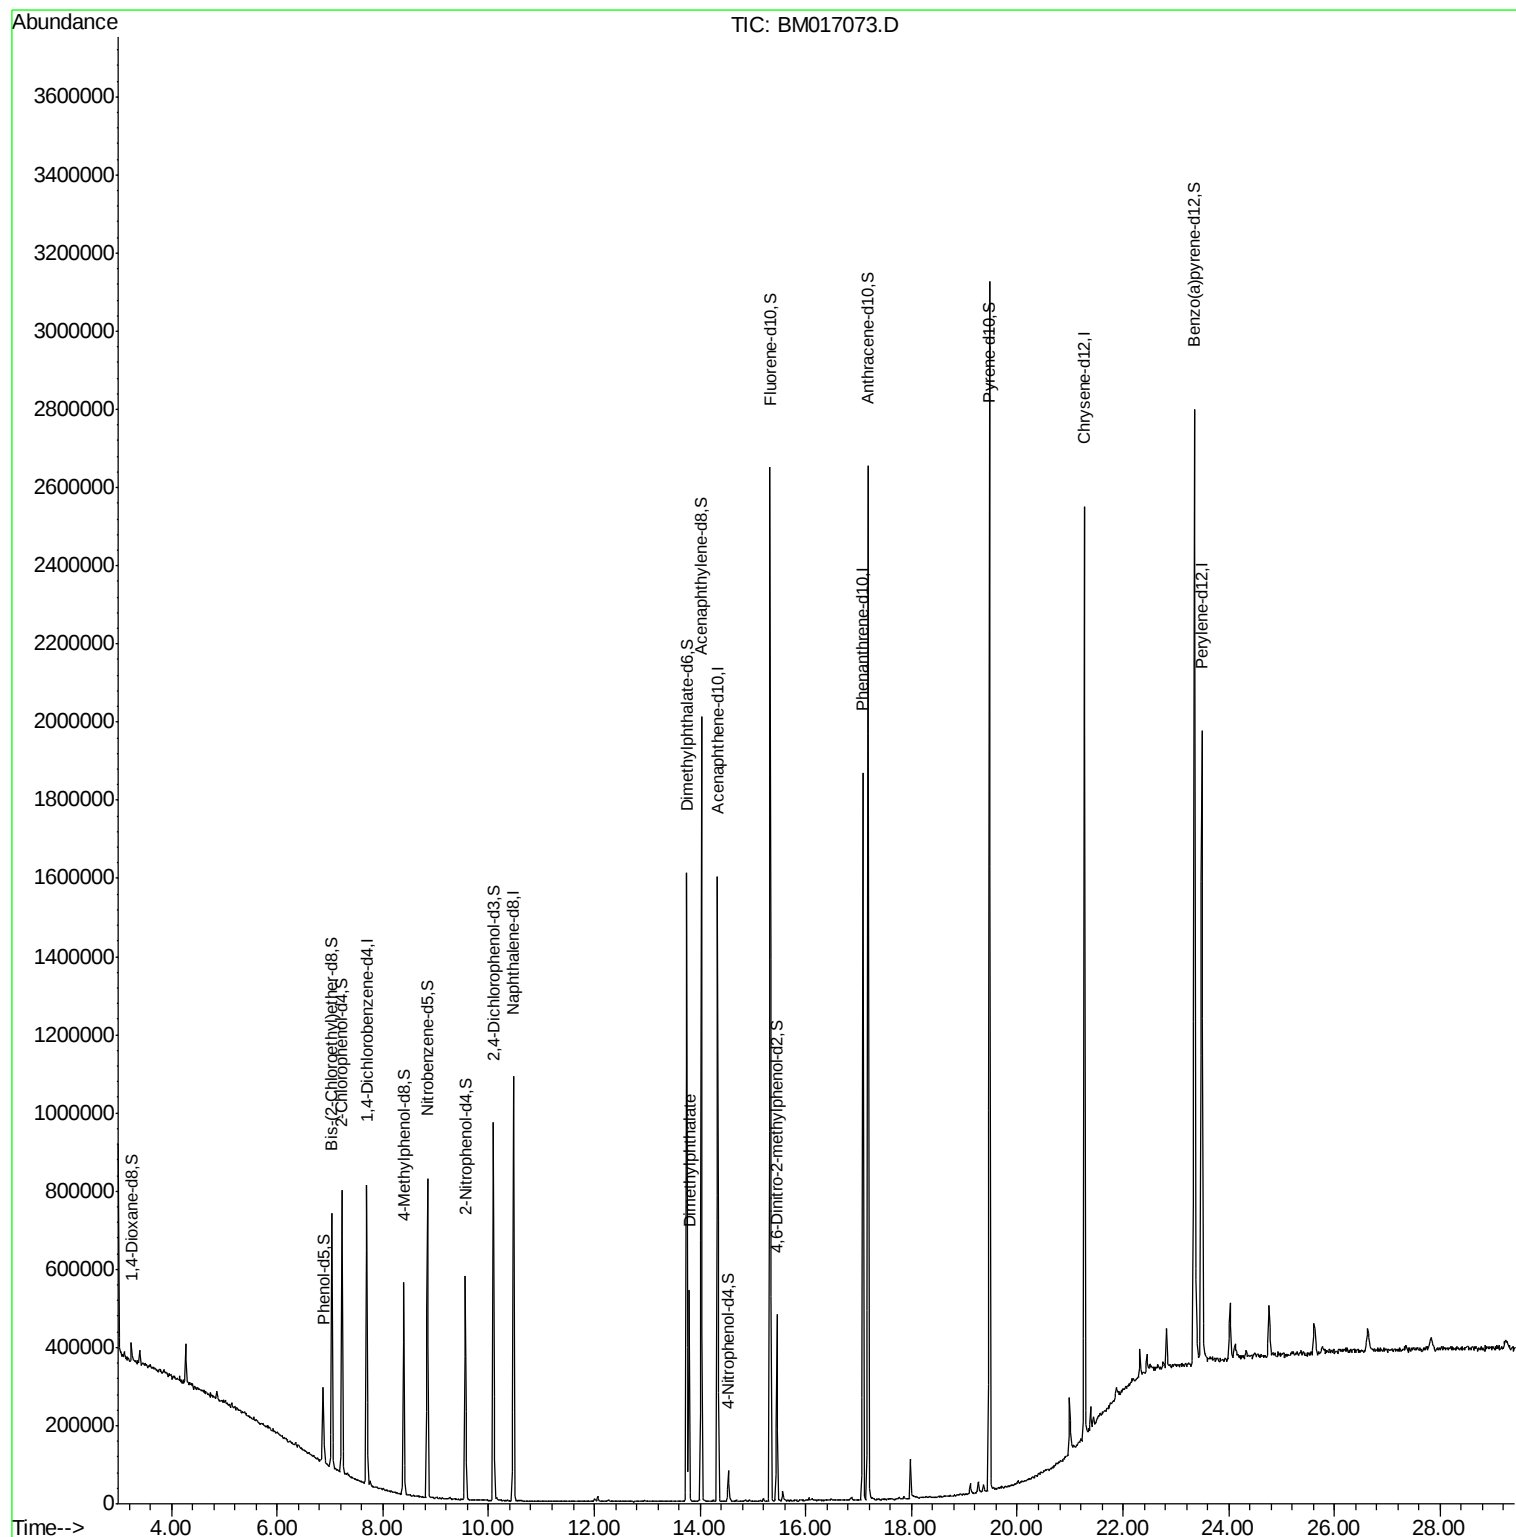

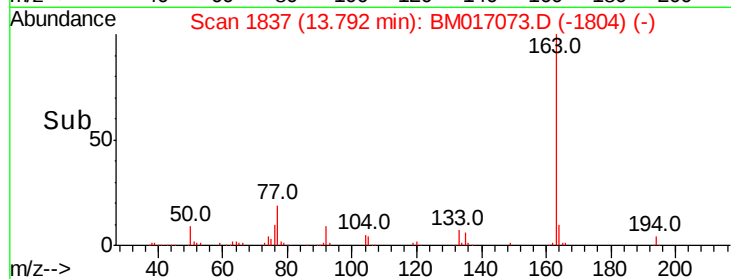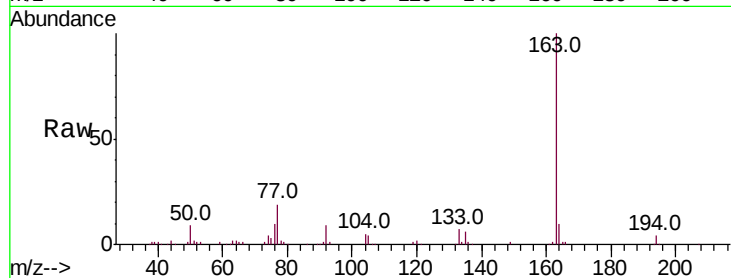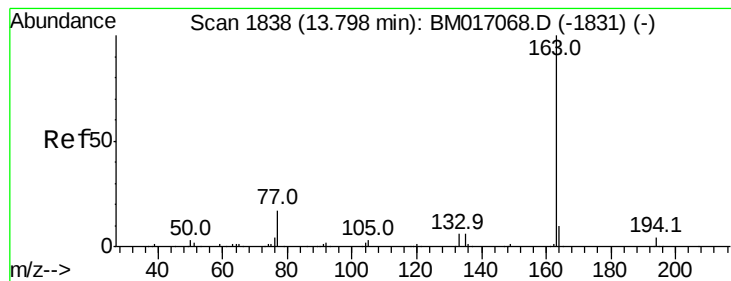

#45

Dimethylphthalate

Concen: 8.678 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BM017073.D

Acq: 08 Oct 2018 19:27

Instrument :

BNA_M

ClientSampleId :

C0AL6

Tot Ion:163 Resp: 327616

Ion Ratio Lower Upper

163 100

194 3.7 3.3 4.9

164 10.2 8.0 12.0

