

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100818\
 Data File : BM017075.D
 Acq On : 08 Oct 2018 20:40
 Operator : MJ/SJ
 Sample : J5234-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK7

Quant Time: Oct 09 04:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 09 04:00:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	185909	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	819844	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	448220	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1038895	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1159424	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	1239827	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	19985	5.34	ng/uL	0.00
5) Phenol-d5	6.86	99	97448	6.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	241557	25.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	279639	21.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	177156	14.55	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	159532	26.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	147972	24.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	314158	25.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	5969	0.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.75	166	1055405	29.68	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	1354993	29.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	17091	2.54	ng/ul	0.00
58) Fluorene-d10	15.33	176	969794	30.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	88683	14.47	ng/ul	0.00
71) Anthracene-d10	17.18	188	1481632	29.86	ng/ul	0.00
79) Pyrene-d10	19.47	212	1701388	32.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	1941873	30.59	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.89	94	22912	1.474	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100818\
Data File : BM017075.D
Acq On : 08 Oct 2018 20:40
Operator : MJ/SJ
Sample : J5234-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK7

Quant Time: Oct 09 04:18:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 09 04:00:09 2018
Response via : Initial Calibration

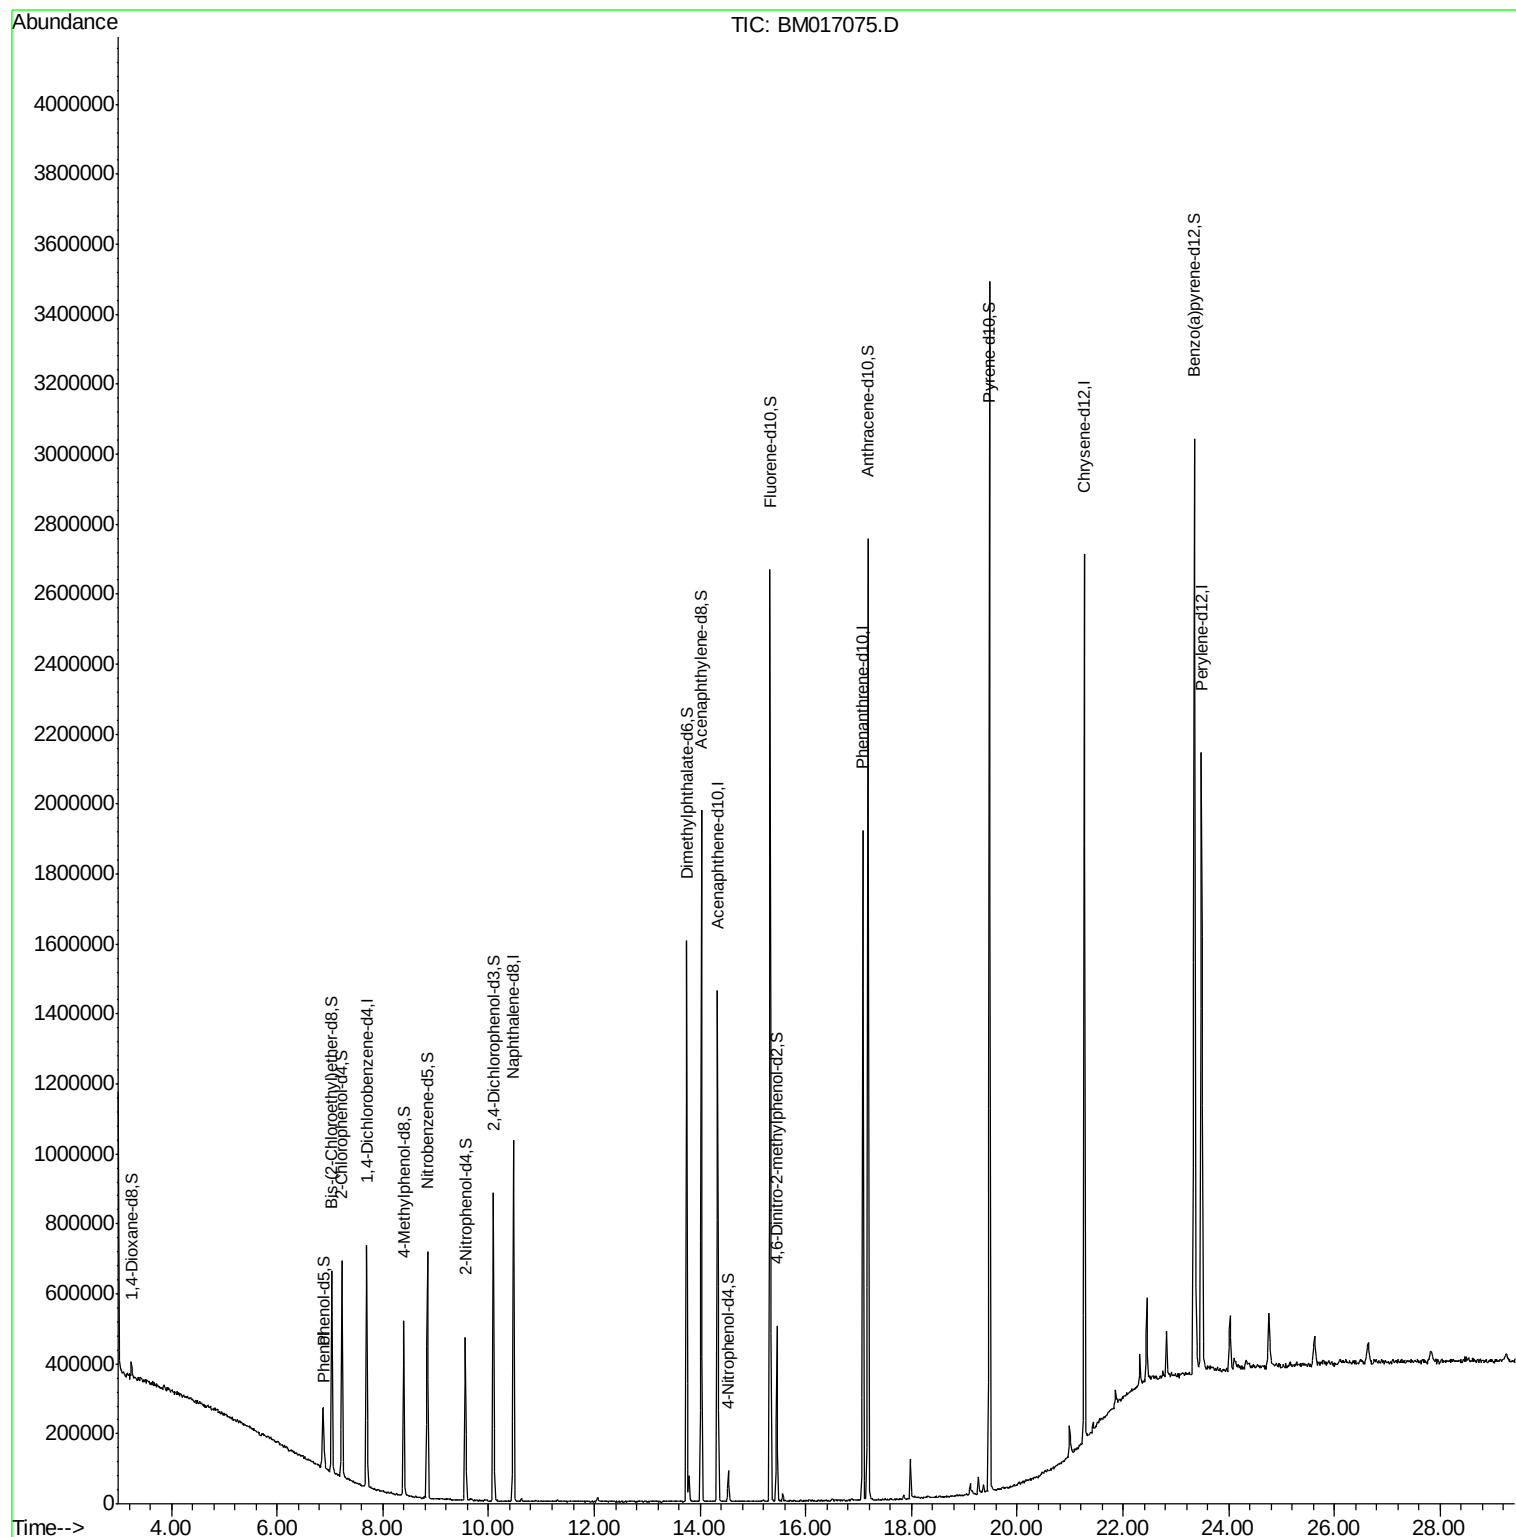

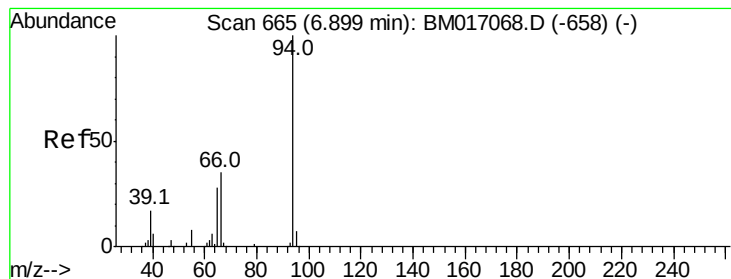

#6

Phenol

Concen: 1.474 ng/ul
 RT: 6.89 min Scan# 664
 Delta R.T. -0.01 min
 Lab File: BM017075.D
 Acq: 08 Oct 2018 20:40

Instrument :
 BNA_M
 ClientSampleId :
 C0AK7

Tot Ion: 94 Resp: 22912
 Ion Ratio Lower Upper
 94 100
 65 25.6 22.8 34.2
 66 37.7 29.5 44.3

