

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100818\
 Data File : BM017078.D
 Acq On : 08 Oct 2018 22:28
 Operator : MJ/SJ
 Sample : J5234-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ7

Quant Time: Oct 09 04:02:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 09 04:00:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	180116	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	787127	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	431356	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	966855	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1060043	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	1152401	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	21818	6.02	ng/uL	0.00
5) Phenol-d5	6.87	99	111805	7.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	283848	31.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	325964	26.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	203433	17.24	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	185569	32.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	170296	29.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	353447	29.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	18111	1.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.75	166	1125908	32.90	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	1495935	34.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	17974	2.78	ng/ul	0.00
58) Fluorene-d10	15.33	176	1040190	34.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	94485	16.57	ng/ul	0.00
71) Anthracene-d10	17.18	188	1569467	33.99	ng/ul	0.00
79) Pyrene-d10	19.47	212	1725702	36.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	2018189	34.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.79	163	77608	2.290	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100818\
Data File : BM017078.D
Acq On : 08 Oct 2018 22:28
Operator : MJ/SJ
Sample : J5234-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ7

Quant Time: Oct 09 04:02:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 09 04:00:09 2018
Response via : Initial Calibration

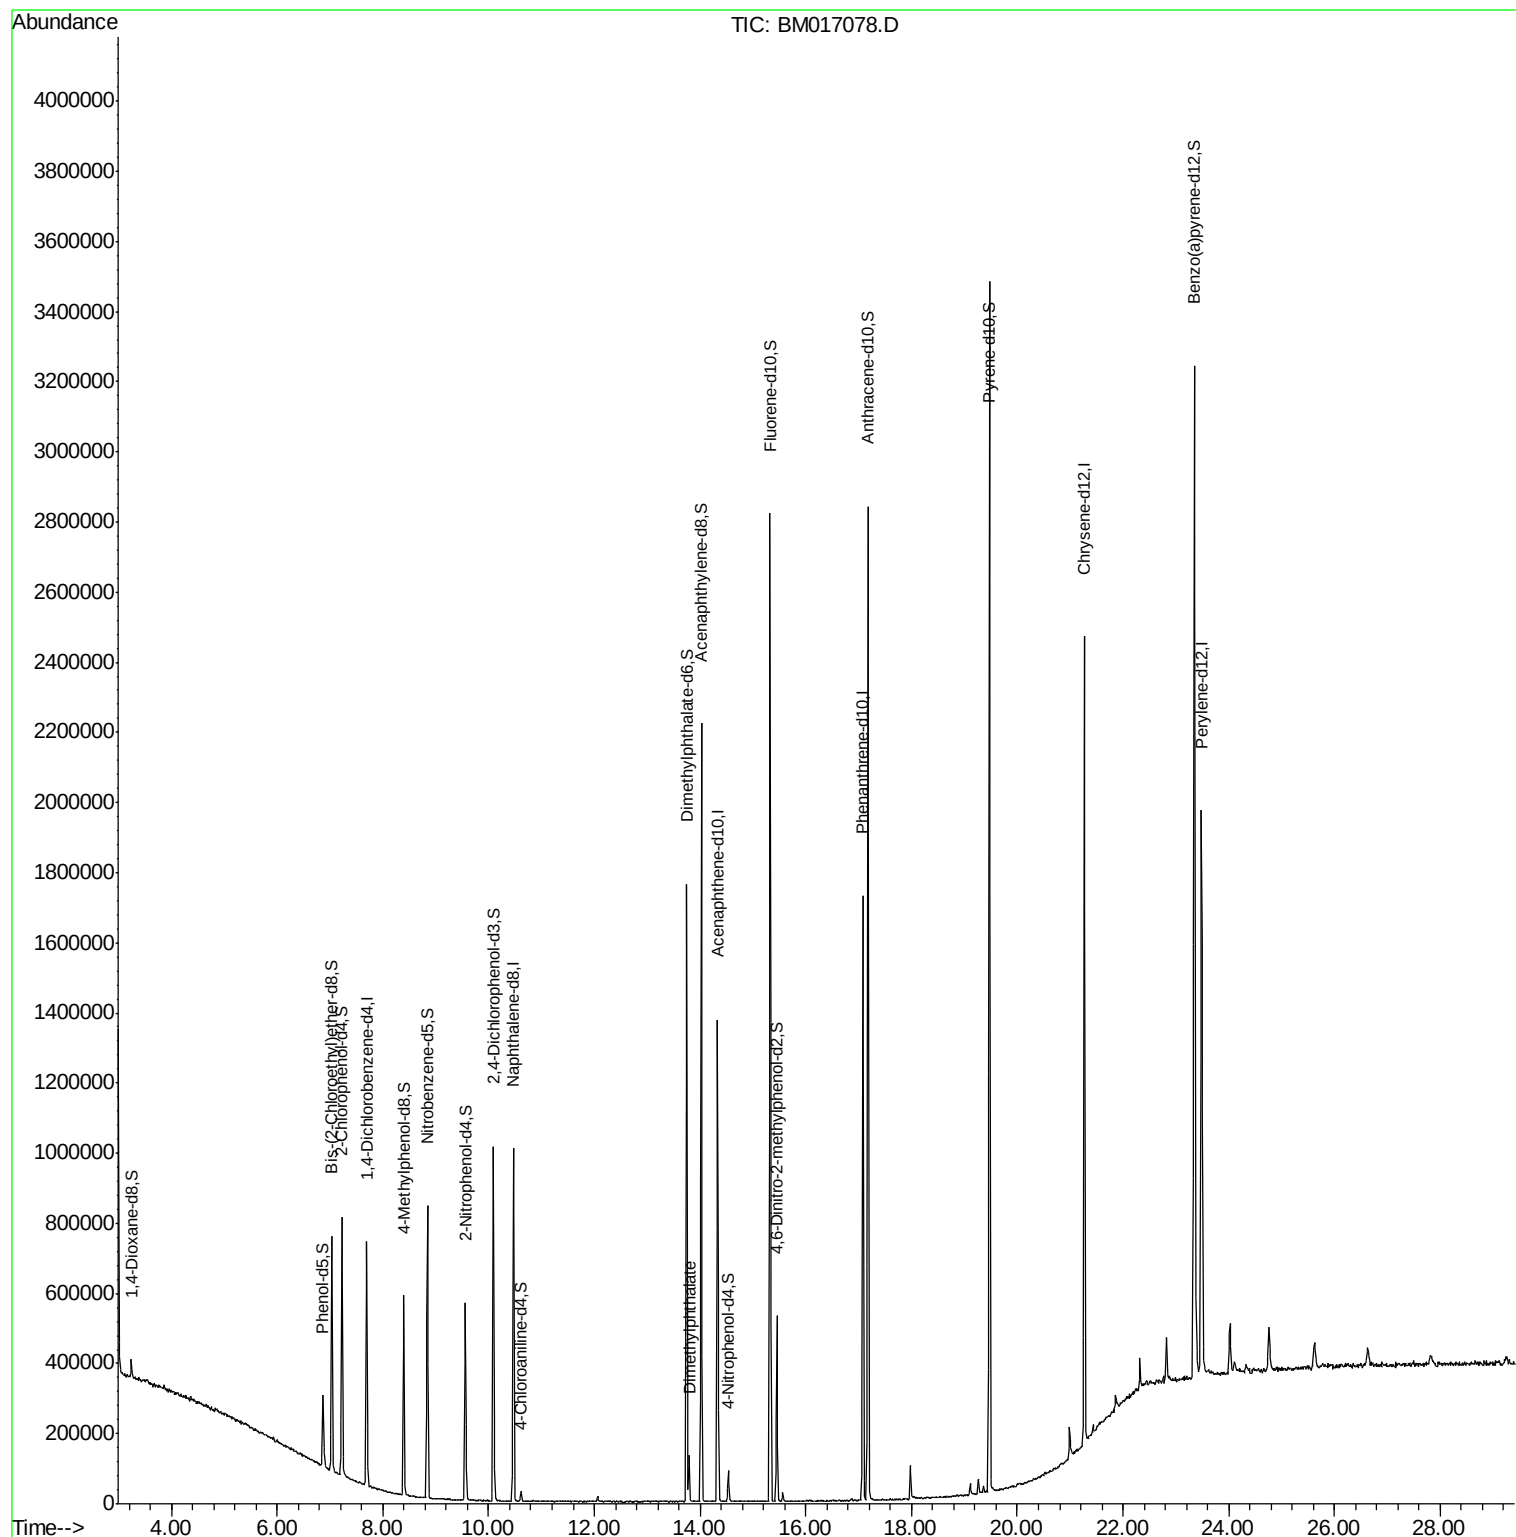

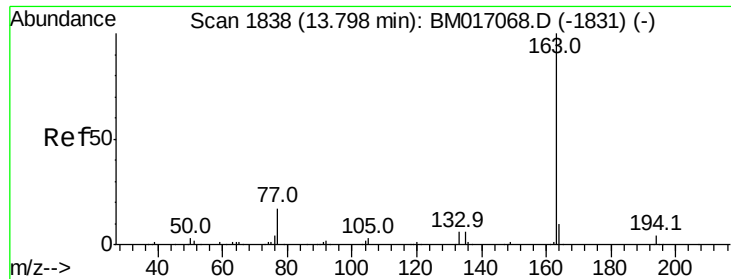

#45

Dimethylphthalate

Concen: 2.290 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BM017078.D

Acq: 08 Oct 2018 22:28

Instrument :

BNA_M

ClientSampleId :

C0AJ7


Tot Ion:163 Resp: 77608

Ion Ratio Lower Upper

163 100

194 4.5 3.3 4.9

164 10.2 8.0 12.0

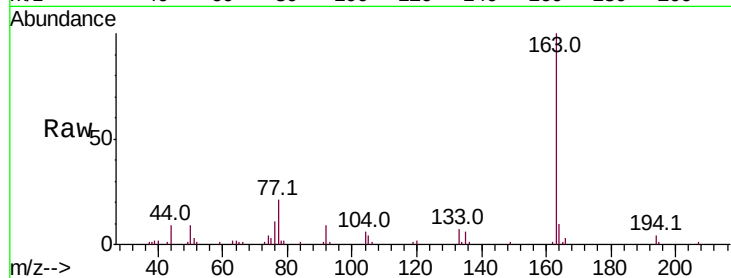

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

