

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100819\
 Data File : BM023039.D
 Acq On : 08 Oct 2019 11:23
 Operator : JU
 Sample : K5056-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAE2

Quant Time: Oct 08 15:08:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 15:02:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	170551	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	690704	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	412525	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.15	188	840289	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	878751	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	1033994	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	19663	4.99	ng/uL	0.00
5) Phenol-d5	6.95	99	348948	23.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	206625	25.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.31	132	295959	24.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	276274	22.39	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	137308	25.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	145281	24.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	276649	23.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	383236	27.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	799818	24.98	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	964430	26.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	96509	15.26	ng/ul	0.00
58) Fluorene-d10	15.40	176	704563	25.82	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	74209	13.57	ng/ul	0.00
71) Anthracene-d10	17.25	188	1078819	26.29	ng/ul	0.00
79) Pyrene-d10	19.54	212	1234902	26.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	1410116	26.36	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.87	163	166680	5.068	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100819\
Data File : BM023039.D
Acq On : 08 Oct 2019 11:23
Operator : JU
Sample : K5056-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAE2

Quant Time: Oct 08 15:08:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 08 15:02:34 2019
Response via : Initial Calibration

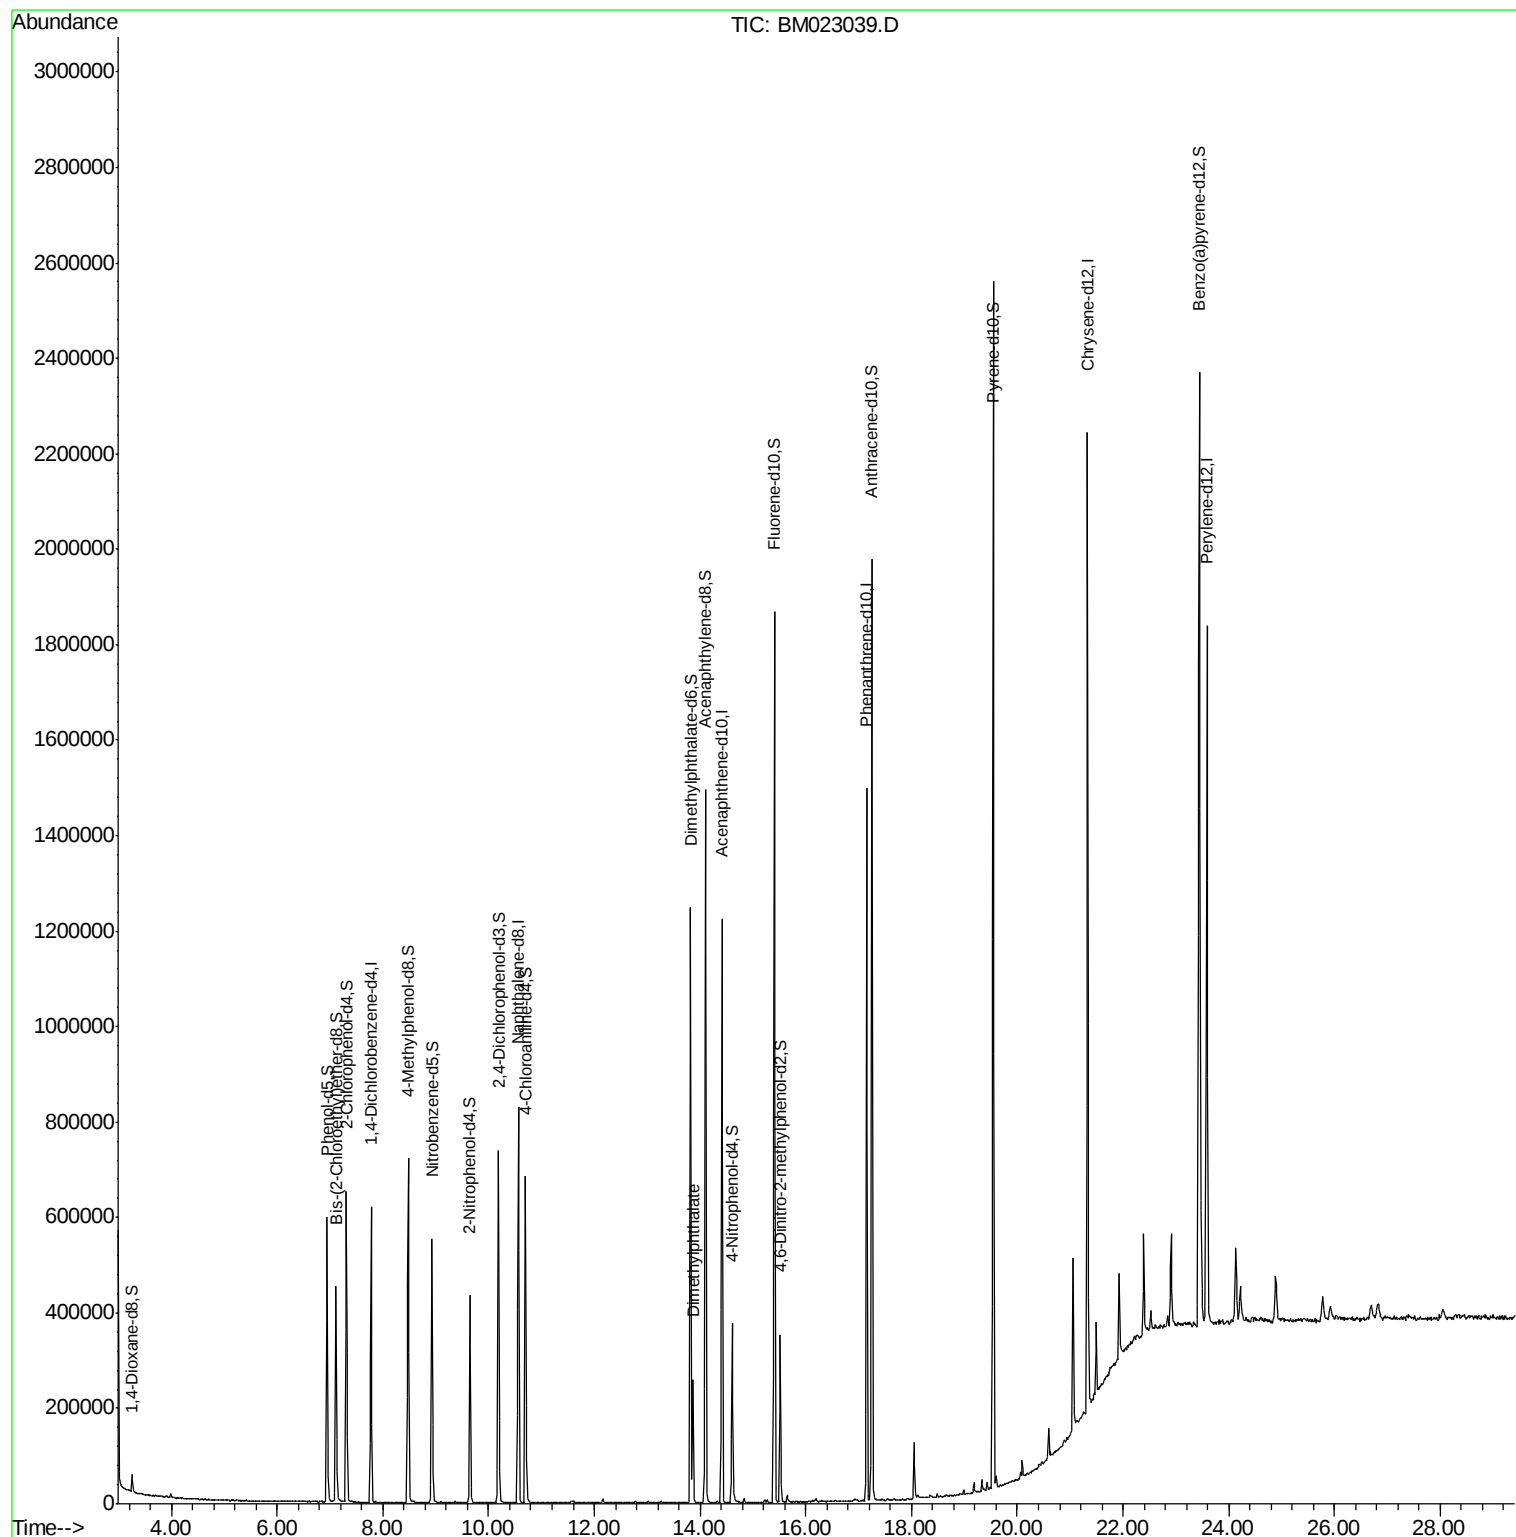

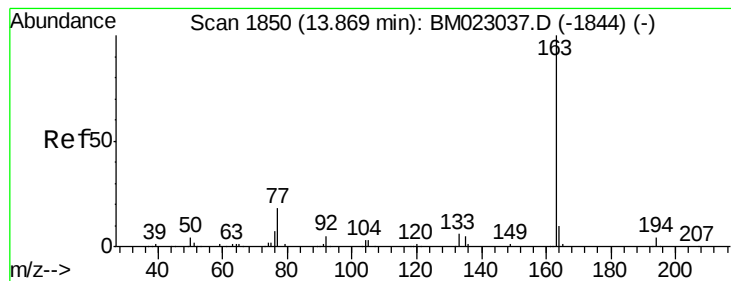

#45
 Dimethylphthalate
 Concen: 5.068 ng/ul
 RT: 13.87 min Scan# 1850
 Delta R.T. -0.00 min
 Lab File: BM023039.D
 Acq: 08 Oct 2019 11:23

Instrument :
 BNA_M
 ClientSampleId :
 DBAE2

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.9	8.1	12.1

