

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100819\
 Data File : BM023101.D
 Acq On : 10 Oct 2019 02:55
 Operator : JU
 Sample : K5177-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP95

Manual Integrations
 APPROVED

mohammad
 10/11/2019 8:28:40 AM

Quant Time: Oct 10 04:11:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 15:02:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	176988	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	722964	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.40	164	398835	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.14	188	750411	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	704512	20.00	ng/ul	0.00
86) Perylene-d12	23.58	264	841149	20.00	ng/ul	0.00


System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	17321	4.23	ng/uL	0.00
5) Phenol-d5	6.93	99	343171	21.95	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.10	67	203453	23.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	298256	23.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	261678	20.44	ng/ul	-0.01
19) Nitrobenzene-d5	8.92	128	142447	25.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	152225	24.99	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.18	165	284043	23.41	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	227867	15.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	805385	26.02	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	963186	26.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	91087	14.89	ng/ul	-0.01
58) Fluorene-d10	15.40	176	686374	26.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	75188	15.40	ng/ul	0.00
71) Anthracene-d10	17.24	188	983553	26.84	ng/ul	0.00
79) Pyrene-d10	19.54	212	1068893	28.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	1204668	27.68	ng/ul	-0.01

Target Compounds

					Ovalue
6) Phenol	6.96	94	48627	2.966	ng/ul 100
45) Dimethylphthalate	13.86	163	272467	8.569	ng/ul 99
48) Acenaphthylene	14.13	152	58015	1.504	ng/ul 99
50) Acenaphthene	14.47	153	35047	1.304	ng/ul 95
59) Fluorene	15.45	166	41356	1.333	ng/ul 98
70) Phenanthrene	17.19	178	758401	16.934	ng/ul 100
72) Anthracene	17.27	178	184294	4.039	ng/ul 100
75) Carbazole	17.54	167	70024	1.727	ng/ul 99
77) Fluoranthene	19.20	202	1578939	31.347	ng/ul 99
80) Pyrene	19.57	202	1704706	34.134	ng/ul 99
83) Benzo(a)anthracene	21.31	228	1002734	19.824	ng/ul 98
84) Bis(2-ethylhexyl)phthalate	21.24	149	699636	23.974	ng/ul 99
85) Chrysene	21.36	228	1032194	22.134	ng/ul 98
88) Benzo(b)fluoranthene	22.90	252	1317057	23.594	ng/ul# 96
89) Benzo(k)fluoranthene	22.94	252	370187m	6.932	ng/ul
91) Benzo(a)pyrene	23.48	252	1014460	19.371	ng/ul# 96
92) Indeno(1,2,3-cd)pyrene	25.85	276	650386	11.692	ng/ul 96
93) Dibenzo(a,h)anthracene	25.86	278	182509	3.922	ng/ul 92
94) Benzo(g,h,i)perylene	26.54	276	616312	13.733	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#6

Phenol

Concen: 2.966 ng/ul

RT: 6.96 min Scan# 676

Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Instrument :

BNA_M





ClientSampleId :

BEP95

Tot Ion:	94	Resp:	48627
Ion	Ratio	Lower	Upper
94	100		
65	26.3	20.9	31.3
66	33.8	27.2	40.8

Manual Integrations
APPROVED

mohammad
10/11/2019 8:28:40 AM

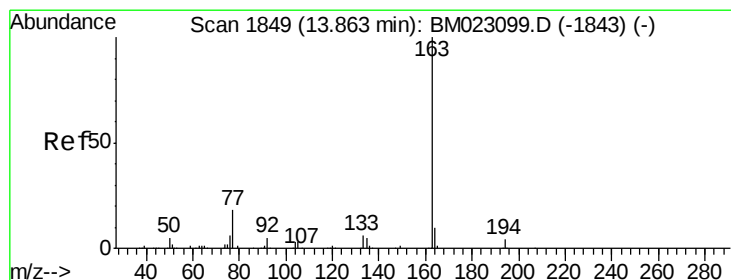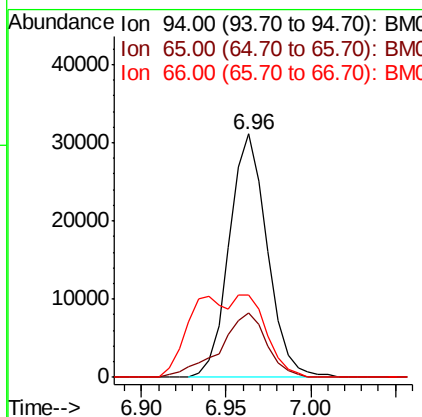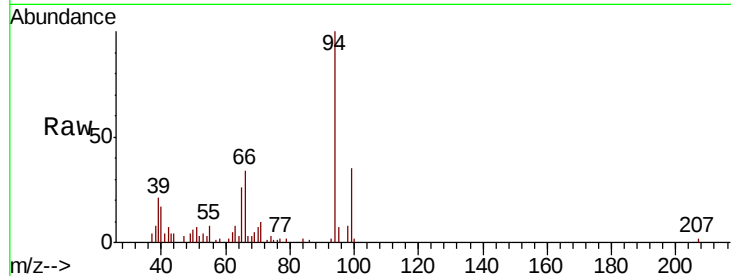

#45

Dimethylphthalate

Concen: 8.569 ng/ul




RT: 13.86 min Scan# 1849


Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Tgt Ion:	163	Resp:	272467
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.9	8.1	12.1

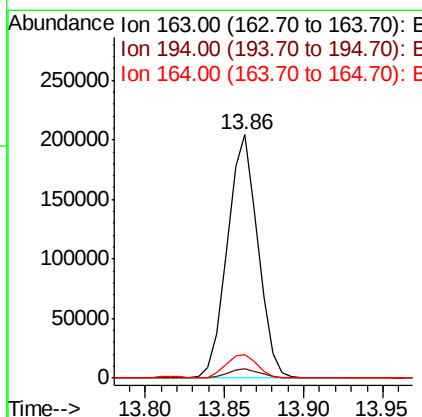







#48
Acenaphthylene
Concen: 1.504 ng/ul
RT: 14.13 min Scan# 1894
Delta R.T. -0.01 min
Lab File: BM023101.D
Acq: 10 Oct 2019 02:55

Instrument :
BNA_M
ClientSampleId :
BEP95

Tot Ion:	152	Resp:	58015
Ion Ratio	Lower	Upper	
152	100		
151	19.4	16.0	24.0
153	13.2	10.6	16.0




Manual Integrations
APPROVED


mohammad
10/11/2019 8:28:40 AM

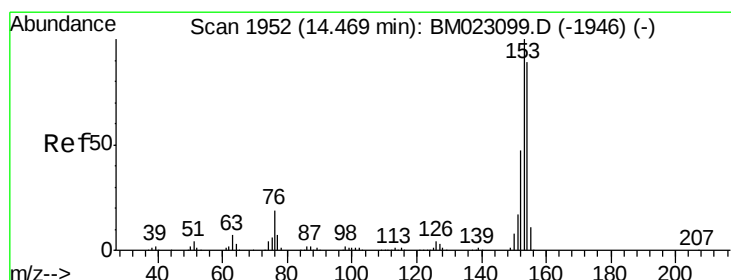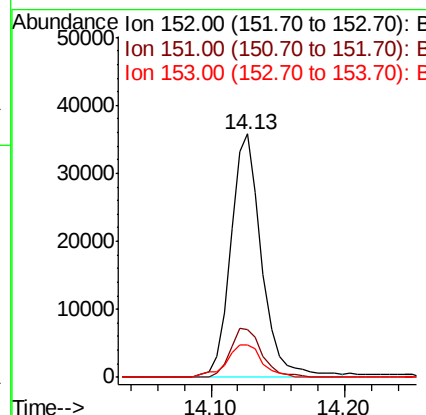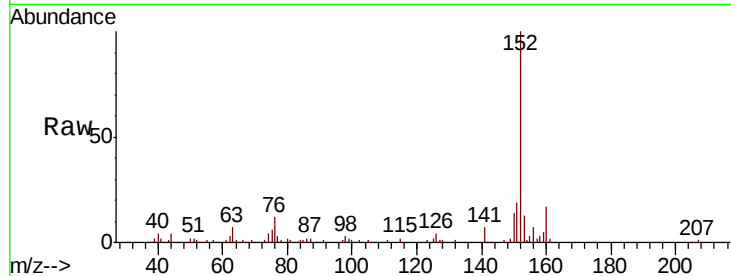

#50
Acenaphthene
Concen: 1.304 ng/ul
RT: 14.47 min Scan# 1952
Delta R.T. -0.01 min
Lab File: BM023101.D
Acq: 10 Oct 2019 02:55

Tgt Ion:	153	Resp:	35047
Ion Ratio	Lower	Upper	
153	100		
152	50.4	38.1	57.1
154	93.6	71.1	106.7

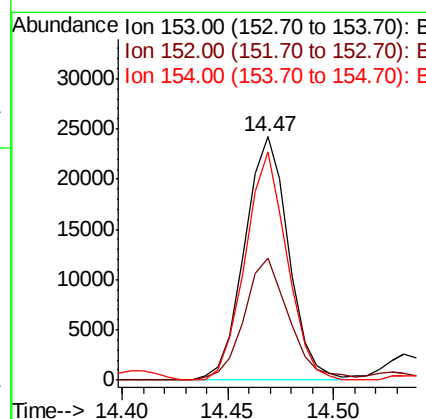



#59

Fluorene

Concen: 1.333 ng/ul

RT: 15.45 min Scan# 2119

Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Instrument :

BNA_M

ClientSampled :

BEP95

Tot Ion:166 Resp: 41356

Ion Ratio Lower Upper


166 100

165 95.8 77.7 116.5




167 14.9 11.0 16.4

Manual Integrations
APPROVED

mohammad
10/11/2019 8:28:40 AM

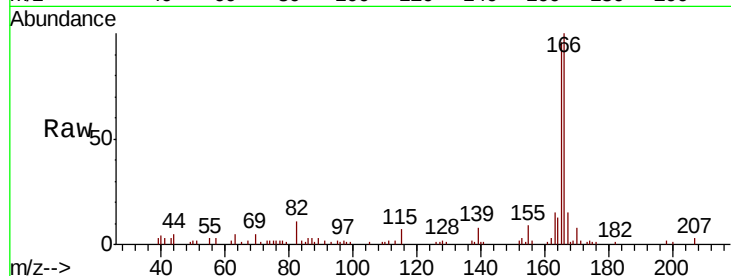

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

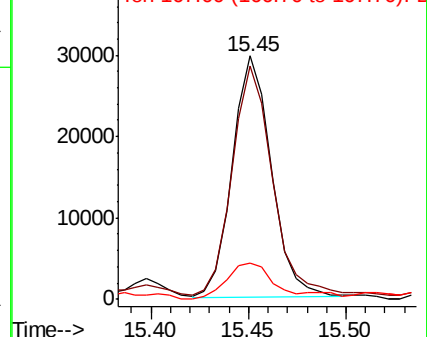

#70

Phenanthrene

Concen: 16.934 ng/ul

RT: 17.19 min Scan# 2414

Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55


Tgt Ion:178 Resp: 758401

Ion Ratio Lower Upper



178 100


179 15.5 12.4 18.6

176 19.4 15.3 22.9



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

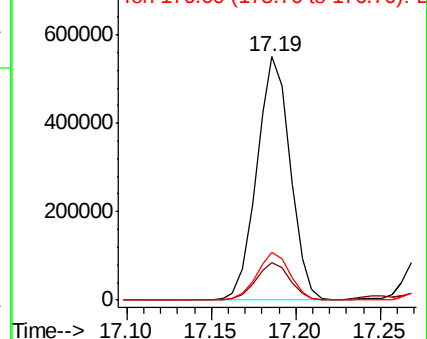

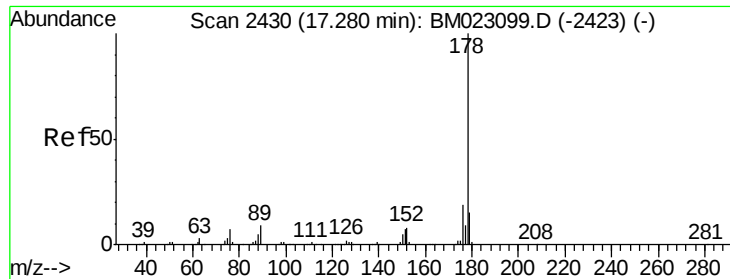

#72

Anthracene

Concen: 4.039 ng/ul

RT: 17.27 min Scan# 2429

Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Instrument :

BNA_M


ClientSampled :

BEP95




Tot Ion:	178	Resp:	184294
Ion Ratio	Lower	Upper	
178	100		
179	15.5	12.4	18.6
176	18.6	15.0	22.6

Manual Integrations
APPROVED

mohammad
10/11/2019 8:28:40 AM

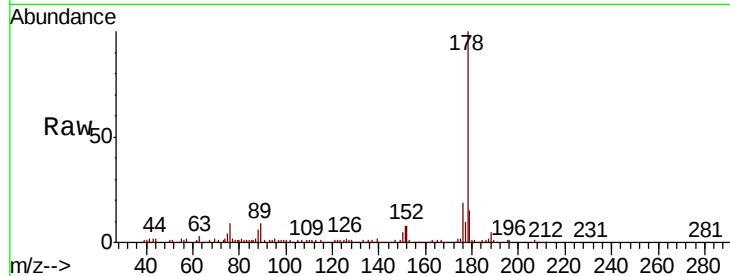

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

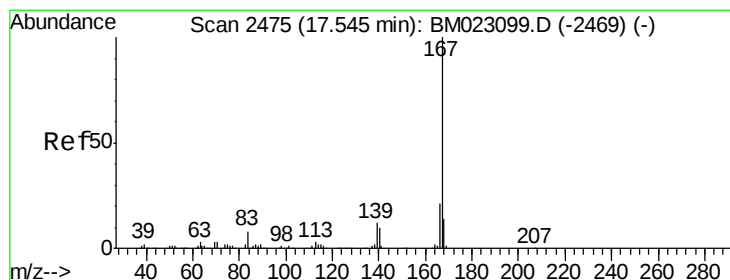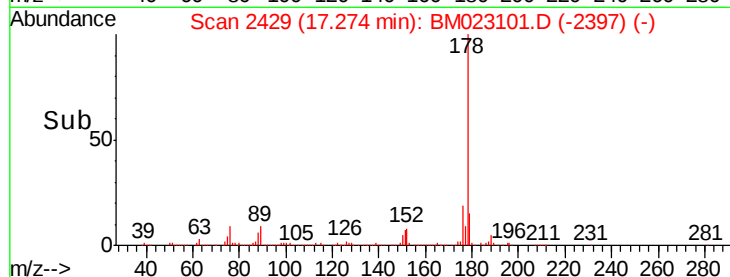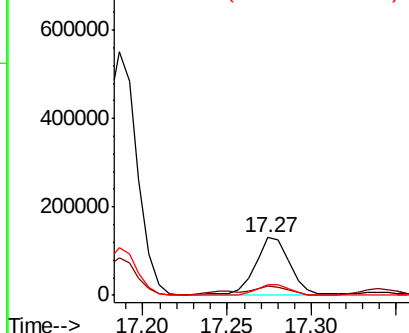

#75

Carbazole

Concen: 1.727 ng/ul


RT: 17.54 min Scan# 2475

Delta R.T. -0.01 min



Lab File: BM023101.D


Acq: 10 Oct 2019 02:55

Tgt Ion:	167	Resp:	70024
Ion Ratio	Lower	Upper	
167	100		
166	21.7	17.1	25.7
139	13.0	9.9	14.9

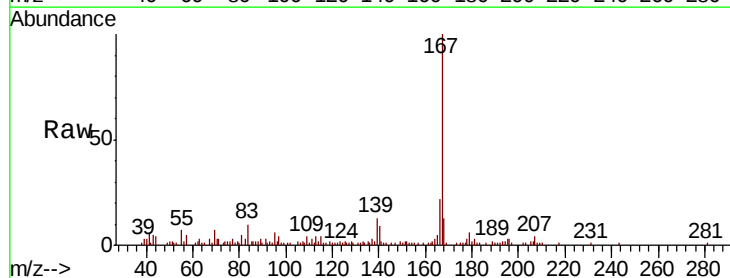

Abundance Ion 167.00 (166.70 to 167.70): E
Ion 166.00 (165.70 to 166.70): E
Ion 139.00 (138.70 to 139.70): E

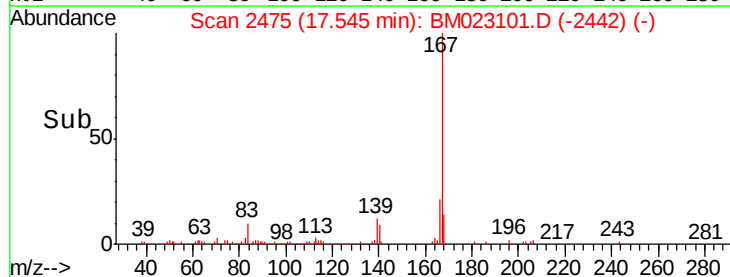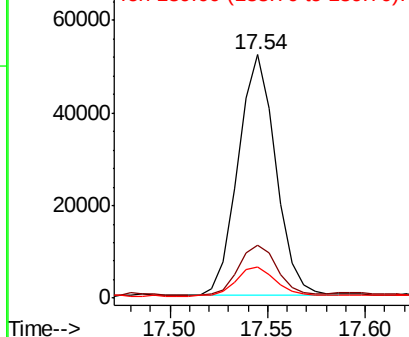







#77
Fluoranthene
 Concen: 31.347 ng/ul
 RT: 19.20 min Scan# 2757
 Delta R.T. -0.01 min
 Lab File: BM023101.D
 Acq: 10 Oct 2019 02:55

Instrument :
 BNA_M
 ClientSampleId :
 BEP95

Tot Ion	Ratio	Lower	Upper
202	100		
101	10.9	8.6	12.8
100	8.1	6.4	9.6




Manual Integrations
 APPROVED


mohammad
 10/11/2019 8:28:40 AM

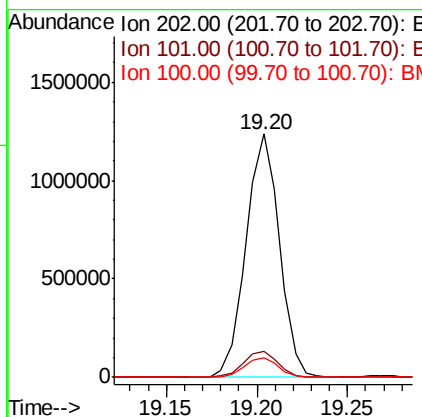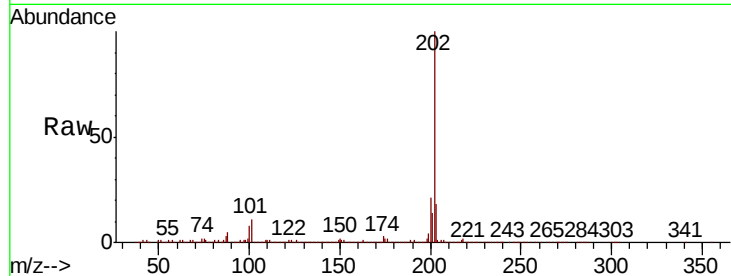

#80
Pyrene
 Concen: 34.134 ng/ul
 RT: 19.57 min Scan# 2819
 Delta R.T. -0.01 min
 Lab File: BM023101.D
 Acq: 10 Oct 2019 02:55

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.5	9.7	14.5
100	10.0	7.8	11.8

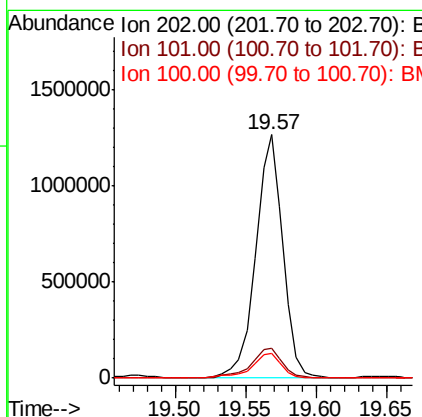



#83

Benzo(a)anthracene

Concen: 19.824 ng/ul

RT: 21.31 min Scan# 3115

Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Instrument :

BNA_M





ClientSampled :

BEP95

Tot Ion:	228	Resp:	1002734
Ion	Ratio	Lower	Upper
228	100		
229	21.1	15.8	23.8
226	28.9	22.4	33.6

Manual Integrations
APPROVED

mohammad
10/11/2019 8:28:40 AM

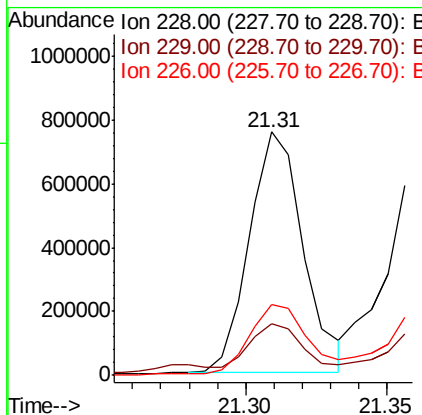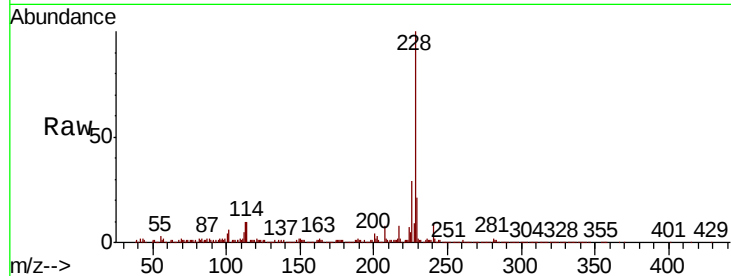

#84

Bis(2-ethylhexyl)phthalate

Concen: 23.974 ng/ul




RT: 21.24 min Scan# 3104


Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Tgt Ion:	149	Resp:	699636
Ion	Ratio	Lower	Upper
149	100		
167	27.1	22.1	33.1
279	4.2	3.3	4.9

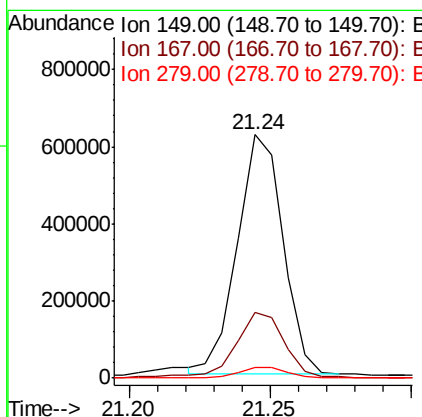



#85

Chrysene

Concen: 22.134 ng/ul

RT: 21.36 min Scan# 3124

Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Instrument :

BNA_M





ClientSampled :

BEP95

Tot Ion:	228	Resp:	1032194
Ion	Ratio	Lower	Upper
228	100		
226	30.6	24.2	36.4
229	21.5	15.9	23.9

Manual Integrations
APPROVED

mohammad
10/11/2019 8:28:40 AM

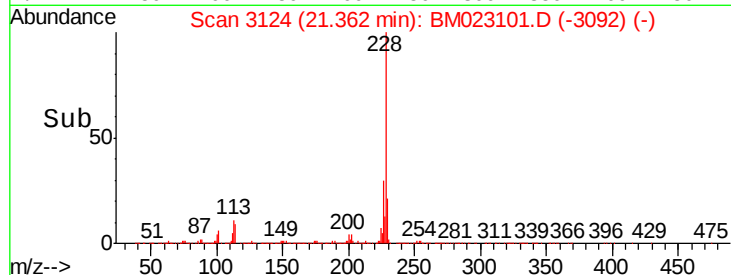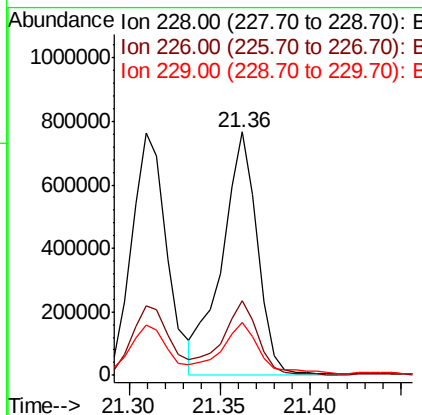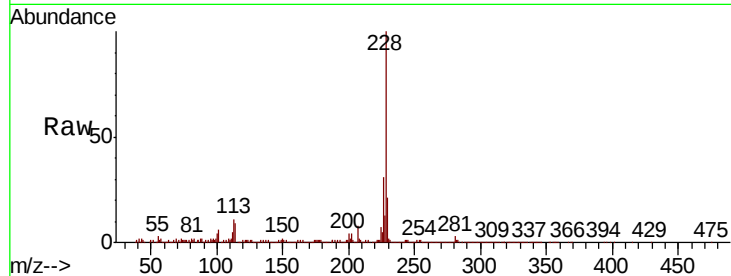

#88

Benzo(b)fluoranthene

Concen: 23.594 ng/ul




RT: 22.90 min Scan# 3386


Delta R.T. -0.01 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Tgt Ion:	252	Resp:	1317057
Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.7	26.5
125	13.3	8.2	12.2#

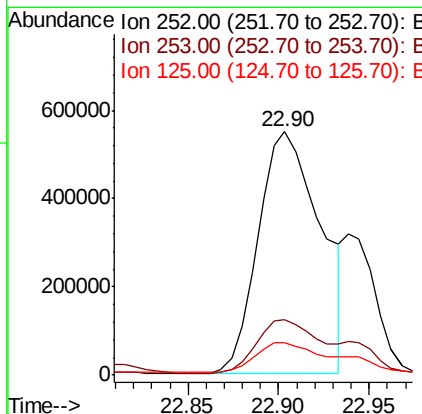







#89
Benzo(k)fluoranthene
Concen: 6.932 ng/ul m
RT: 22.94 min Scan# 3392
Delta R.T. -0.02 min
Lab File: BM023101.D
Acq: 10 Oct 2019 02:55

Instrument :
BNA_M
ClientSampleId :
BEP95

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.2	17.5	26.3
125	13.4	7.9	11.9




Manual Integrations
APPROVED


mohammad
10/11/2019 8:28:40 AM

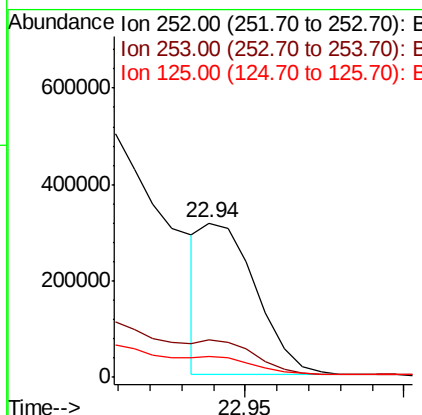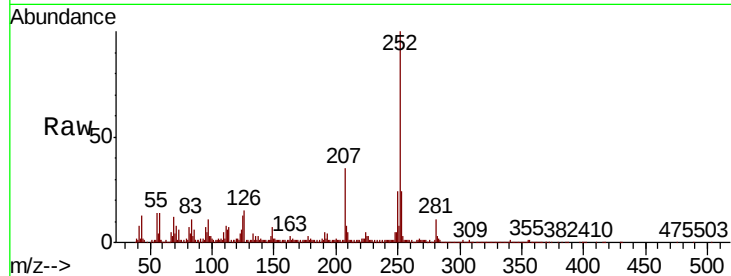

#91
Benzo(a)pyrene
Concen: 19.371 ng/ul
RT: 23.48 min Scan# 3484
Delta R.T. -0.01 min
Lab File: BM023101.D
Acq: 10 Oct 2019 02:55

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.6	26.4
125	13.1	8.7	13.1

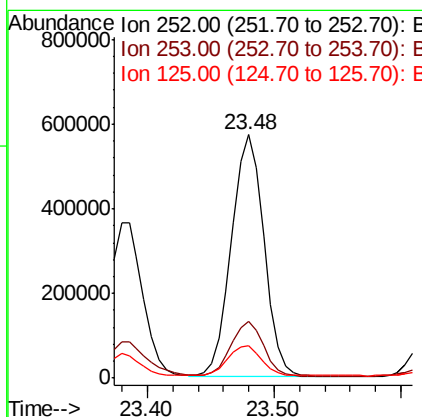

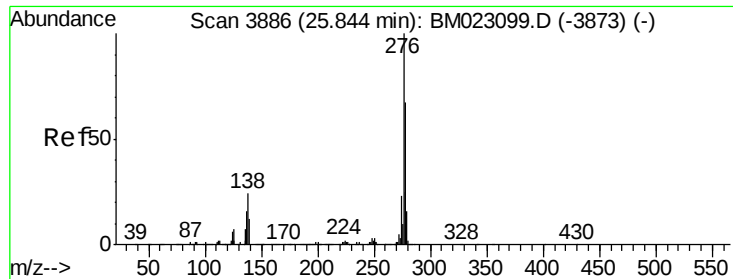





#92
Indeno(1,2,3-cd)pyrene
Concen: 11.692 ng/ul
RT: 25.85 min Scan# 3887
Delta R.T. -0.02 min
Lab File: BM023101.D
Acq: 10 Oct 2019 02:55

Instrument :
BNA_M
ClientSampleId :
BEP95

Tot Ion	Ratio	Lower	Upper
276	100		
138	21.0	19.8	29.8
277	24.7	20.3	30.5




Manual Integrations
APPROVED


mohammad
10/11/2019 8:28:40 AM

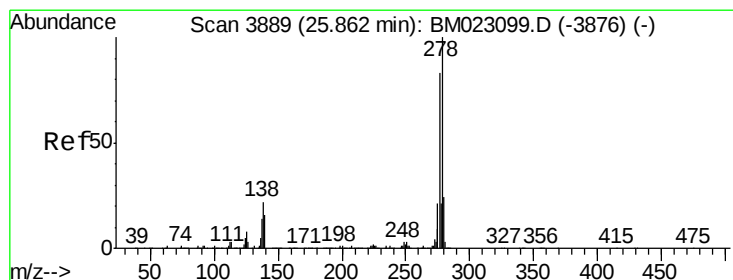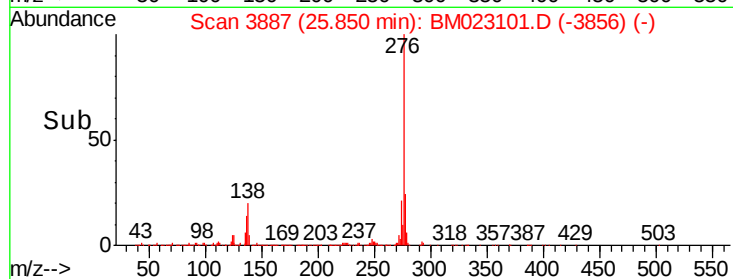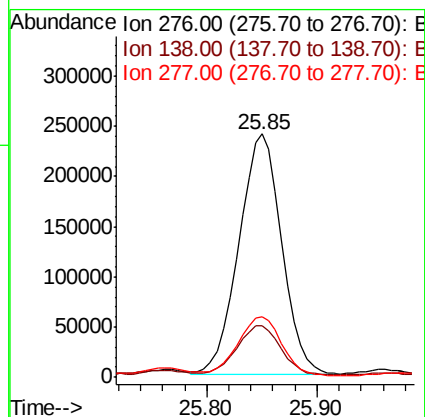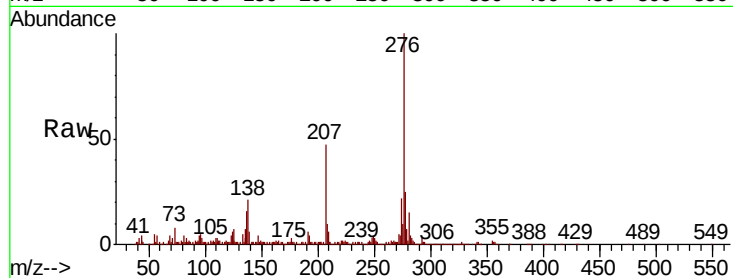

#93
Dibenzo(a,h)anthracene
Concen: 3.922 ng/ul
RT: 25.86 min Scan# 3888
Delta R.T. -0.02 min
Lab File: BM023101.D
Acq: 10 Oct 2019 02:55

Tgt Ion	Ratio	Lower	Upper
278	100		
139	19.7	13.2	19.8
279	27.6	19.0	28.6

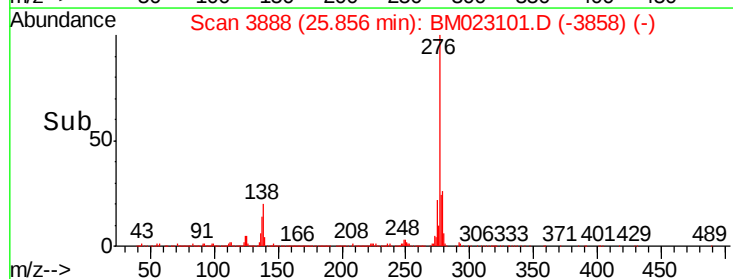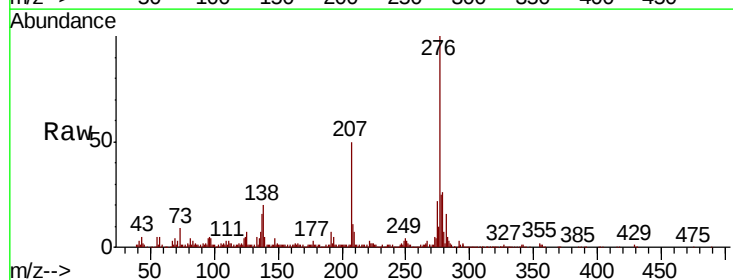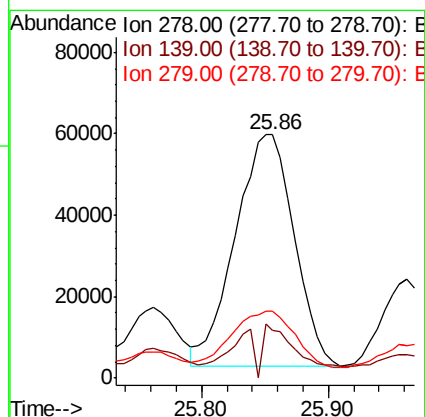



#94

Benzo(a,h,i)perylene

Concen: 13.733 ng/ul

RT: 26.54 min Scan# 4005

Delta R.T. -0.02 min

Lab File: BM023101.D

Acq: 10 Oct 2019 02:55

Instrument :

BNA_M

ClientSampleId :

BEP95

Tot Ion:	276	Resp:	616312
Ion Ratio	Lower	Upper	
276	100		
138	21.2	17.6	26.4
277	24.6	19.1	28.7

Manual Integrations
APPROVED

mohammad
10/11/2019 8:28:40 AM

