

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032377.D
 Acq On : 08 Oct 2021 04:11
 Operator : CG/JU
 Sample : M4003-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00T2

Quant Time: Oct 08 04:56:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 15:38:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	6315	0.40	ng/ul	0.00
4) Naphthalene-d8	10.411	136	20975	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	12897	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	24791	0.40	ng/ul	0.00
17) Chrysene-d12	21.154	240	18558	0.40	ng/ul	0.00
23) Perylene-d12	23.295	264	18123	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.965	96	38426	5.66	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.003	152	12207	0.44	ng/ul	0.00
18) Fluoranthene-d10	19.015	212	28893	0.57	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.460	128	2270	0.04	ng/ul#	88
11) Acenaphthene	14.346	153	1039	0.02	ng/ul#	39
15) Phenanthrene	17.036	178	3616	0.04	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032377.D
Acq On : 08 Oct 2021 04:11
Operator : CG/JU
Sample : M4003-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00T2

Quant Time: Oct 08 04:56:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 15:38:40 2021
Response via : Initial Calibration




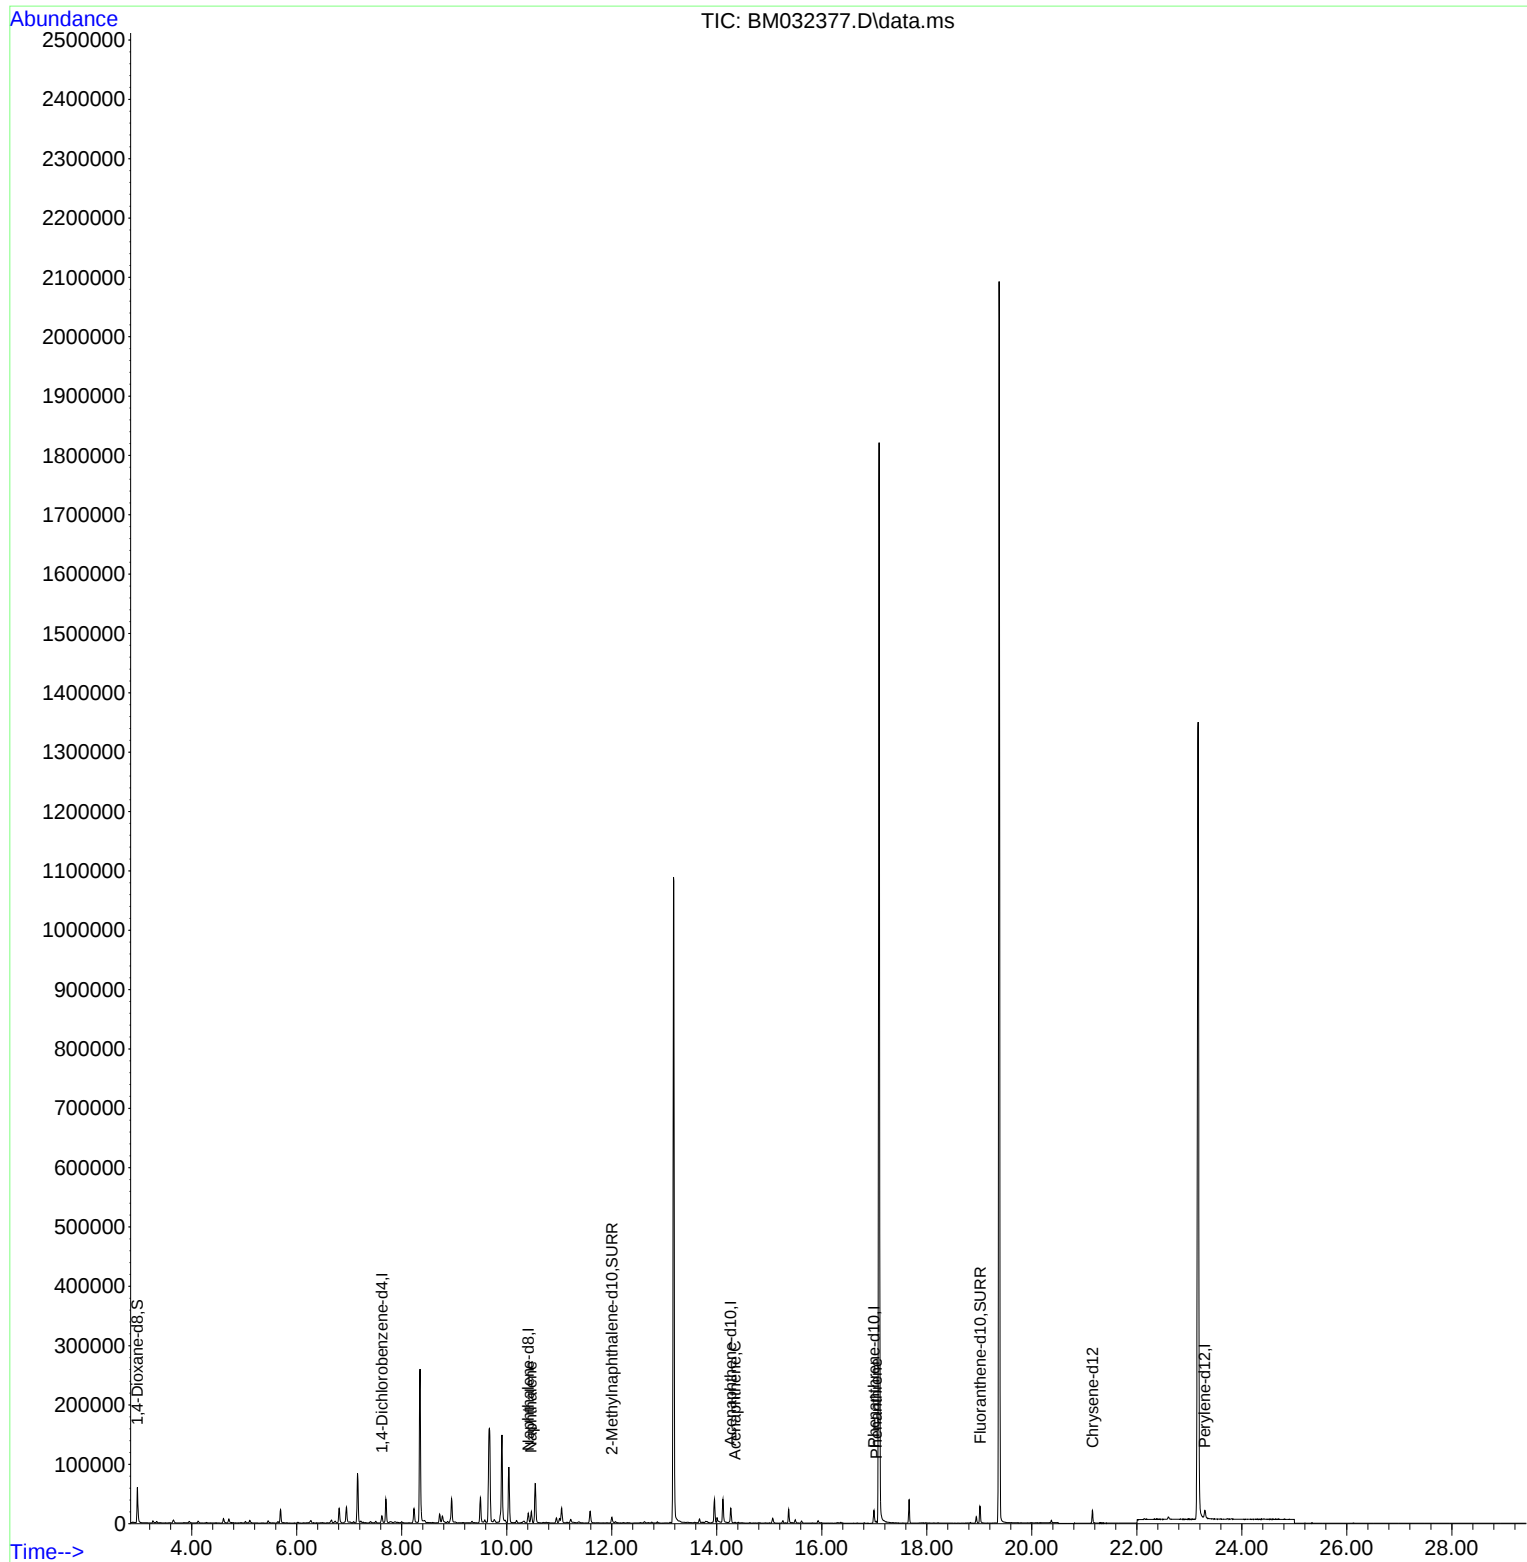


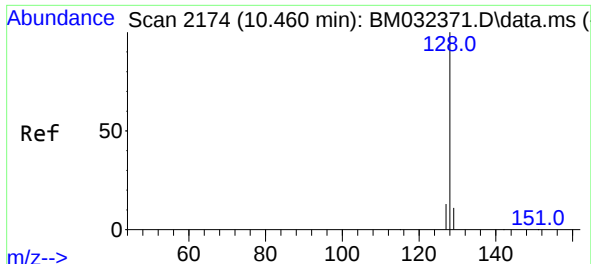

#5
Naphthalene
Concen: 0.04 ng/ul
RT: 10.460 min Scan# 2174
Delta R.T. 0.000 min
Lab File: BM032377.D
Acq: 08 Oct 2021 04:11




Instrument :
BNA_M
ClientSampled :
C00T2


Tgt Ion:128 Resp: 2270
Ion Ratio Lower Upper
128 100
129 17.4 9.0 13.4#
127 16.7 10.5 15.7#

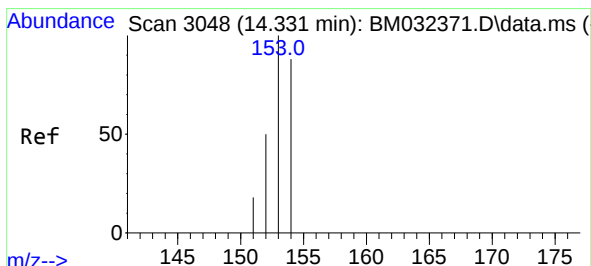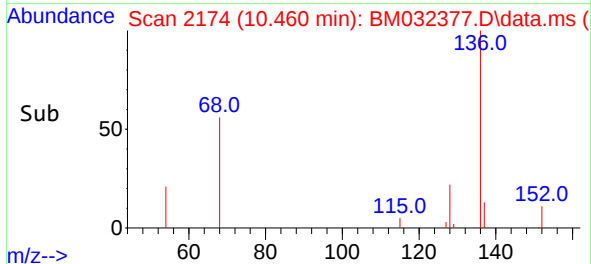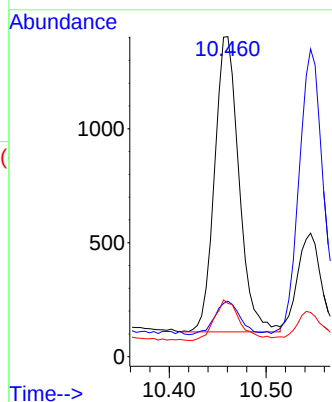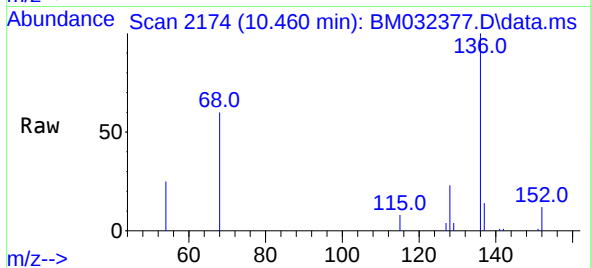

#11
Acenaphthene
Concen: 0.02 ng/ul
RT: 14.346 min Scan# 3052
Delta R.T. 0.011 min
Lab File: BM032377.D
Acq: 08 Oct 2021 04:11


Tgt Ion:153 Resp: 1039
Ion Ratio Lower Upper
153 100
152 25.7 41.6 62.4#
154 19.5 71.2 106.8#

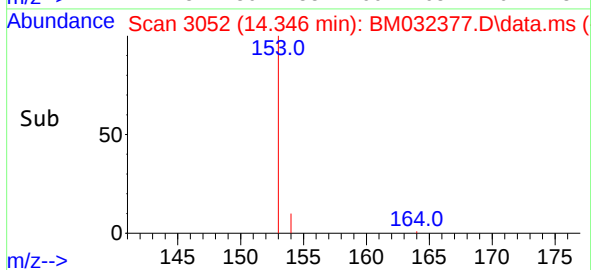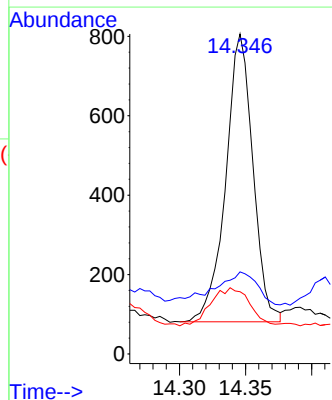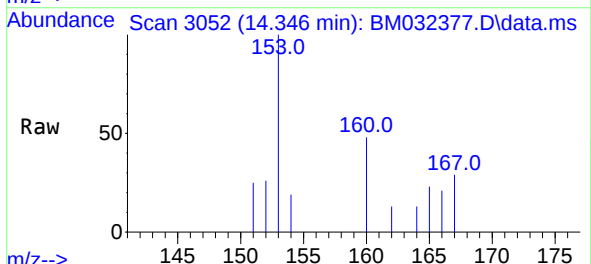

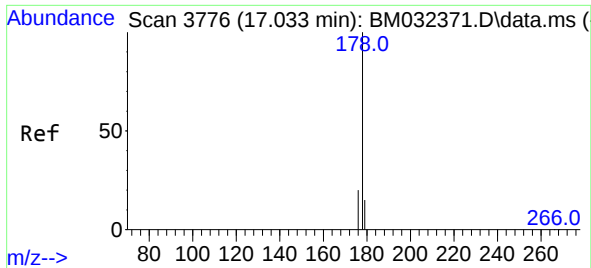

#15
Phenanthrene
Concen: 0.04 ng/ul
RT: 17.036 min Scan# 3777
Delta R.T. 0.000 min
Lab File: BM032377.D
Acq: 08 Oct 2021 04:11

Instrument :
BNA_M
ClientSampleId :
C00T2

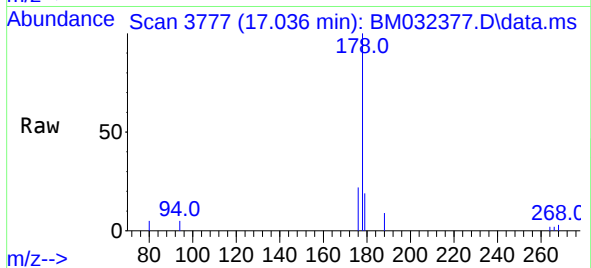

Tgt Ion:178 Resp: 3616
Ion Ratio Lower Upper
178 100
179 19.4 12.6 18.8#
176 22.0 15.8 23.6

