

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032381.D
 Acq On : 08 Oct 2021 06:34
 Operator : CG/JU
 Sample : M4003-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S3

Quant Time: Oct 08 07:51:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 15:38:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	6043	0.40	ng/ul	0.00
4) Naphthalene-d8	10.411	136	20989	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	11902	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	24412	0.40	ng/ul	0.00
17) Chrysene-d12	21.155	240	18599	0.40	ng/ul	0.00
23) Perylene-d12	23.298	264	18804	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.965	96	34885	5.37	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.999	152	9535	0.34	ng/ul	0.00
18) Fluoranthene-d10	19.011	212	26428	0.52	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.003	88	717	0.11	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032381.D
Acq On : 08 Oct 2021 06:34
Operator : CG/JU
Sample : M4003-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S3


Quant Time: Oct 08 07:51:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 15:38:40 2021
Response via : Initial Calibration

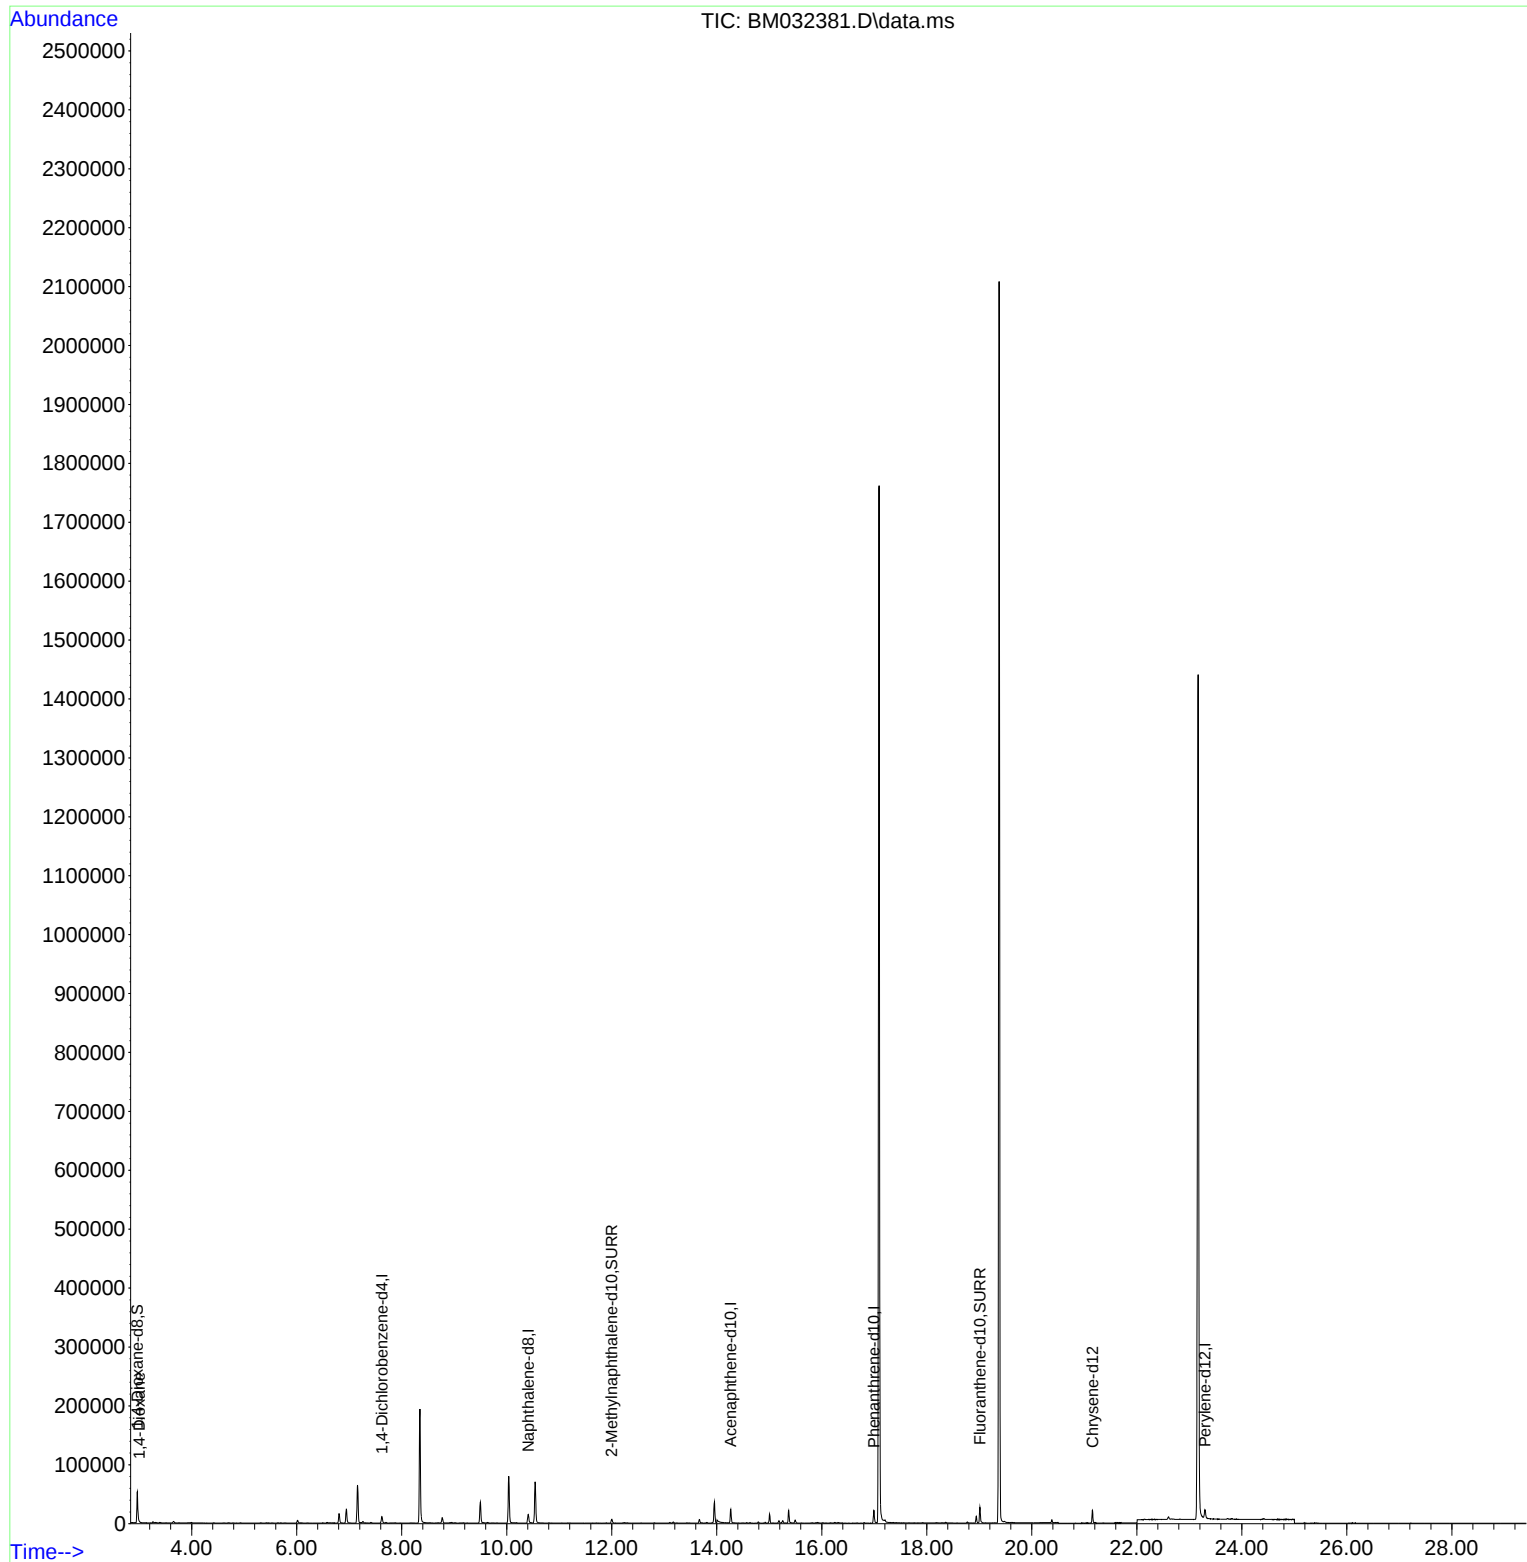


Abundance Scan 50 (3.006 min): BM032371.D\data.ms (-39)

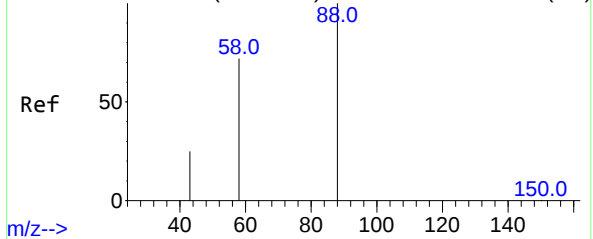

Abundance Scan 49 (3.003 min): BM032381.D\data.ms

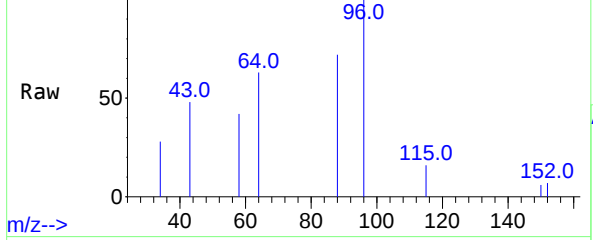


Abundance Scan 49 (3.003 min): BM032381.D\data.ms (-34)

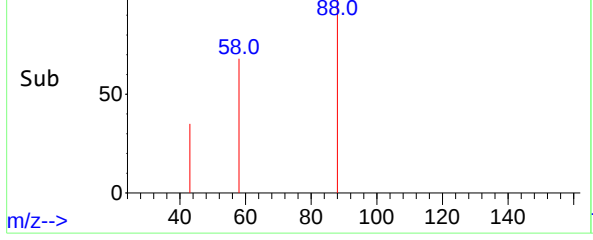

#2
1,4-Dioxane
Concen: 0.11 ng/ul
RT: 3.003 min Scan# 49
Delta R.T. 0.000 min
Lab File: BM032381.D
Acq: 08 Oct 2021 06:34

Tgt Ion:	88	Resp:	717
Ion	Ratio	Lower	Upper
88	100		
43	67.1	26.1	39.1#
58	58.8	50.2	75.2

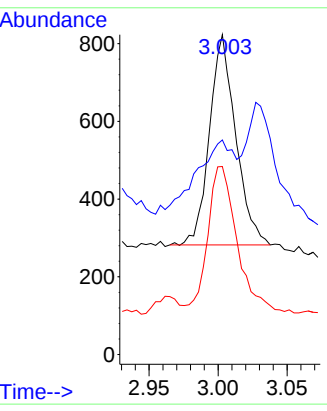

Instrument :
BNA_M
ClientSampleId :
C00S3