

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032386.D
 Acq On : 08 Oct 2021 10:10
 Operator : CG/JU
 Sample : M4003-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00Q0

Quant Time: Oct 08 11:07:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 15:38:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	6757	0.40	ng/ul	0.00
4) Naphthalene-d8	10.411	136	24021	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	13702	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	27903	0.40	ng/ul	0.00
17) Chrysene-d12	21.154	240	21321	0.40	ng/ul	0.00
23) Perylene-d12	23.298	264	21316	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.965	96	35125	4.84	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.003	152	10234	0.32	ng/ul	0.00
18) Fluoranthene-d10	19.011	212	29512	0.51	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.033	178	2274	0.03	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032386.D
Acq On : 08 Oct 2021 10:10
Operator : CG/JU
Sample : M4003-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00Q0


Quant Time: Oct 08 11:07:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 15:38:40 2021
Response via : Initial Calibration

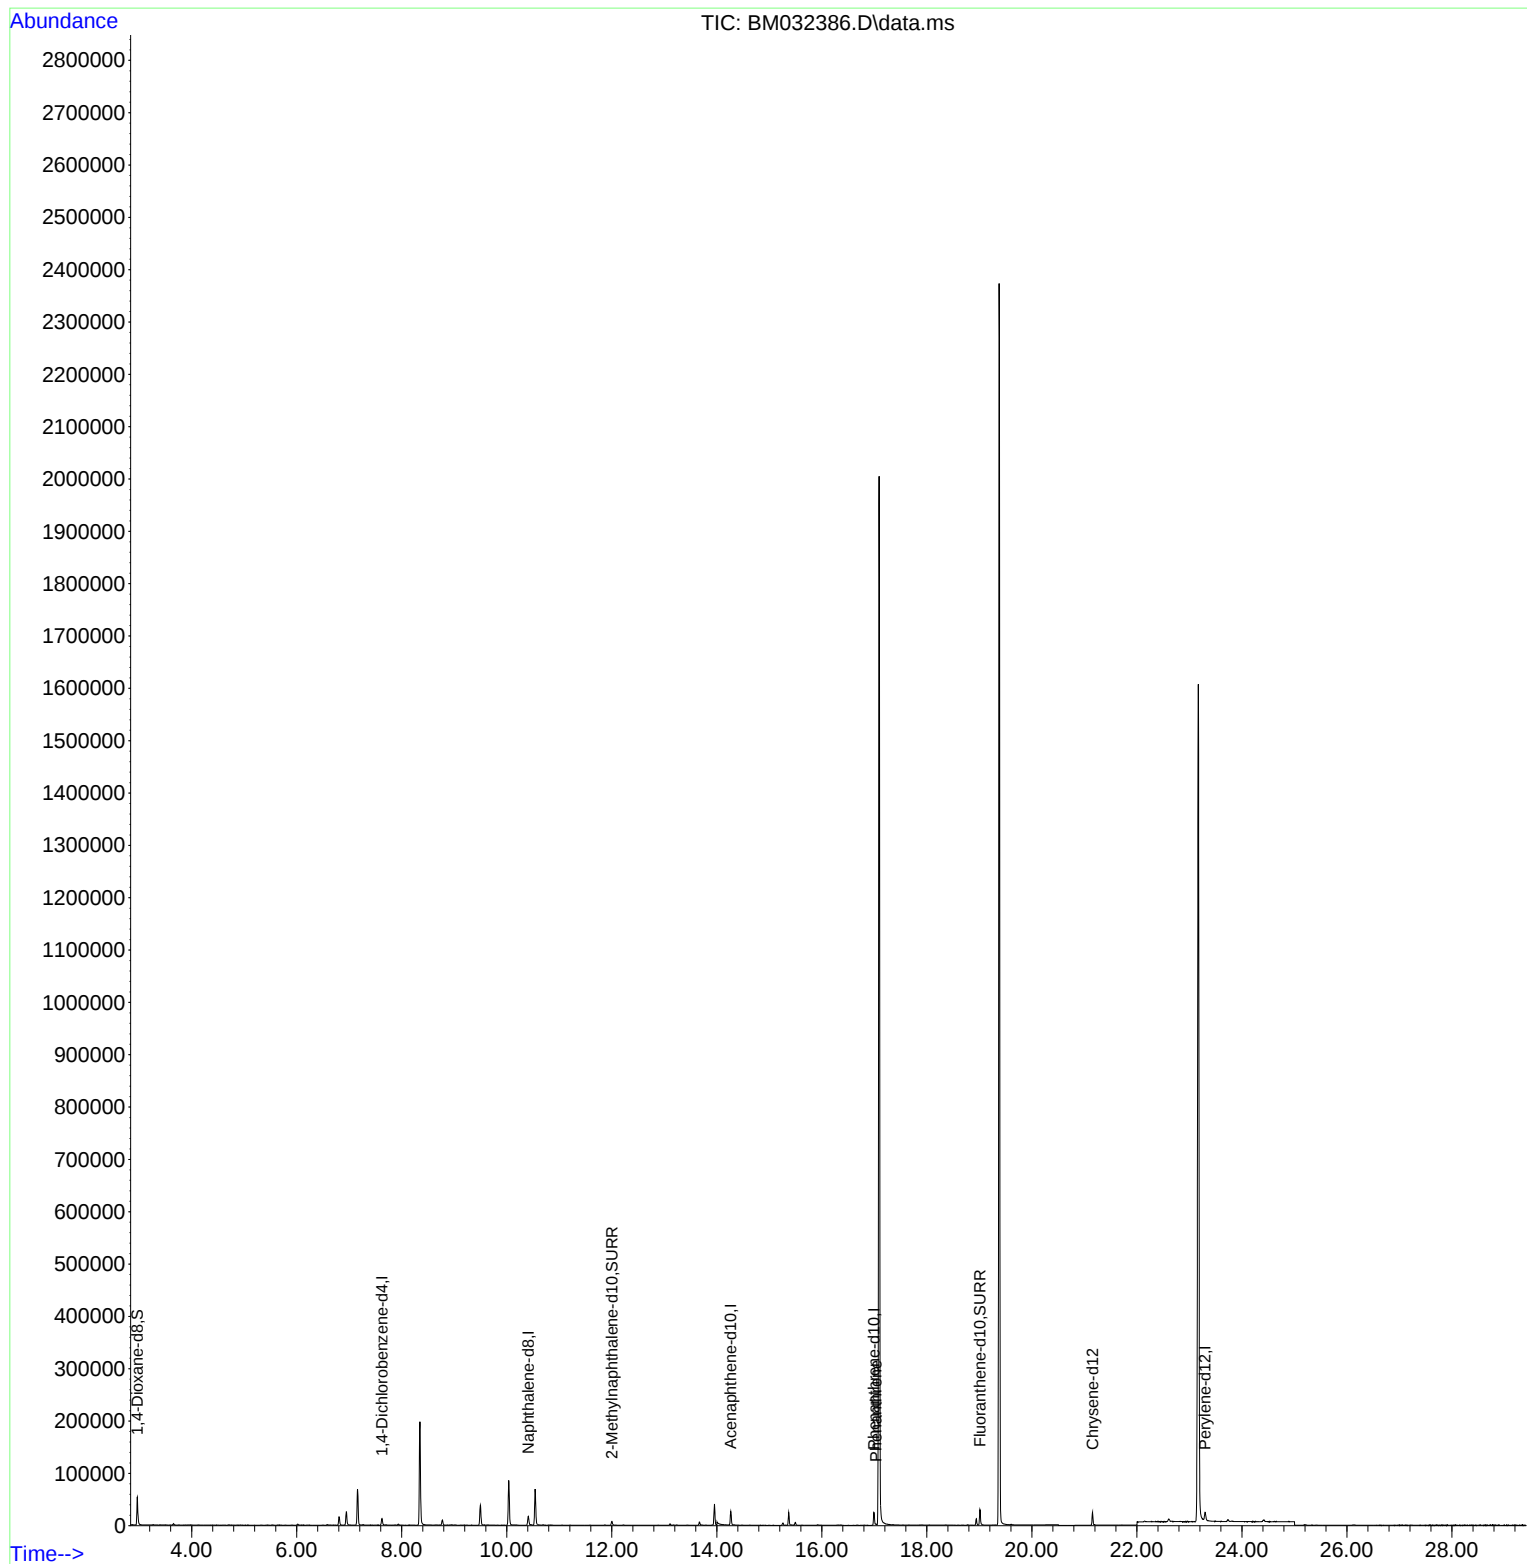

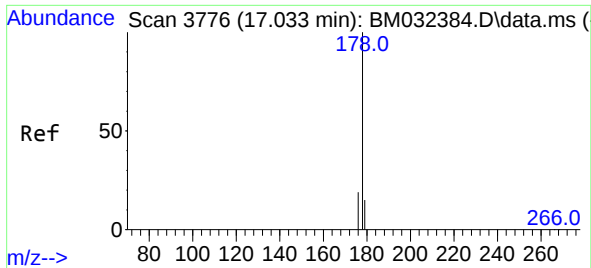

#15
Phenanthrene
Concen: 0.03 ng/ul
RT: 17.033 min Scan# 3776
Delta R.T. -0.003 min
Lab File: BM032386.D
Acq: 08 Oct 2021 10:10

Instrument :
BNA_M
ClientSampleId :
C00Q0

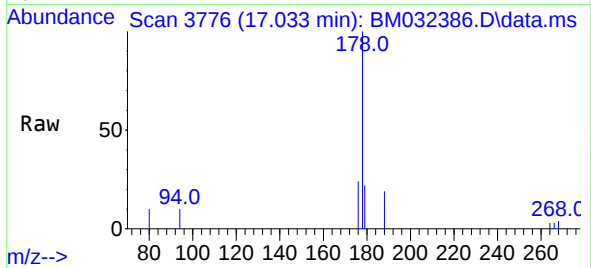

Tgt Ion:	178	Resp:	2274
Ion	Ratio	Lower	Upper
178	100		
179	22.4	12.6	18.8#
176	23.9	15.8	23.6#

