

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032387.D
 Acq On : 08 Oct 2021 10:46
 Operator : CG/JU
 Sample : M4003-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00T2

Quant Time: Oct 08 12:29:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 12:27:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	6687	0.40	ng/ul	0.00
4) Naphthalene-d8	10.411	136	22761	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	13548	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.991	188	26436	0.40	ng/ul	0.00
17) Chrysene-d12	21.157	240	20618	0.40	ng/ul	0.00
23) Perylene-d12	23.298	264	21039	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.965	96	33848	4.71	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.999	152	11169	0.37	ng/ul	0.00
18) Fluoranthene-d10	19.011	212	26543	0.47	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.456	128	2083	0.03	ng/ul#	87
15) Phenanthrene	17.033	178	3284	0.04	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032387.D
Acq On : 08 Oct 2021 10:46
Operator : CG/JU
Sample : M4003-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00T2

Quant Time: Oct 08 12:29:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 12:27:26 2021
Response via : Initial Calibration




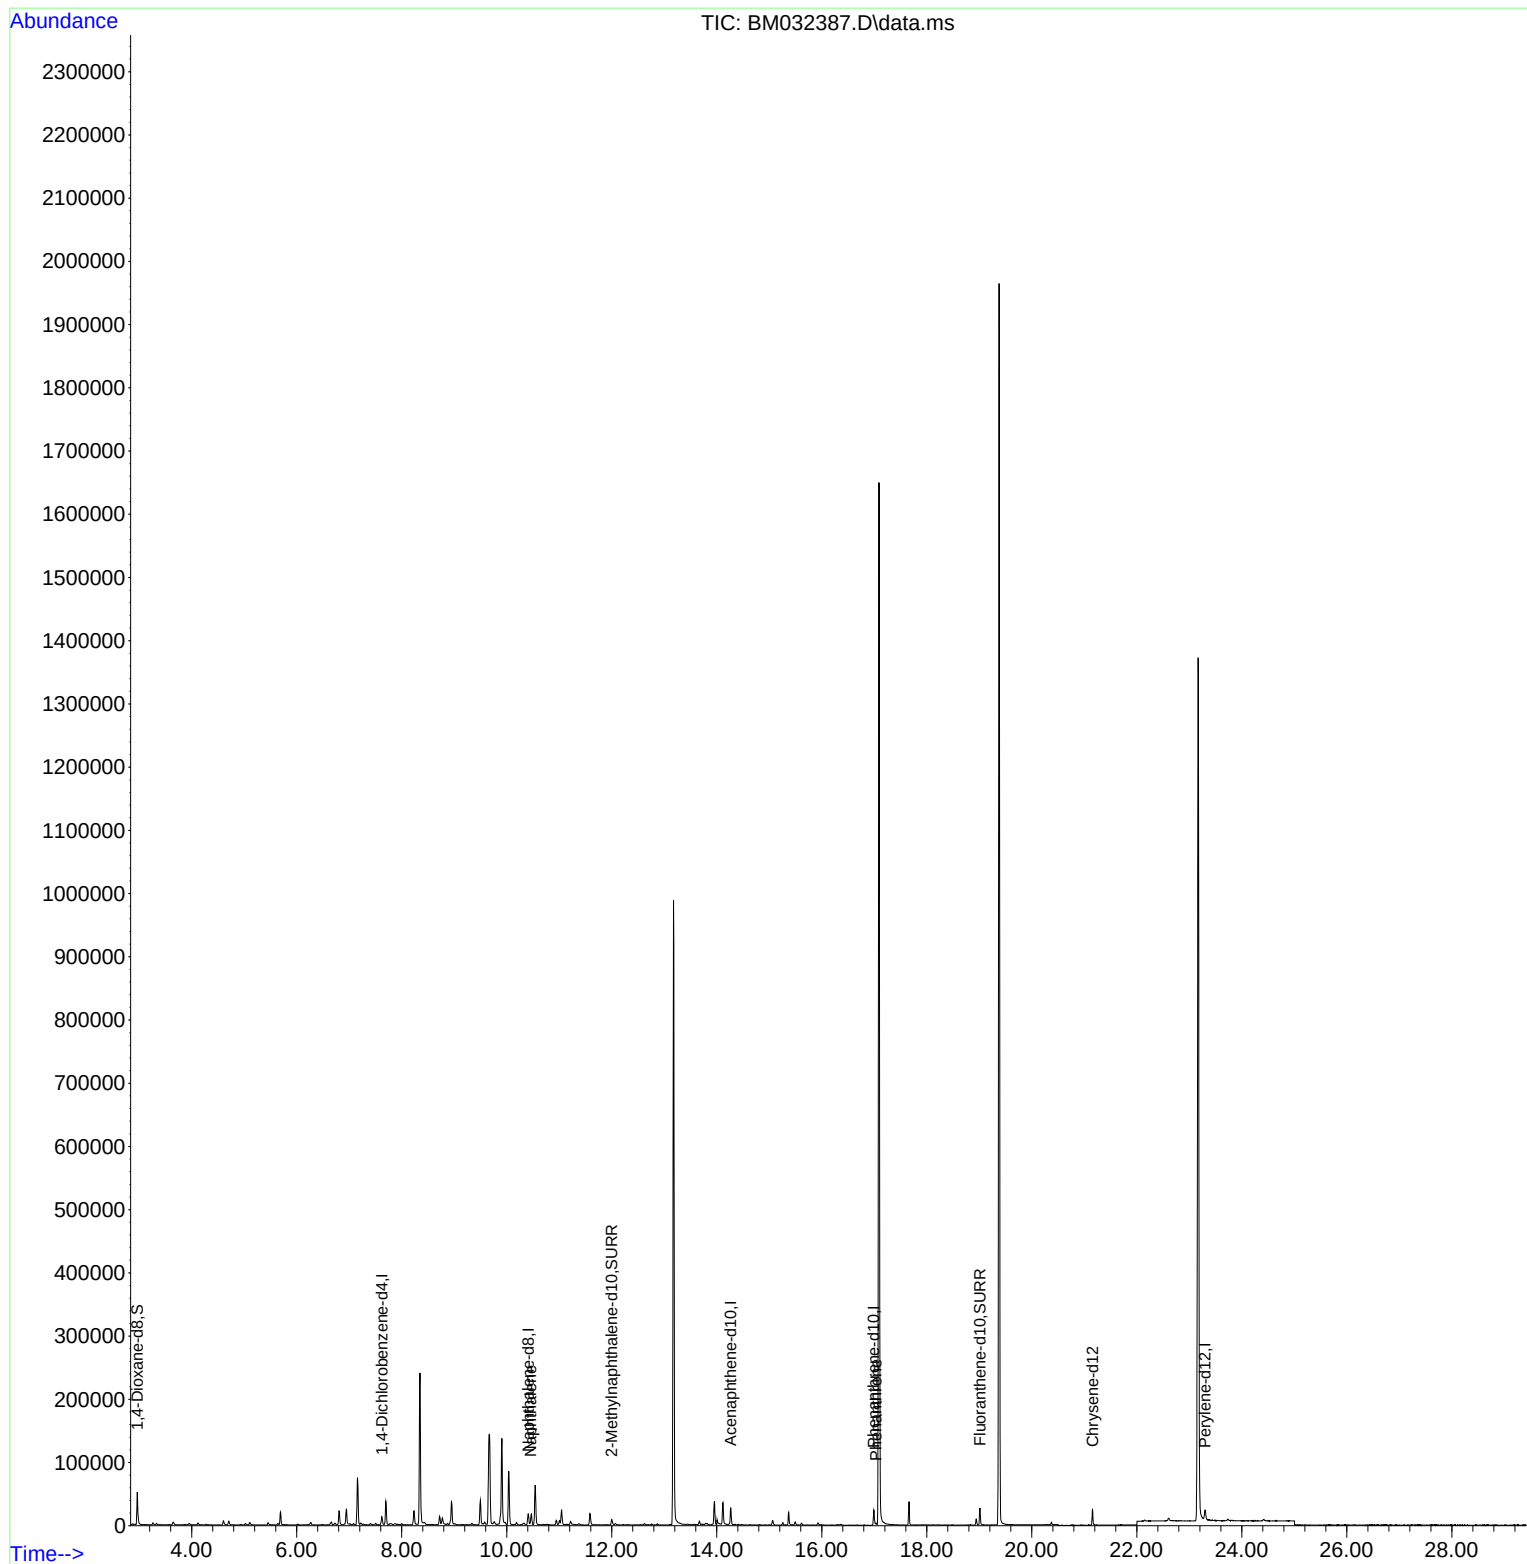


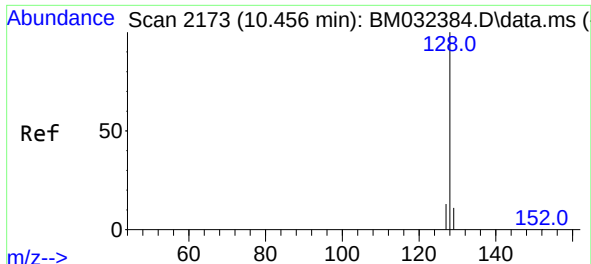

#5
Naphthalene
Concen: 0.03 ng/ul
RT: 10.456 min Scan# 2173
Delta R.T. -0.000 min
Lab File: BM032387.D
Acq: 08 Oct 2021 10:46

Instrument :
BNA_M
ClientSampled :
C00T2

Tgt Ion:128 Resp: 2083
Ion Ratio Lower Upper
128 100
129 16.7 9.0 13.4#
127 17.9 10.5 15.7#

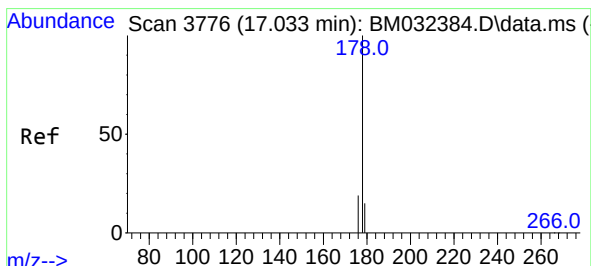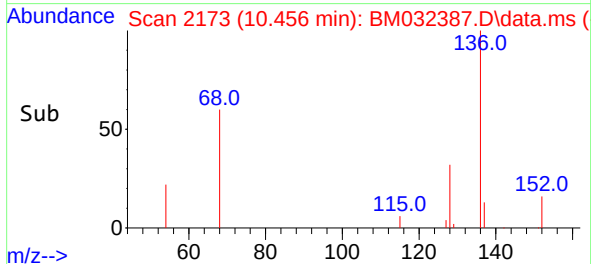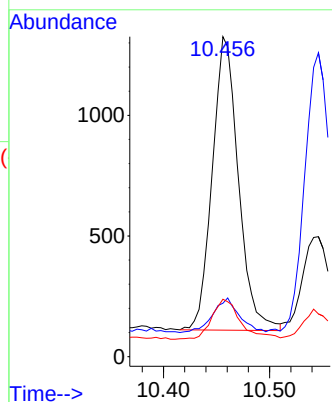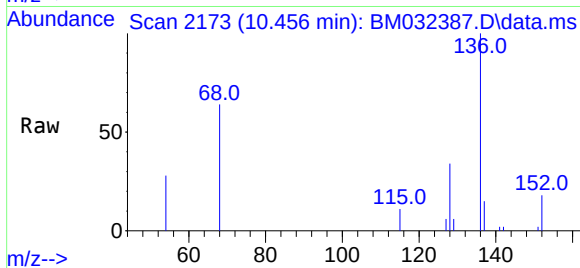

#15
Phenanthrene
Concen: 0.04 ng/ul
RT: 17.033 min Scan# 3776
Delta R.T. -0.000 min
Lab File: BM032387.D
Acq: 08 Oct 2021 10:46

Tgt Ion:178 Resp: 3284
Ion Ratio Lower Upper
178 100
179 19.5 12.6 18.8#
176 22.2 15.8 23.6

