

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032388.D
 Acq On : 08 Oct 2021 11:23
 Operator : CG/JU
 Sample : M4003-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S1

Quant Time: Oct 08 12:30:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 12:27:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	7947	0.40	ng/ul	0.00
4) Naphthalene-d8	10.411	136	28105	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	15900	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.991	188	32928	0.40	ng/ul	0.00
17) Chrysene-d12	21.157	240	25641	0.40	ng/ul	0.00
23) Perylene-d12	23.300	264	25690	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.965	96	41223	4.83	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.003	152	11489	0.31	ng/ul	0.00
18) Fluoranthene-d10	19.011	212	33174	0.48	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.006	88	846	0.10	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032388.D
Acq On : 08 Oct 2021 11:23
Operator : CG/JU
Sample : M4003-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S1


Quant Time: Oct 08 12:30:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 12:27:26 2021
Response via : Initial Calibration

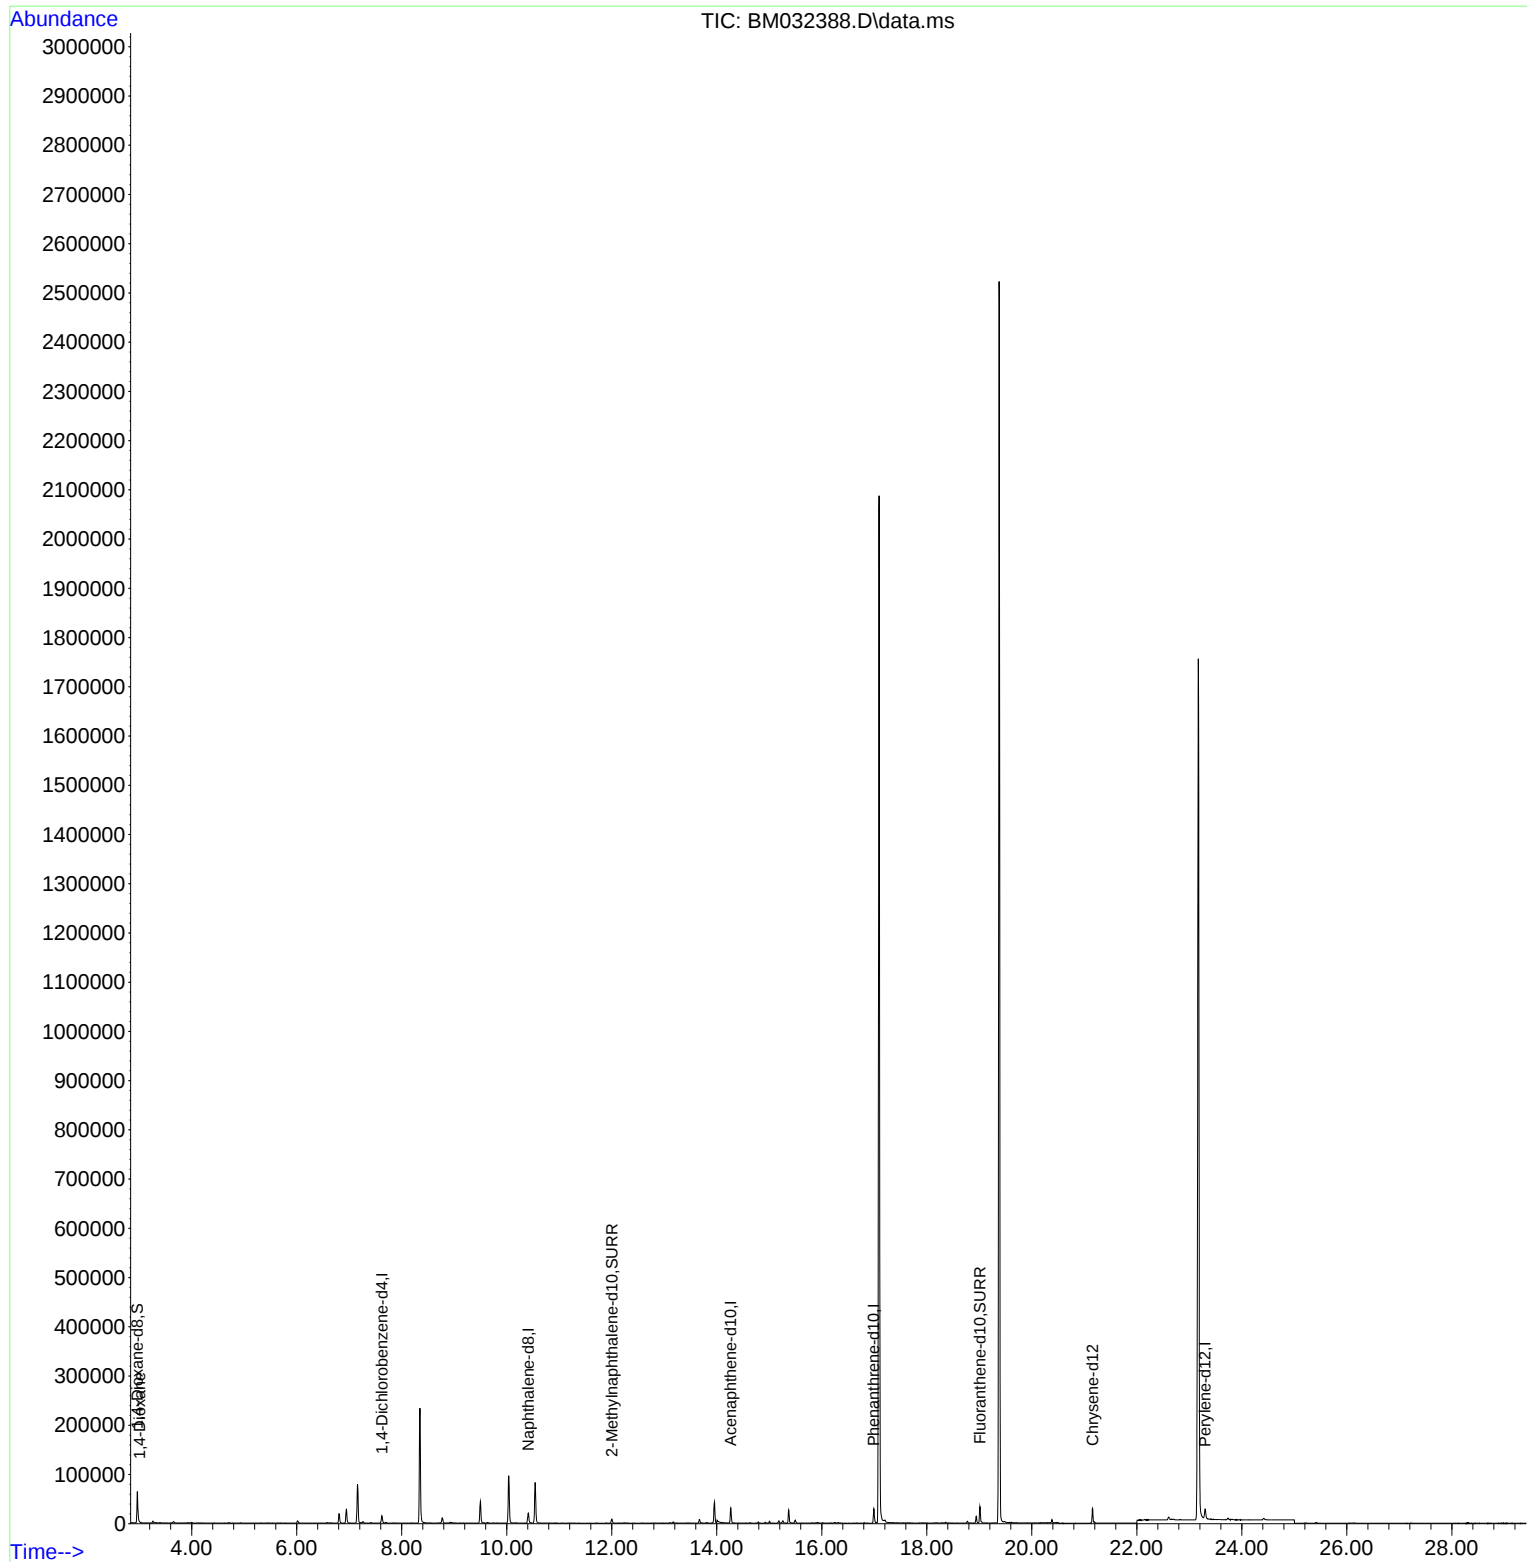


Abundance Scan 49 (3.003 min): BM032384.D\data.ms (-40)

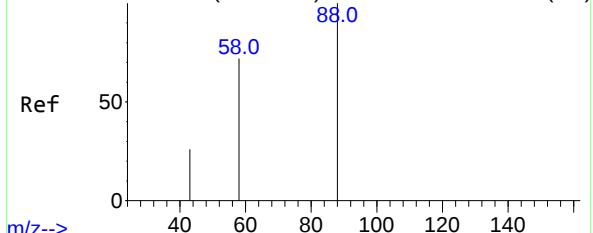

Abundance Scan 50 (3.006 min): BM032388.D\data.ms

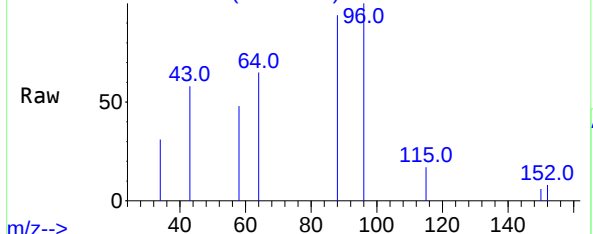


Abundance Scan 50 (3.006 min): BM032388.D\data.ms (-35)

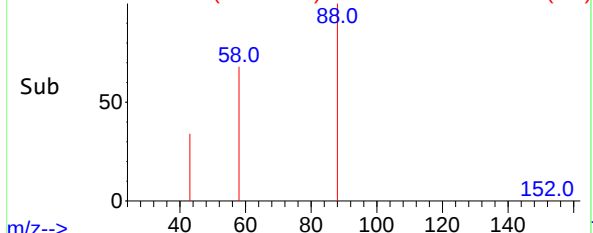

#2
1,4-Dioxane
Concen: 0.10 ng/ul
RT: 3.006 min Scan# 50
Delta R.T. 0.003 min
Lab File: BM032388.D
Acq: 08 Oct 2021 11:23

Tgt Ion: 88	Resp: 846
Ion Ratio	Lower Upper
88	100
43	61.6 26.1 39.1#
58	50.7 50.2 75.2

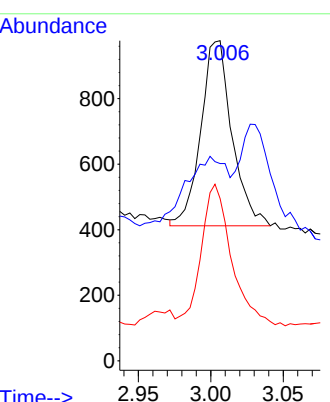

Instrument :
BNA_M
ClientSampleId :
C00S1