

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032389.D
 Acq On : 08 Oct 2021 11:59
 Operator : CG/JU
 Sample : M4003-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00Q6

Quant Time: Oct 08 12:31:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 12:27:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	6391	0.40	ng/ul	0.00
4) Naphthalene-d8	10.411	136	22434	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	12852	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.991	188	25476	0.40	ng/ul	0.00
17) Chrysene-d12	21.157	240	19471	0.40	ng/ul	0.00
23) Perylene-d12	23.300	264	19923	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.962	96	33024	4.81	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.003	152	9618	0.32	ng/ul	0.00
18) Fluoranthene-d10	19.012	212	26286	0.50	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.003	88	914	0.13	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032389.D
Acq On : 08 Oct 2021 11:59
Operator : CG/JU
Sample : M4003-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00Q6


Quant Time: Oct 08 12:31:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 12:27:26 2021
Response via : Initial Calibration

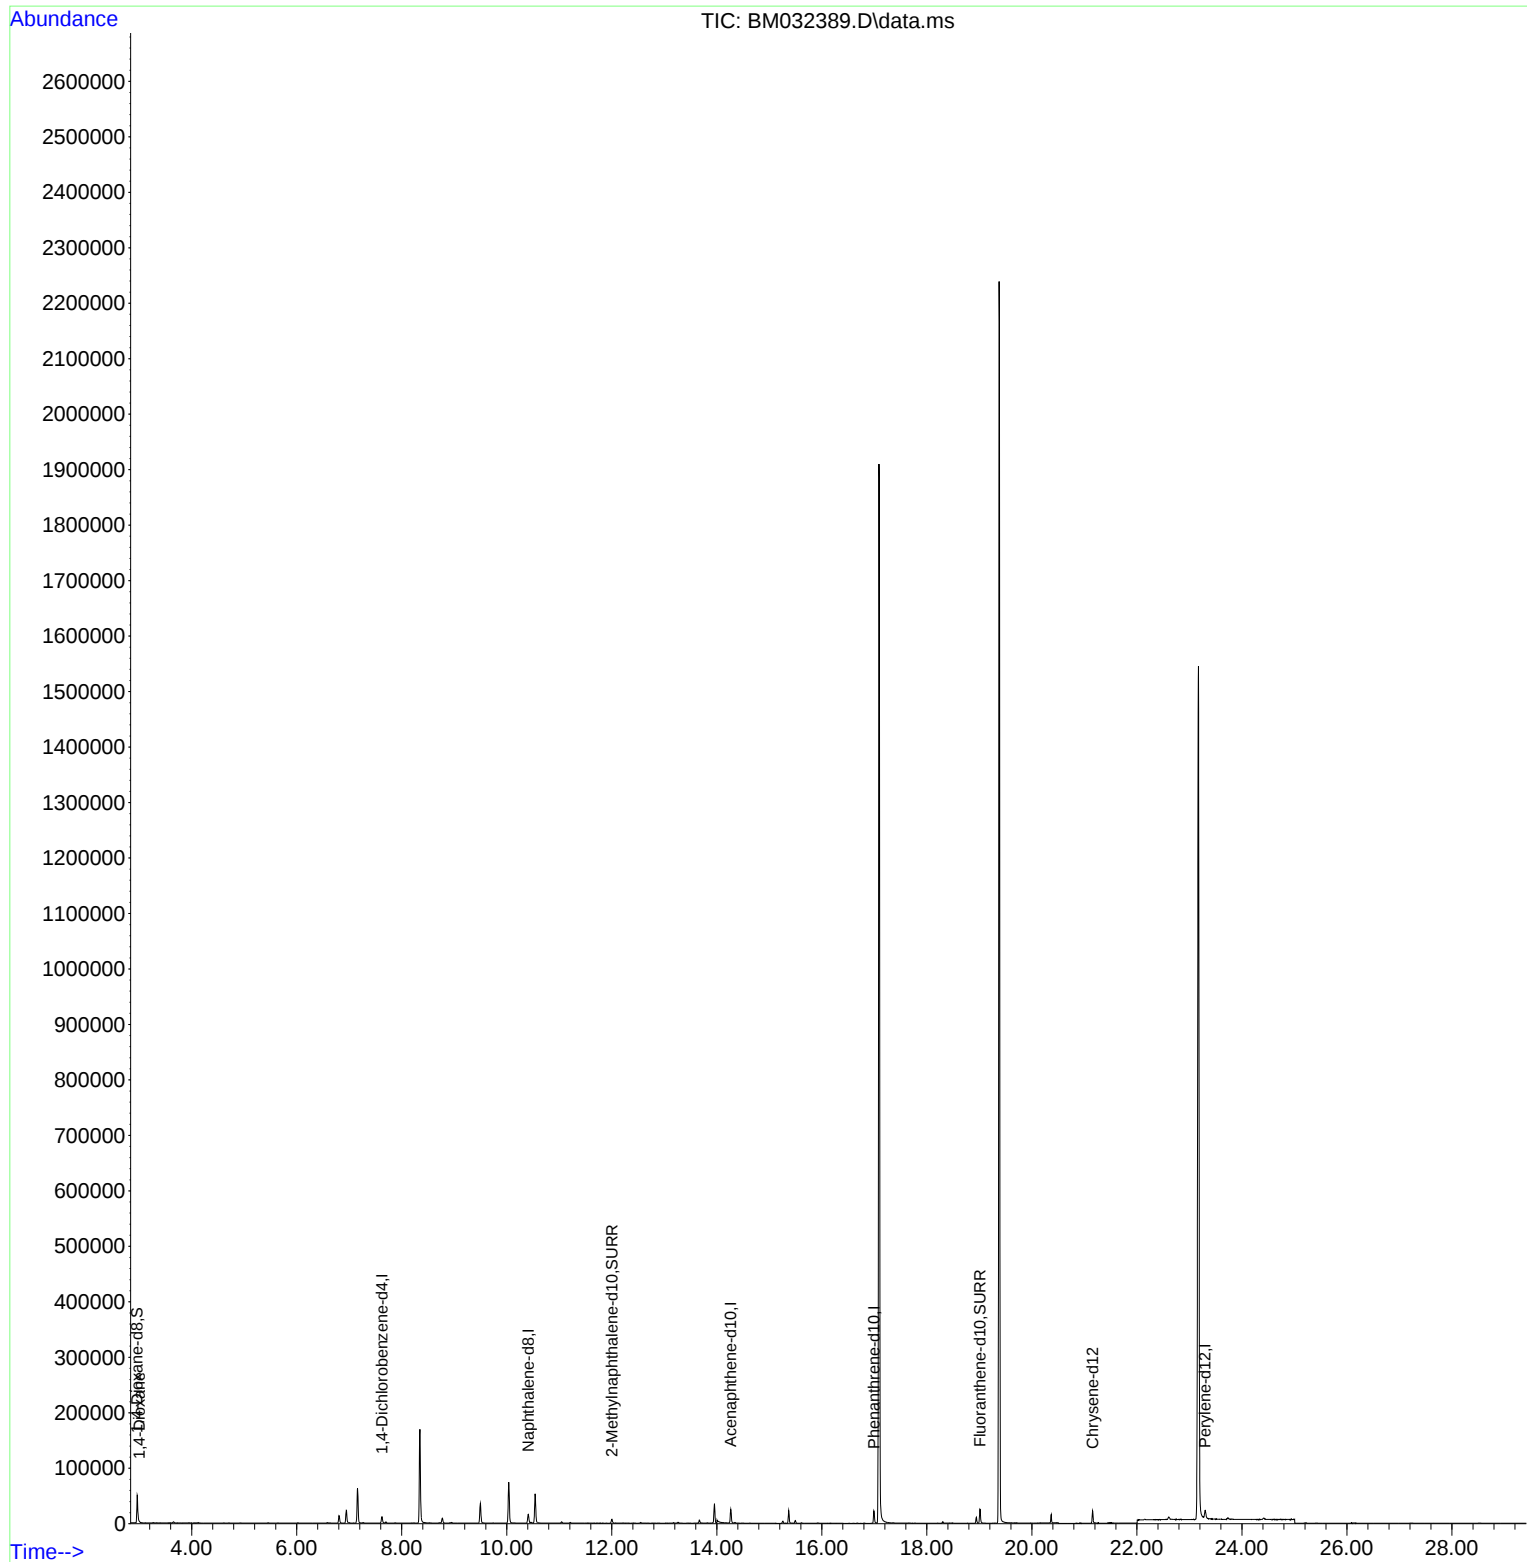


Abundance Scan 49 (3.003 min): BM032384.D\data.ms (-40)

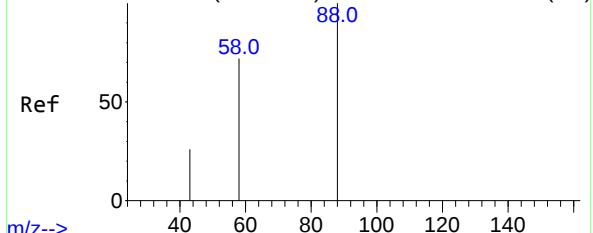

Abundance Scan 49 (3.003 min): BM032389.D\data.ms

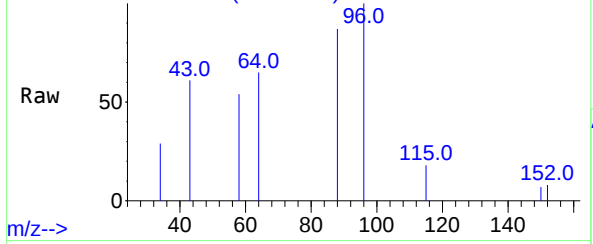


Abundance Scan 49 (3.003 min): BM032389.D\data.ms (-35)

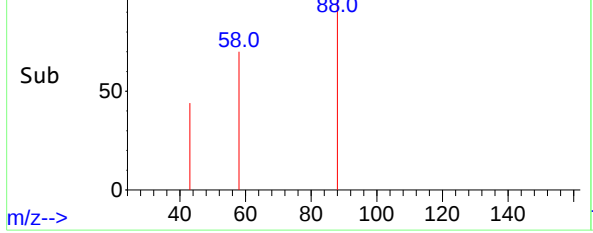

#2
1,4-Dioxane
Concen: 0.13 ng/ul
RT: 3.003 min Scan# 49
Delta R.T. 0.000 min
Lab File: BM032389.D
Acq: 08 Oct 2021 11:59

Tgt Ion: 88	Resp: 914
Ion Ratio	Lower Upper
88	100
43	70.8 26.1 39.1#
58	62.6 50.2 75.2

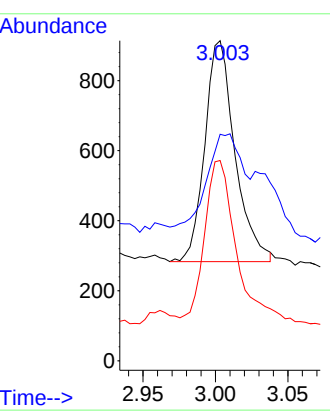

Instrument :
BNA_M
ClientSampleId :
C00Q6