

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
 Data File : BM032391.D
 Acq On : 08 Oct 2021 13:28
 Operator : CG/JU
 Sample : M4003-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S3

Quant Time: Oct 08 13:59:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 12:27:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	6590	0.40	ng/ul	0.00
4) Naphthalene-d8	10.407	136	23139	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.266	164	13240	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	27225	0.40	ng/ul	0.00
17) Chrysene-d12	21.157	240	20721	0.40	ng/ul	0.00
23) Perylene-d12	23.300	264	20960	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.962	96	36666	5.18	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.999	152	10214	0.33	ng/ul	0.00
18) Fluoranthene-d10	19.012	212	28266	0.50	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.000	88	779	0.11	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100821\
Data File : BM032391.D
Acq On : 08 Oct 2021 13:28
Operator : CG/JU
Sample : M4003-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S3


Quant Time: Oct 08 13:59:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 12:27:26 2021
Response via : Initial Calibration

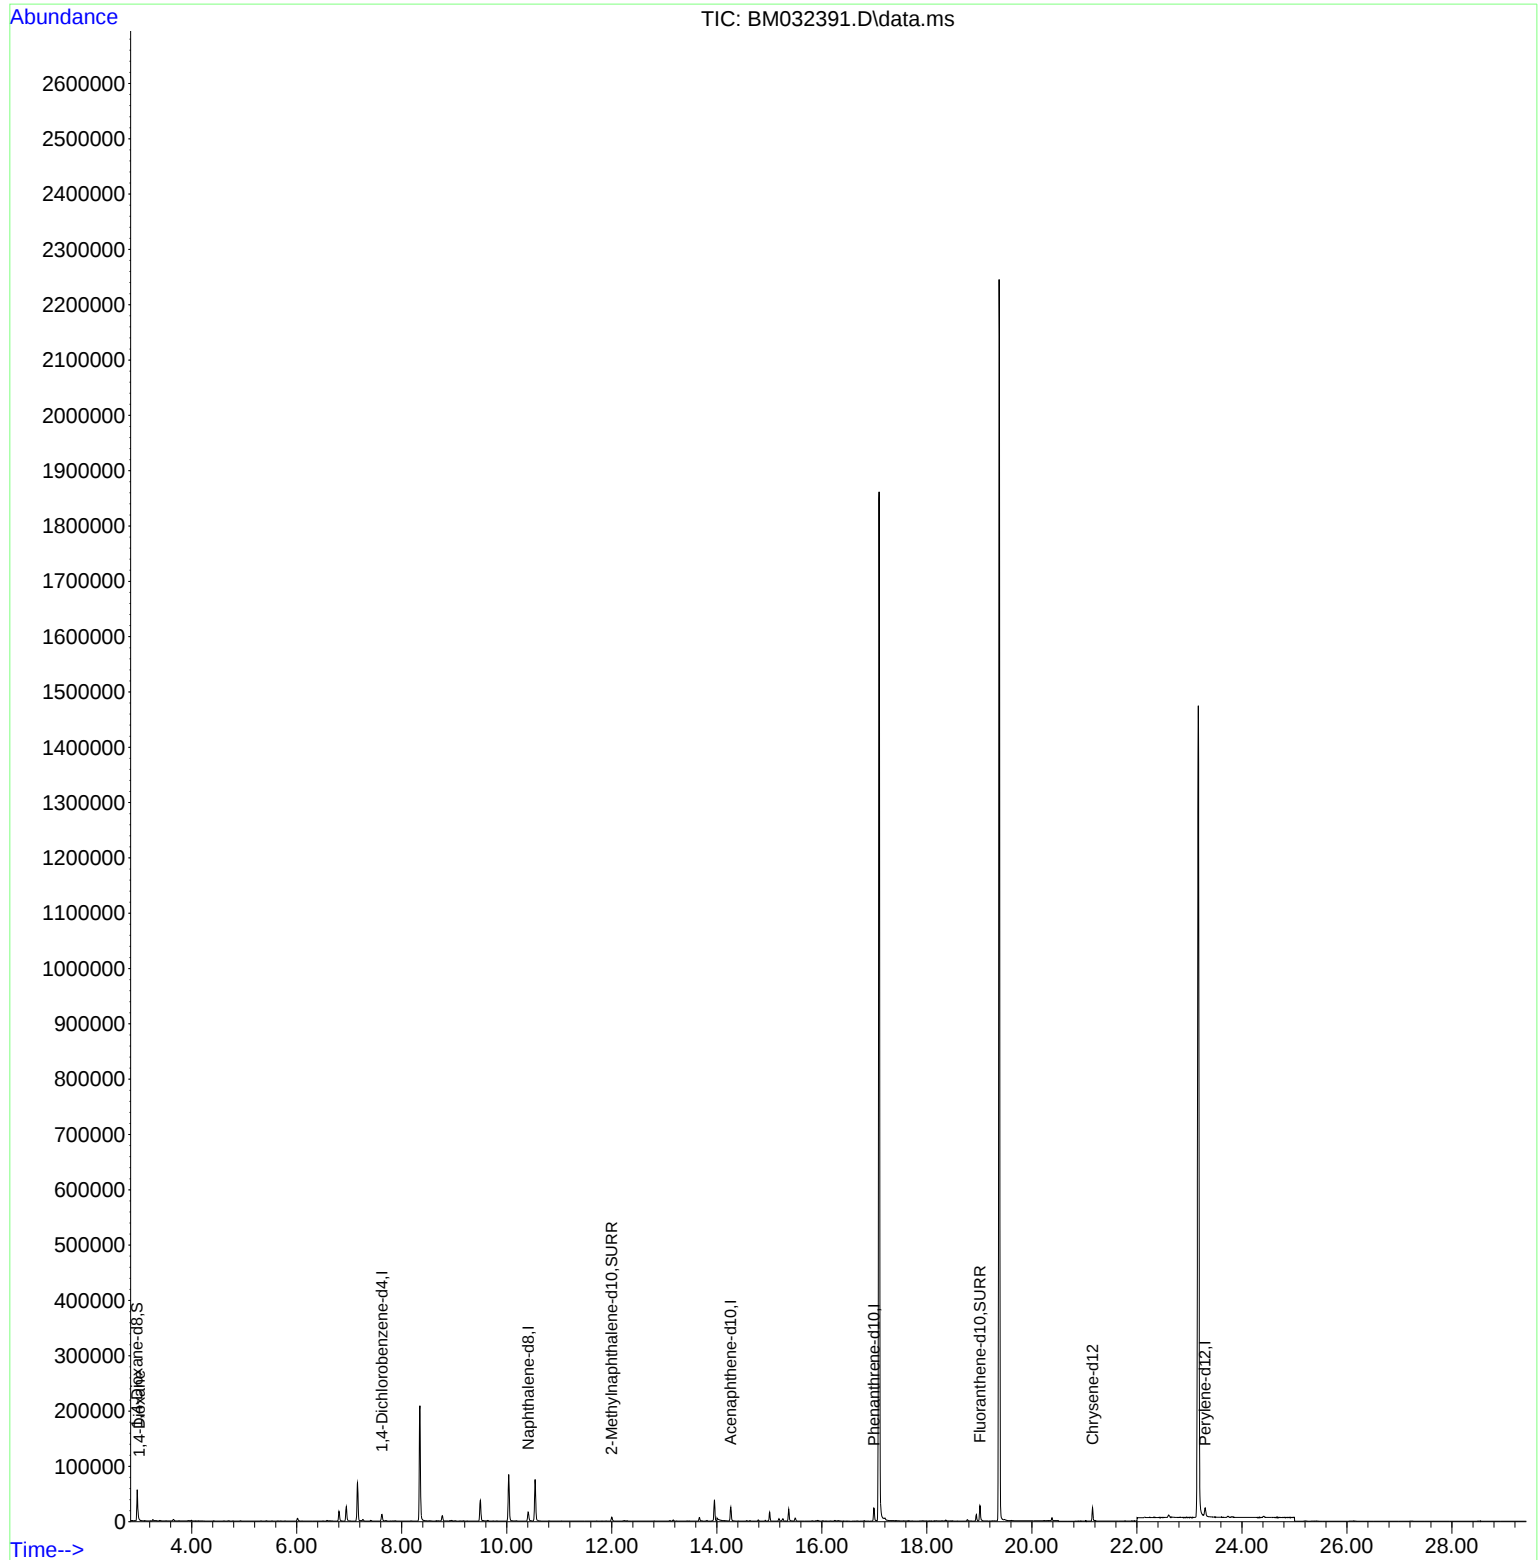


Abundance Scan 49 (3.003 min): BM032384.D\data.ms (-40)

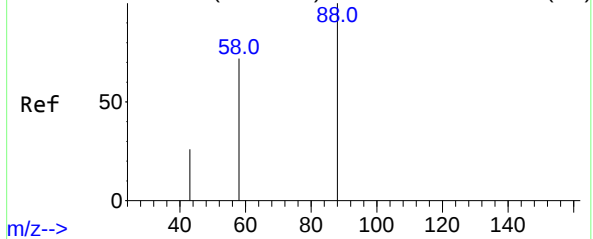

Abundance Scan 48 (3.000 min): BM032391.D\data.ms

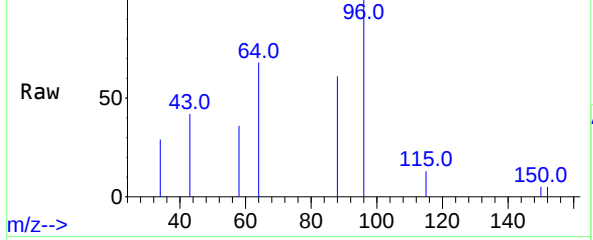


Abundance Scan 48 (3.000 min): BM032391.D\data.ms (-35)

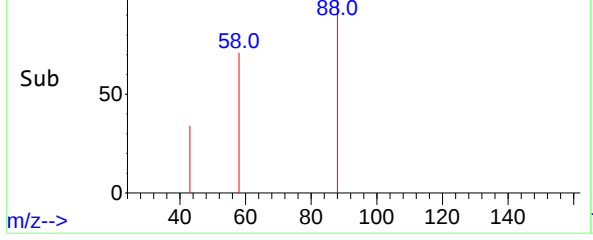

#2
1,4-Dioxane
Concen: 0.11 ng/ul
RT: 3.000 min Scan# 48
Delta R.T. -0.003 min
Lab File: BM032391.D
Acq: 08 Oct 2021 13:28

Tgt Ion:	88	Resp:	779
Ion	Ratio	Lower	Upper
88	100		
43	69.8	26.1	39.1#
58	60.0	50.2	75.2

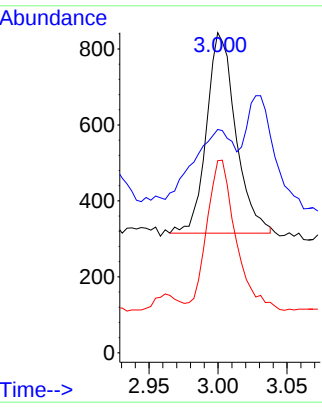

Instrument :
BNA_M
ClientSampleId :
C00S3