




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM100923\  
 Data File : BM042221.D  
 Acq On : 09 Oct 2023 12:28  
 Operator : MA/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 LabSampleId :  
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Oct 09 13:34:52 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM100223.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Oct 09 13:33:32 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/10/2023  
 Supervised By :mohammad ahmed 10/11/2023

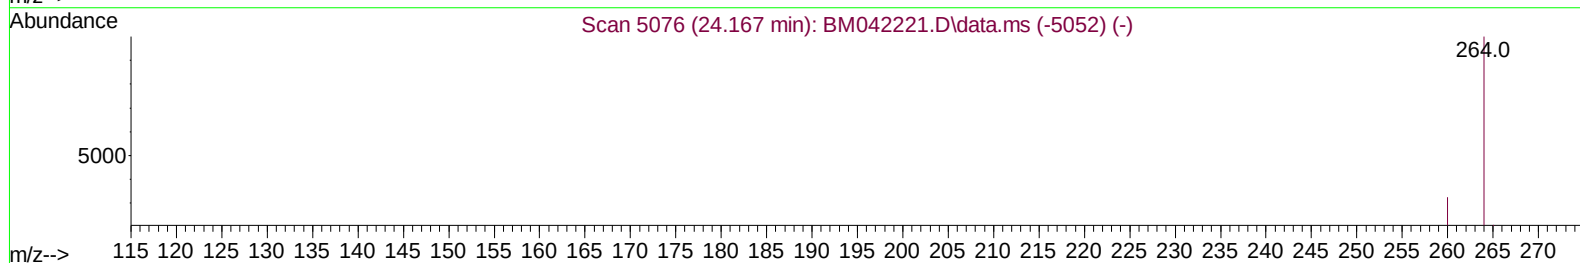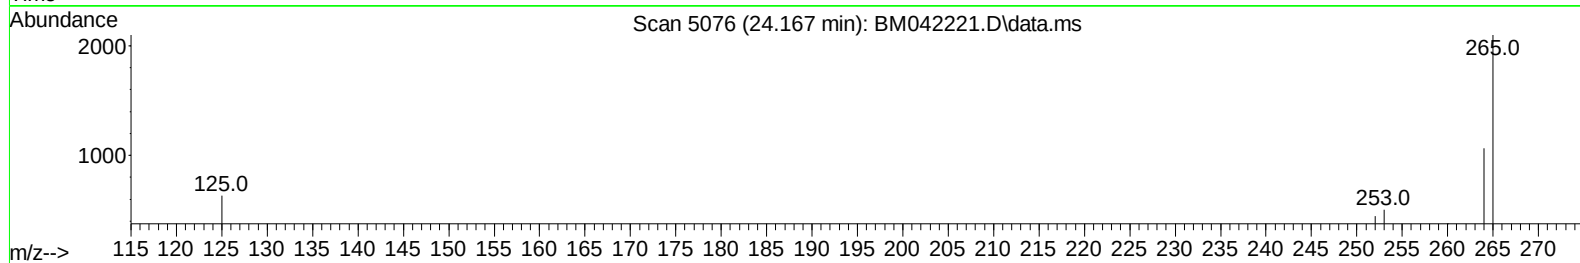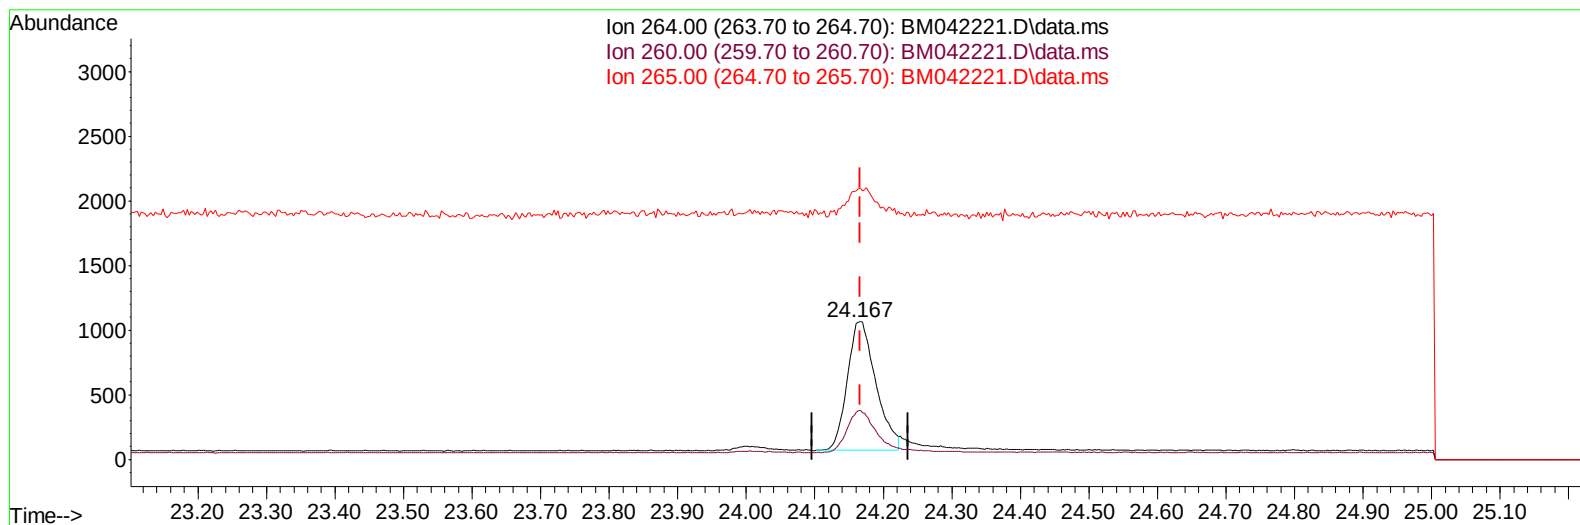

TIC: BM042221.D\data.ms

**(23) Perylene-d12 (I)**

24.167min ( 0.000) 0.40 ng/u1

response 2875

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 264.00 | 100.00 | 100.00  |
| 260.00 | 30.70  | 35.37   |
| 265.00 | 133.30 | 196.72# |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM100923\  
 Data File : BM042221.D  
 Acq On : 09 Oct 2023 12:28  
 Operator : MA/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 LabSampleId :  
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Oct 09 13:34:52 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM100223.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Oct 09 13:33:32 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/10/2023  
 Supervised By :mohammad ahmed 10/11/2023

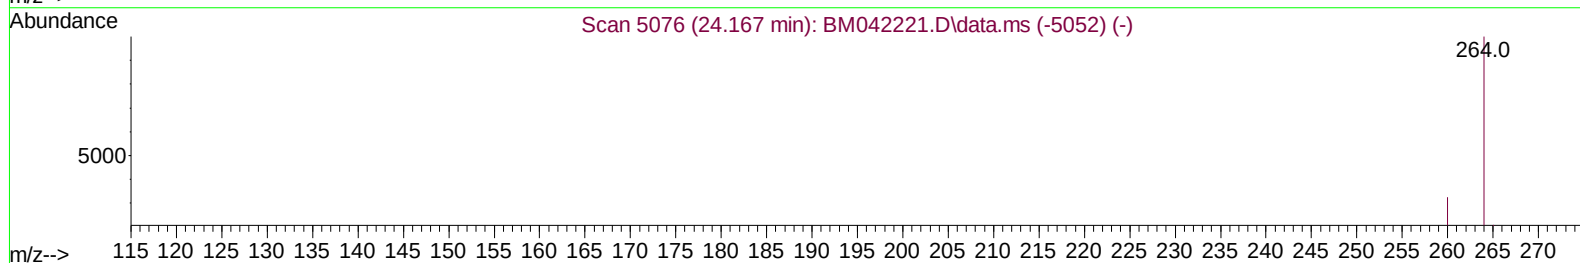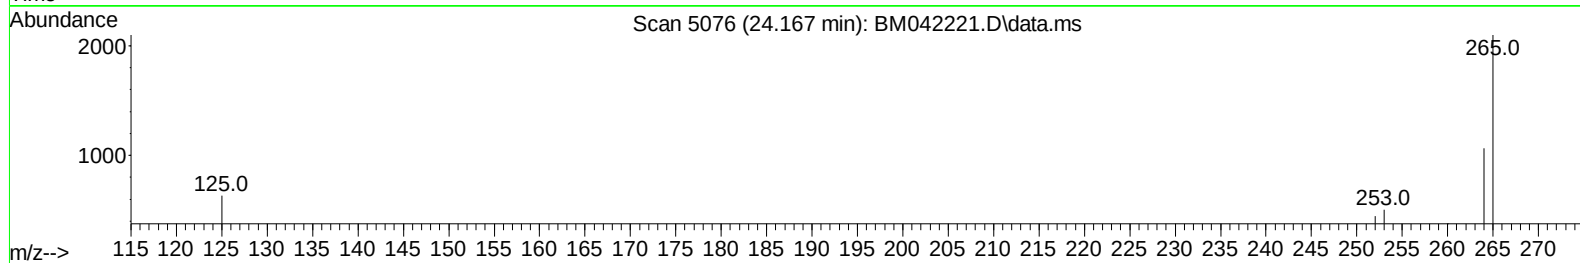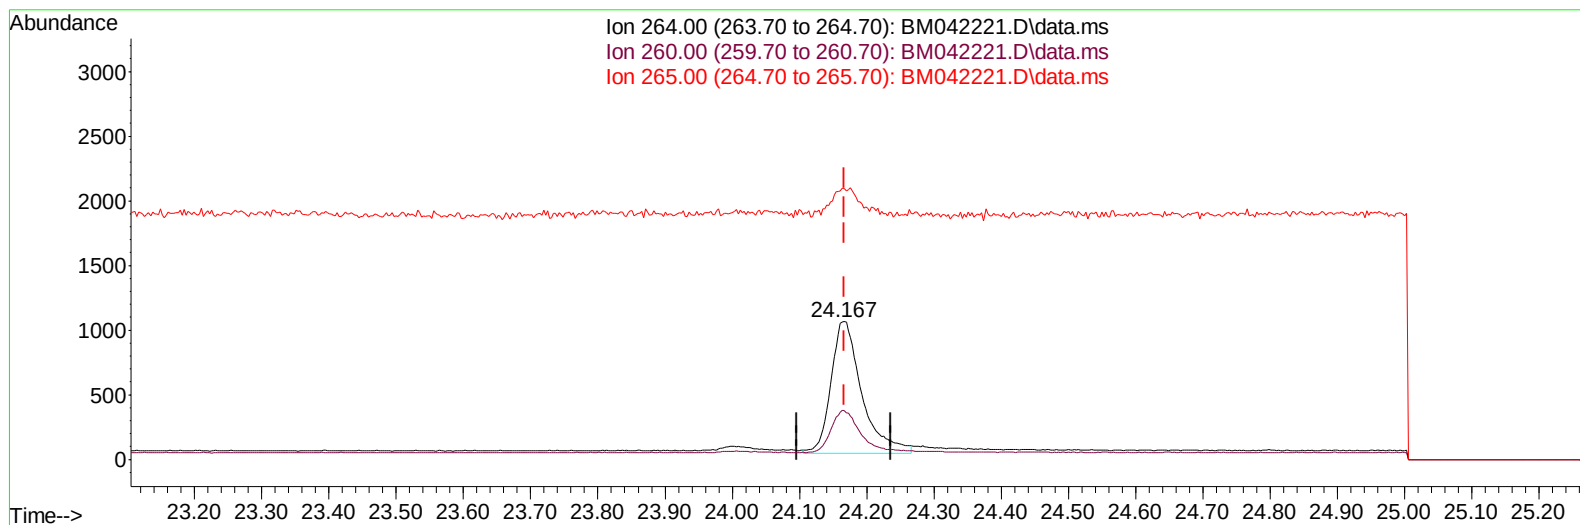

TIC: BM042221.D\data.ms

**(23) Perylene-d12 (I)**

24.167min ( 0.000) 0.40 ng/ul m

response 3250

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 264.00 | 100.00 | 100.00  |
| 260.00 | 30.70  | 35.37   |
| 265.00 | 133.30 | 196.72# |
| 0.00   | 0.00   | 0.00    |