

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042226.D
 Acq On : 09 Oct 2023 15:30
 Operator : MA/JU
 Sample : 04744-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH579

Quant Time: Oct 09 16:12:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 13:33:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	3195	0.400	ng/u1	0.00
4) Naphthalene-d8	10.878	136	8209	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.694	164	3357	0.400	ng/u1	#-0.02
13) Phenanthrene-d10	17.447	188	7040	0.400	ng/u1	#-0.03
17) Chrysene-d12	21.635	240	3111	0.400	ng/u1	#-0.02
23) Perylene-d12	24.134	264	3358	0.400	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	18778	4.413	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.456	152	2172	0.193	ng/u1	-0.01
18) Fluoranthene-d10	19.469	212	4515	0.387	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	725	0.163	ng/u1	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042226.D
Acq On : 09 Oct 2023 15:30
Operator : MA/JU
Sample : 04744-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH579


Quant Time: Oct 09 16:12:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 13:33:32 2023
Response via : Initial Calibration

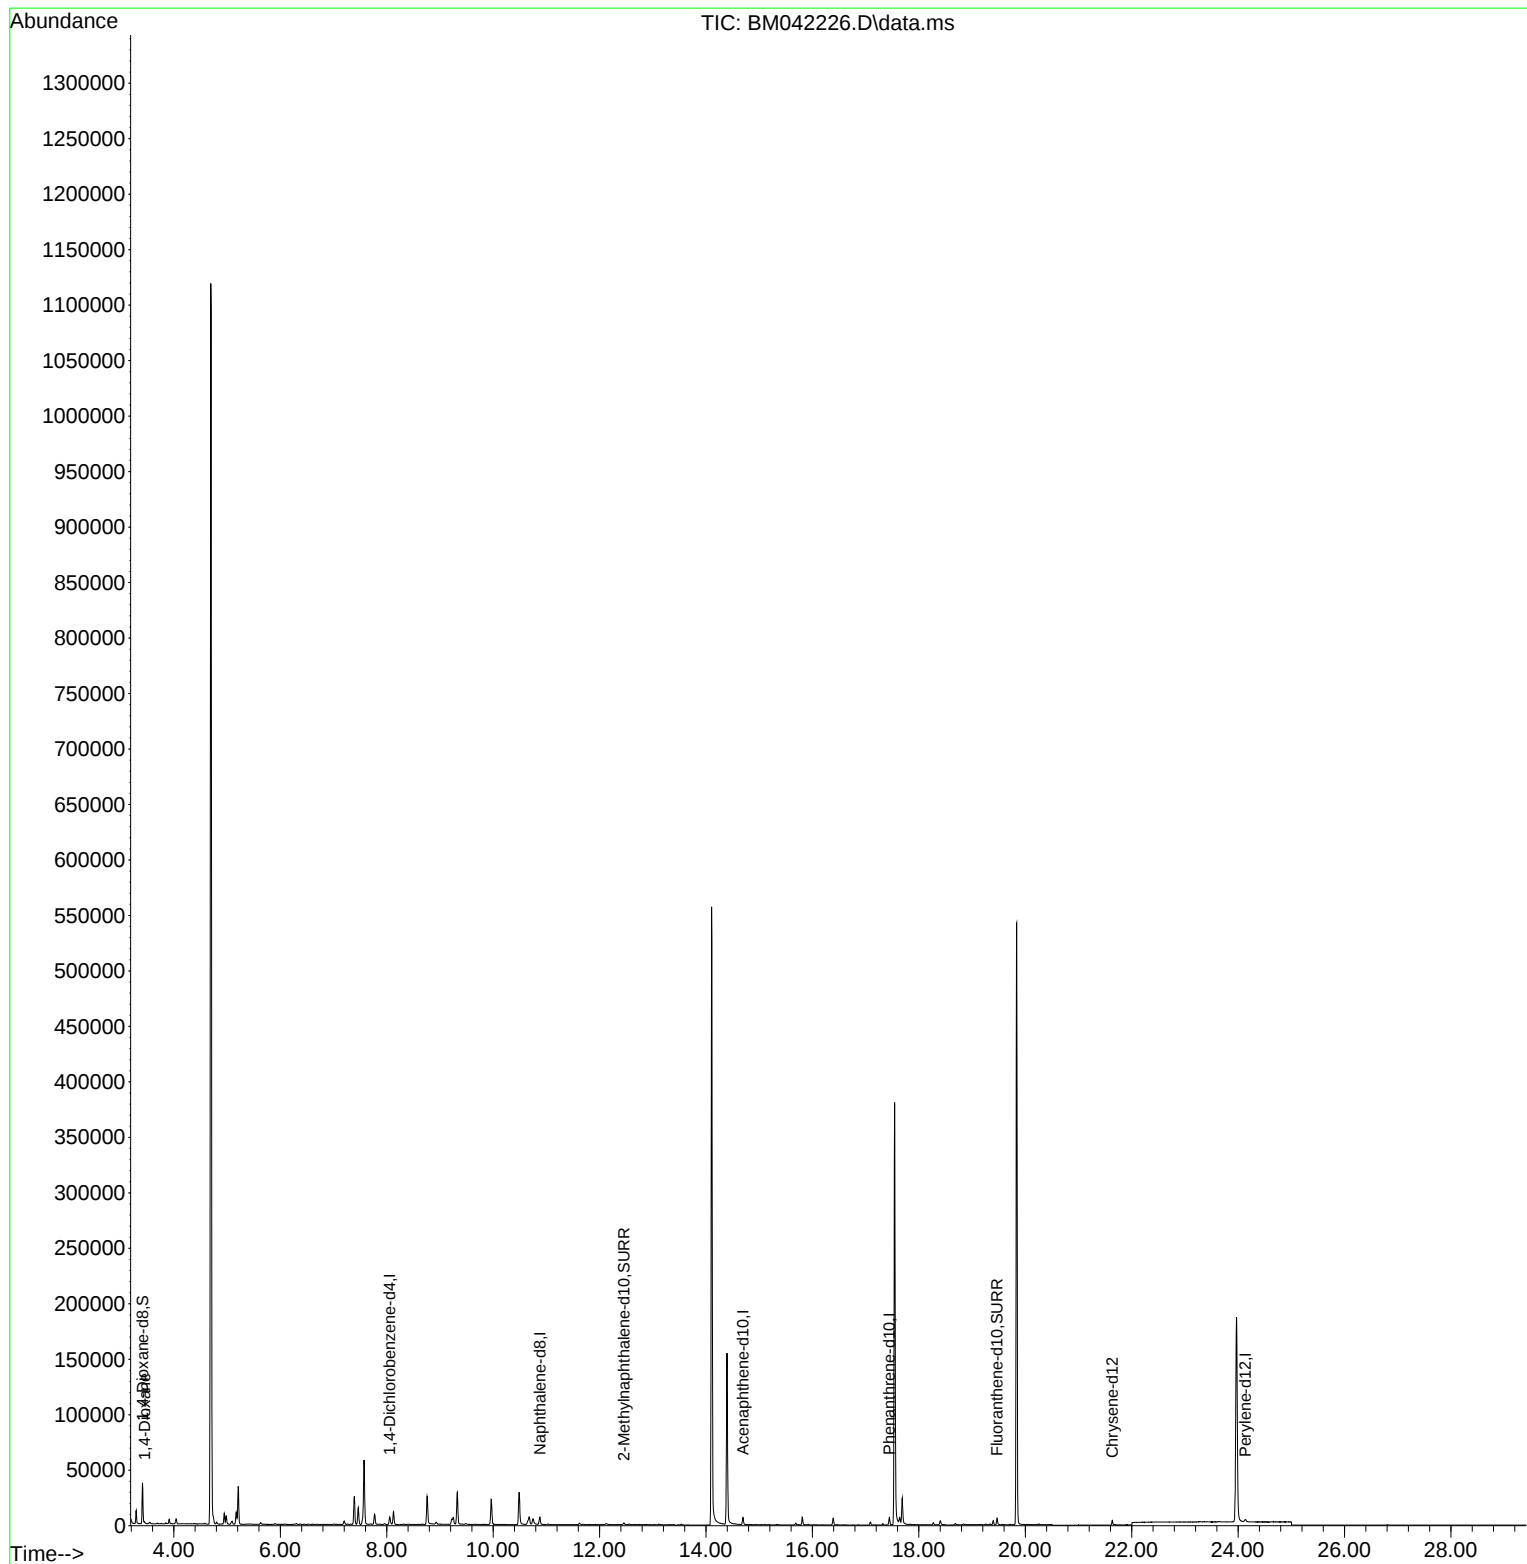


Abundance Scan 64 (3.452 min): BM042221.D\data.ms (-53)

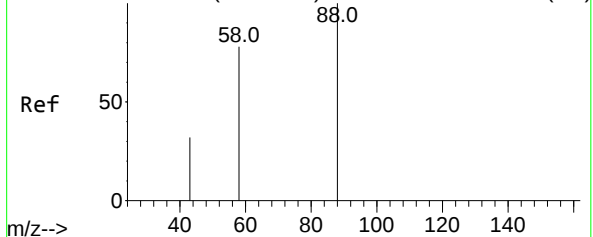

Abundance Scan 63 (3.448 min): BM042226.D\data.ms

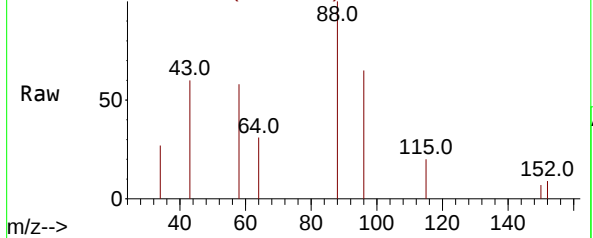

Abundance Scan 63 (3.448 min): BM042226.D\data.ms (-50)

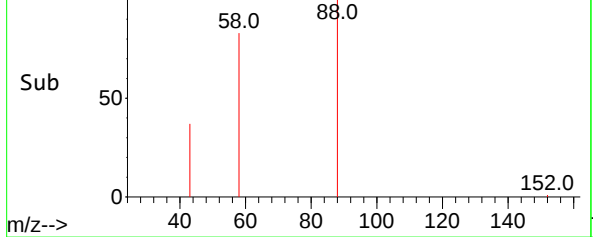

#2
1,4-Dioxane
Concen: 0.163 ng/ul
RT: 3.448 min Scan# 61
Delta R.T. -0.004 min
Lab File: BM042226.D
Acq: 09 Oct 2023 15:30

Instrument :
BNA_M
ClientSampleId :
BH579

Tgt Ion: 88	Resp: 725
Ion Ratio	Lower Upper
88	100
43	60.1 52.1 78.1
58	57.8 53.8 80.6

