

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042228.D
 Acq On : 09 Oct 2023 16:43
 Operator : MA/JU
 Sample : 04744-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH582

Quant Time: Oct 09 17:14:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 13:33:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	3065	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	7941	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.694	164	3244	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.447	188	6951	0.400	ng/ul	#-0.03
17) Chrysene-d12	21.635	240	3079	0.400	ng/ul	#-0.02
23) Perylene-d12	24.132	264	3229	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	16148	3.956	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	2067	0.190	ng/ul	-0.01
18) Fluoranthene-d10	19.468	212	5238	0.453	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	546	0.128	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042228.D
Acq On : 09 Oct 2023 16:43
Operator : MA/JU
Sample : 04744-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH582

Quant Time: Oct 09 17:14:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 13:33:32 2023
Response via : Initial Calibration

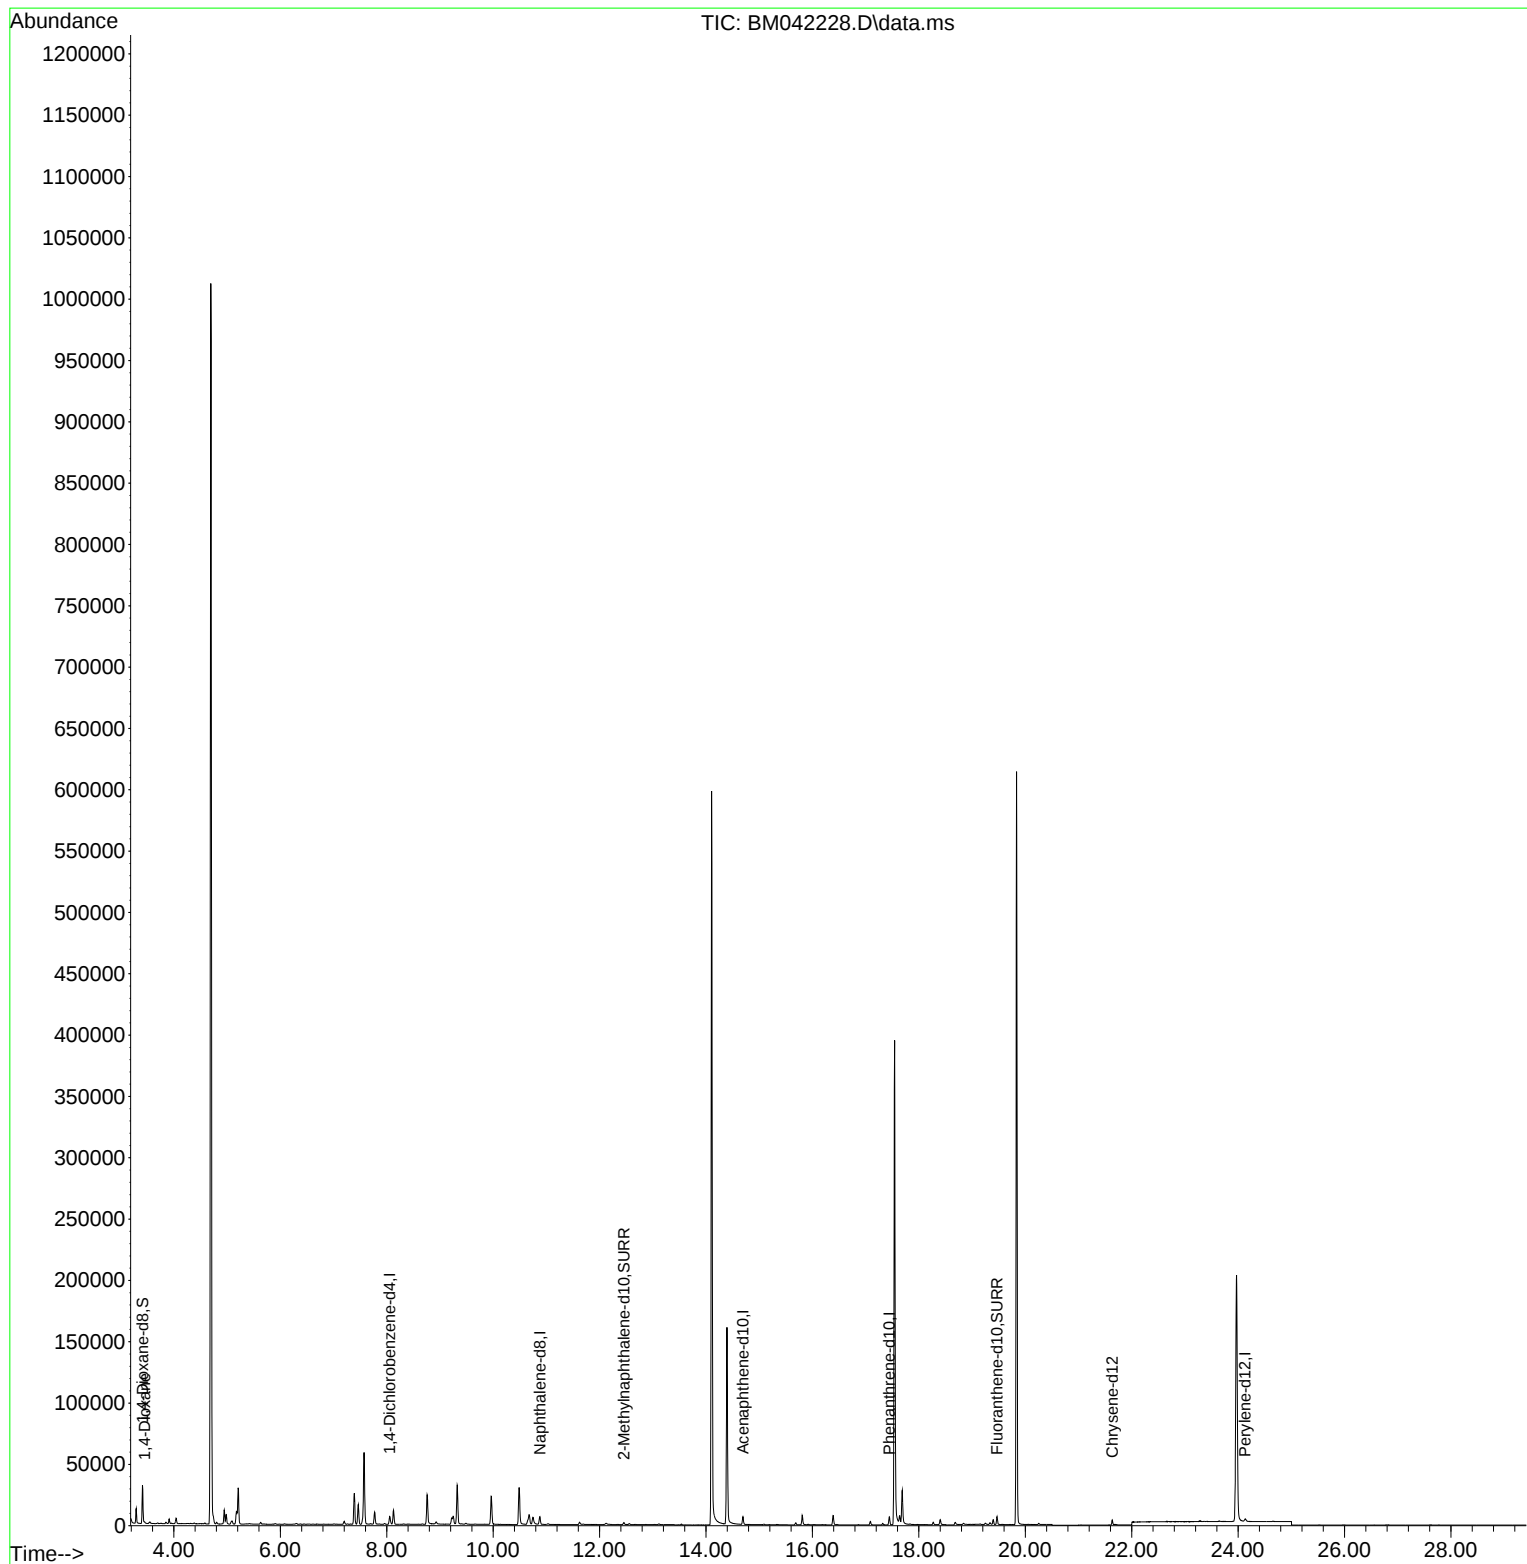

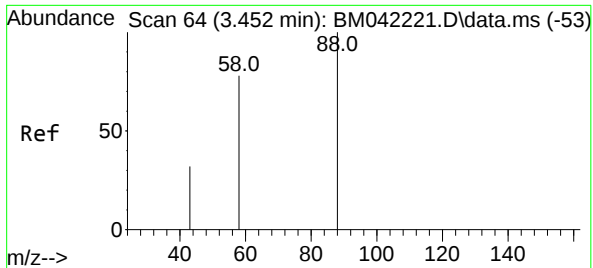

#2
 1,4-Dioxane
 Concen: 0.128 ng/ul
 RT: 3.452 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BM042228.D
 Acq: 09 Oct 2023 16:43

Instrument :
 BNA_M
 ClientSampleId :
 BH582

Tgt Ion:	88	Resp:	546
Ion	Ratio	Lower	Upper
88	100		
43	62.7	52.1	78.1
58	48.9	53.8	80.6

