

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042235.D
 Acq On : 09 Oct 2023 21:58
 Operator : MA/JU
 Sample : 04654-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHB7

Quant Time: Oct 10 00:01:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 23:59:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4856	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	13434	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.694	164	5684	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.443	188	11958	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.632	240	4347	0.400	ng/ul	# 0.00
23) Perylene-d12	24.132	264	4364	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	22683	3.508	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	4982	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.468	212	7400	0.453	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.448	88	3987	0.590	ng/ul#	83
14) Pentachlorophenol	17.080	266	145	0.027	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042235.D
Acq On : 09 Oct 2023 21:58
Operator : MA/JU
Sample : 04654-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHB7

Quant Time: Oct 10 00:01:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 23:59:28 2023
Response via : Initial Calibration




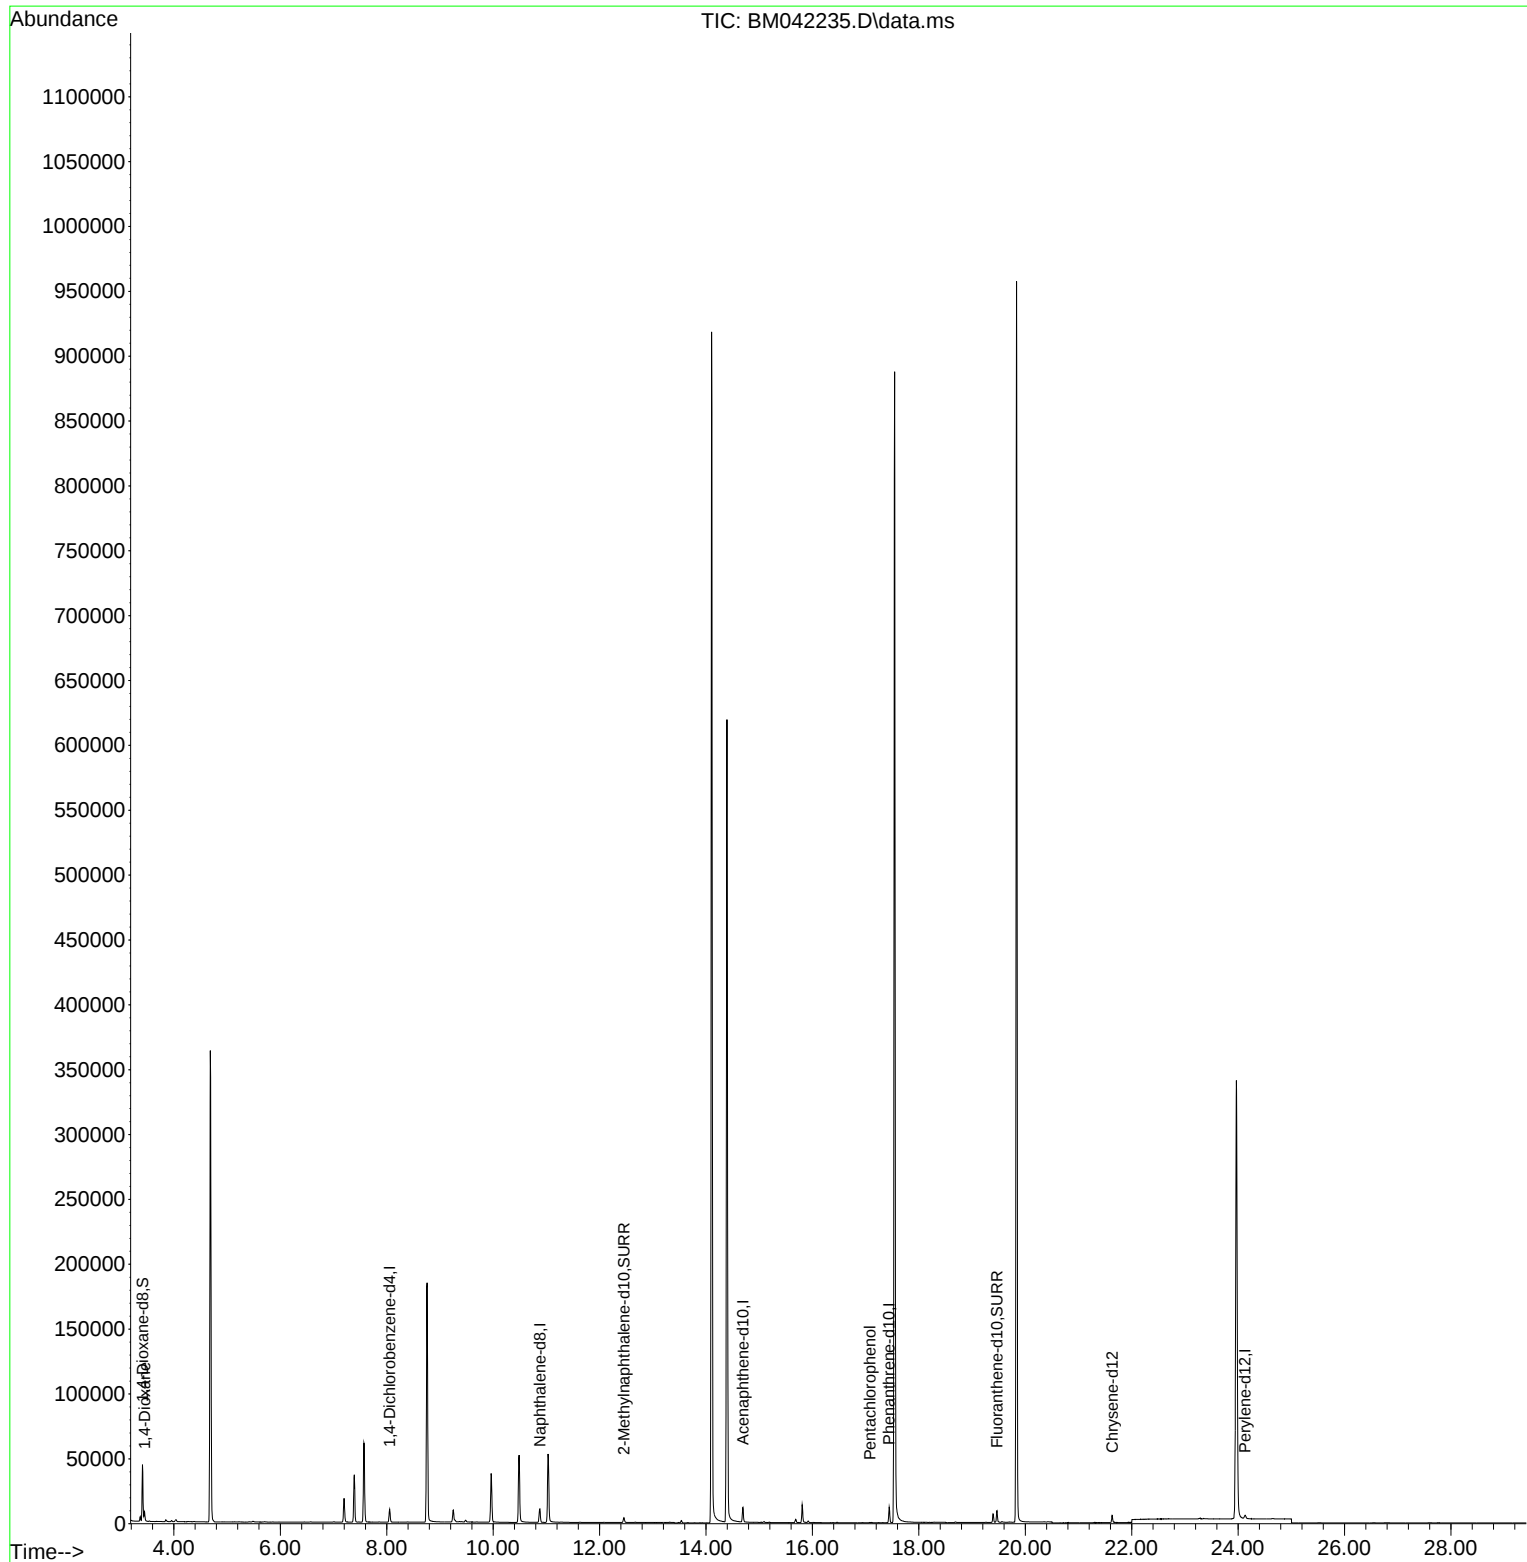


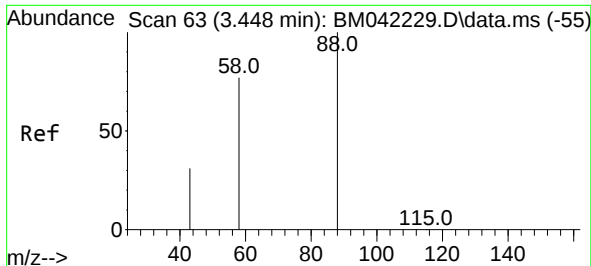

#2
 1,4-Dioxane
 Concen: 0.590 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM042235.D
 Acq: 09 Oct 2023 21:58

Instrument :
 BNA_M
 ClientSampleId :
 BBHB7

Tgt Ion: 88 Resp: 3987
 Ion Ratio Lower Upper
 88 100
 43 45.5 52.1 78.1#
 58 75.5 53.8 80.6

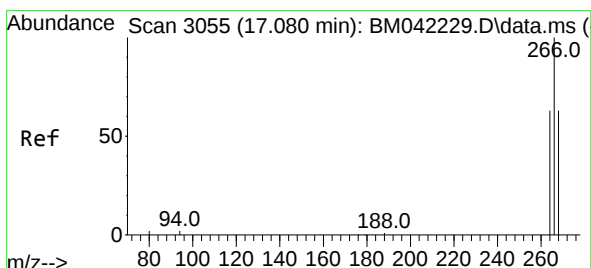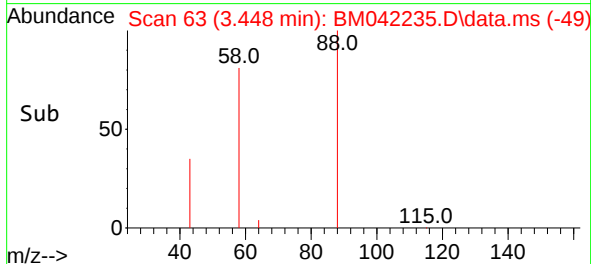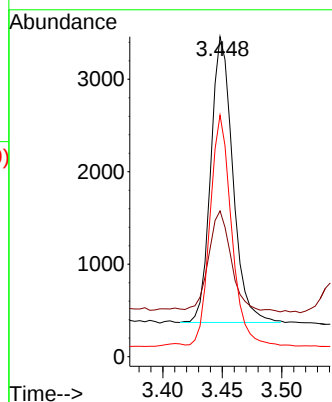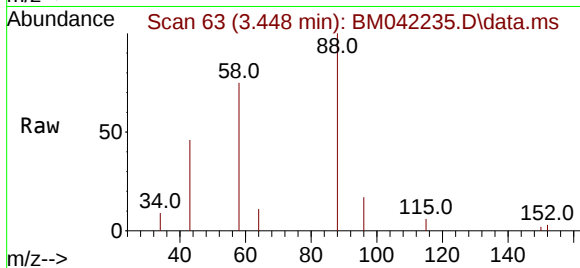

#14
 Pentachlorophenol
 Concen: 0.027 ng/ul
 RT: 17.080 min Scan# 3055
 Delta R.T. -0.000 min
 Lab File: BM042235.D
 Acq: 09 Oct 2023 21:58

Tgt Ion: 266 Resp: 145
 Ion Ratio Lower Upper
 266 100
 264 64.8 51.1 76.7
 268 73.1 52.1 78.1

