

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042237.D
 Acq On : 09 Oct 2023 23:11
 Operator : MA/JU
 Sample : 04654-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHD1

Quant Time: Oct 10 00:02:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 23:59:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4097	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	10435	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.694	164	4520	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.443	188	9191	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.629	240	4402	0.400	ng/ul	# 0.00
23) Perylene-d12	24.129	264	4867	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	19970	3.660	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	4445	0.311	ng/ul	0.00
18) Fluoranthene-d10	19.468	212	6648	0.402	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.448	88	3461	0.607	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042237.D
Acq On : 09 Oct 2023 23:11
Operator : MA/JU
Sample : 04654-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHD1

Quant Time: Oct 10 00:02:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 23:59:28 2023
Response via : Initial Calibration

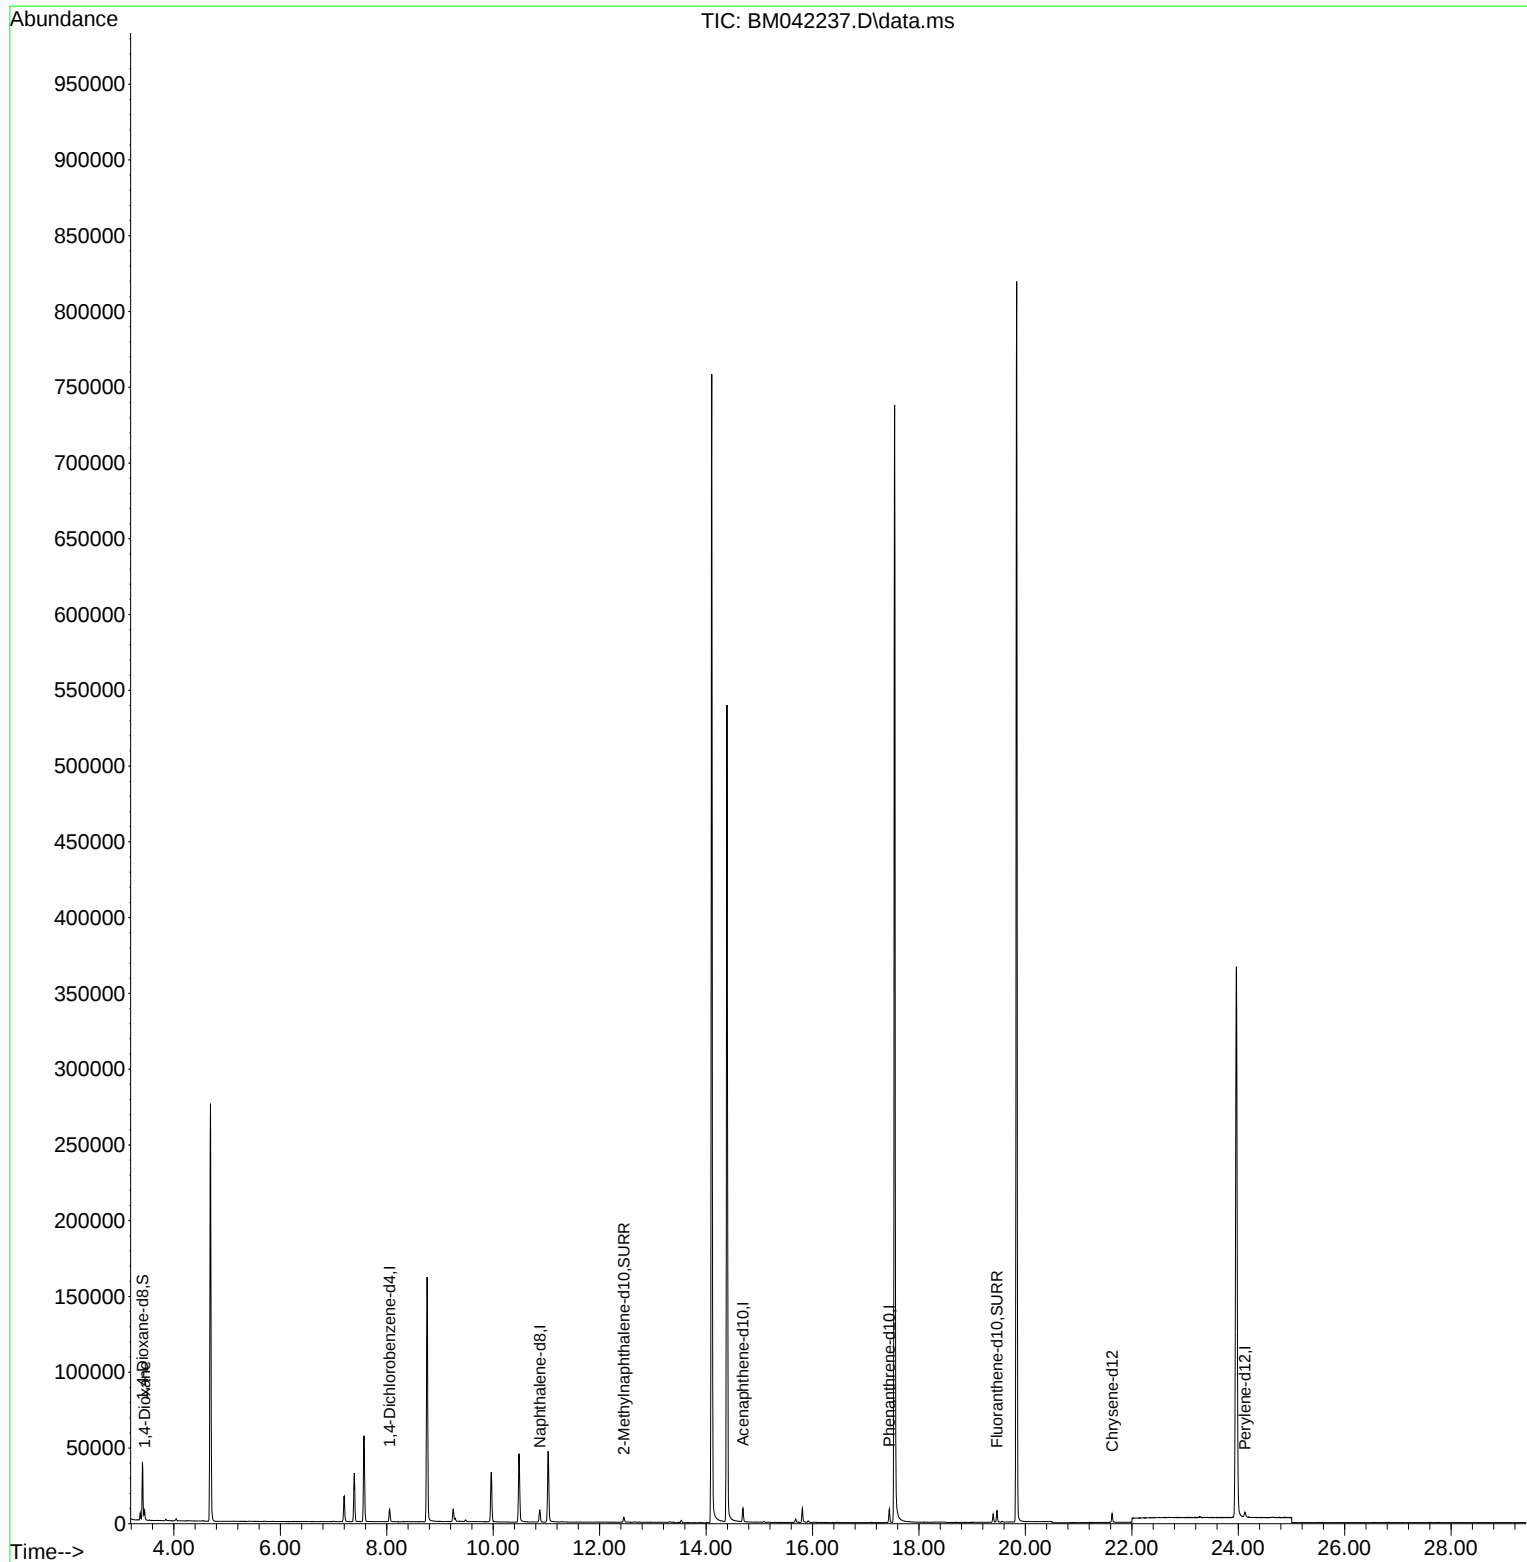

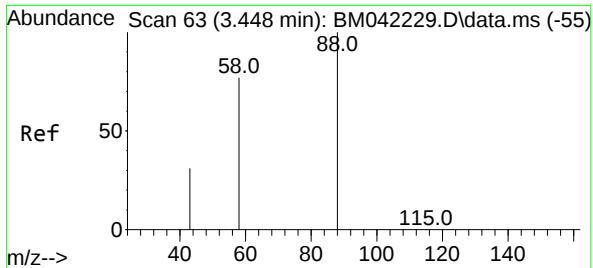

#2
 1,4-Dioxane
 Concen: 0.607 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM042237.D
 Acq: 09 Oct 2023 23:11

Instrument :
 BNA_M
 ClientSampleId :
 BBHD1

Tgt Ion: 88 Resp: 3461

Ion	Ratio	Lower	Upper
88	100		
43	55.0	52.1	78.1
58	76.1	53.8	80.6

