

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042238.D
 Acq On : 09 Oct 2023 23:47
 Operator : MA/JU
 Sample : 04654-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHZ9

Quant Time: Oct 10 00:18:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 23:59:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4386	0.400	ng/u1	0.00
4) Naphthalene-d8	10.872	136	11995	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.694	164	5311	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.443	188	11610	0.400	ng/u1	# 0.00
17) Chrysene-d12	21.629	240	5049	0.400	ng/u1	# 0.00
23) Perylene-d12	24.126	264	4764	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	24101	4.126	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.456	152	5752	0.350	ng/u1	0.00
18) Fluoranthene-d10	19.468	212	9063	0.478	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.448	88	1047	0.172	ng/u1	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042238.D
Acq On : 09 Oct 2023 23:47
Operator : MA/JU
Sample : 04654-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHZ9


Quant Time: Oct 10 00:18:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 23:59:28 2023
Response via : Initial Calibration

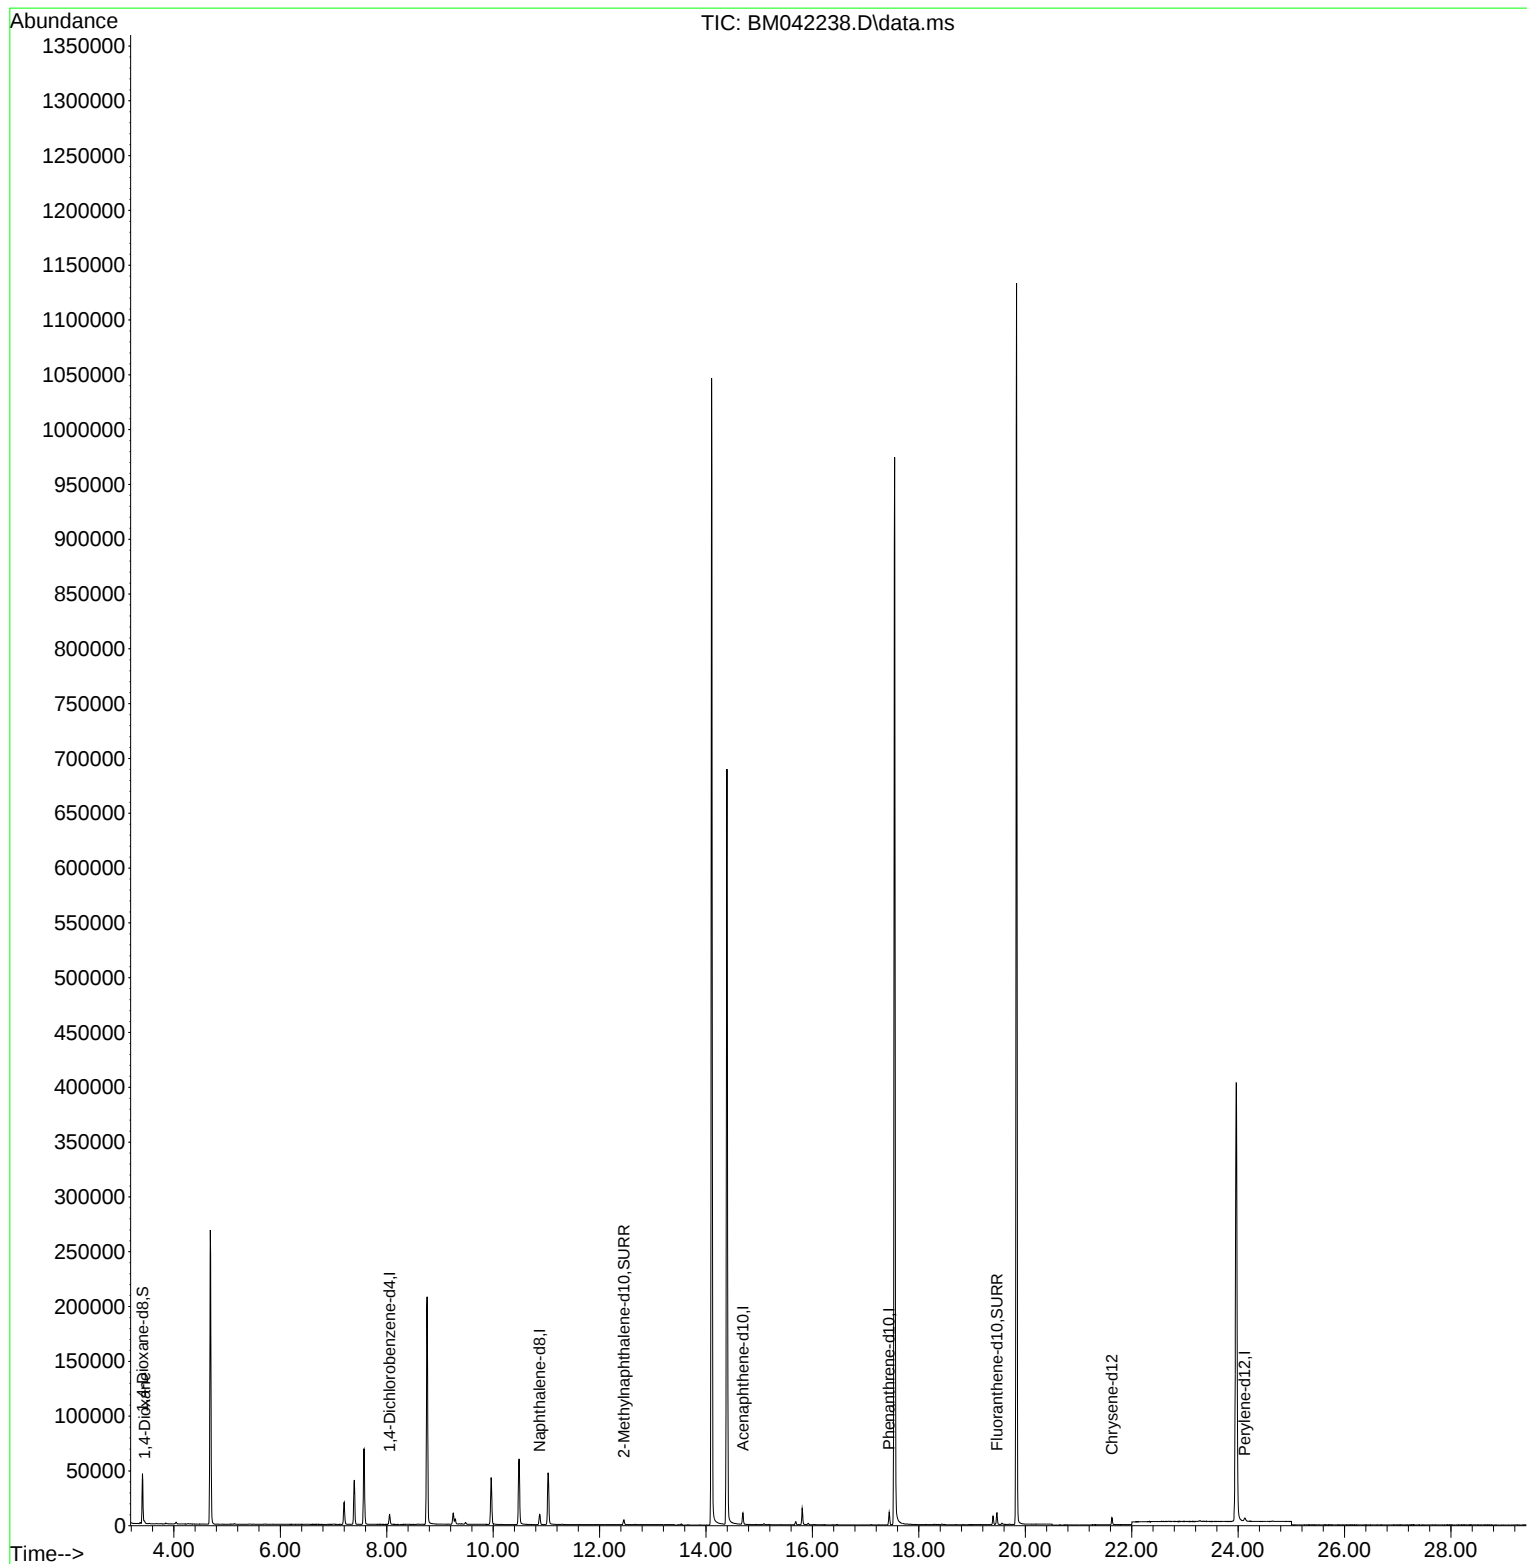

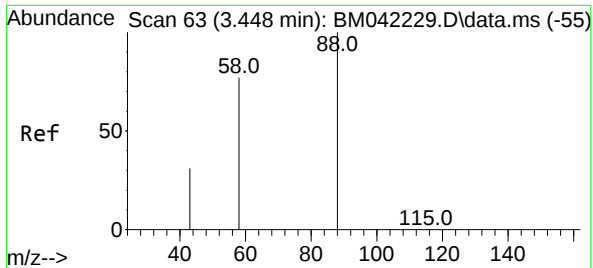

#2
 1,4-Dioxane
 Concen: 0.172 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM042238.D
 Acq: 09 Oct 2023 23:47

Instrument :
 BNA_M
 ClientSampleId :
 BBHZ9

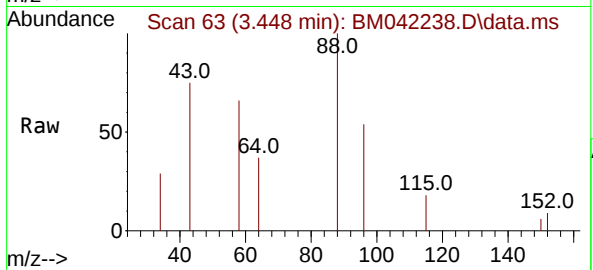

Tgt Ion:	88	Resp:	1047
Ion	Ratio	Lower	Upper
88	100		
43	75.3	52.1	78.1
58	66.4	53.8	80.6

