

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042241.D
 Acq On : 10 Oct 2023 01:35
 Operator : MA/JU
 Sample : 04654-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHC7

Quant Time: Oct 10 02:28:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 23:59:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4778	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	12925	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.694	164	5512	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.443	188	11368	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.629	240	4218	0.400	ng/ul	# 0.00
23) Perylene-d12	24.126	264	4369	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	25415	3.994	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	5746	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.468	212	8031	0.507	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	6031	0.908	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042241.D
Acq On : 10 Oct 2023 01:35
Operator : MA/JU
Sample : 04654-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHC7

Quant Time: Oct 10 02:28:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 23:59:28 2023
Response via : Initial Calibration

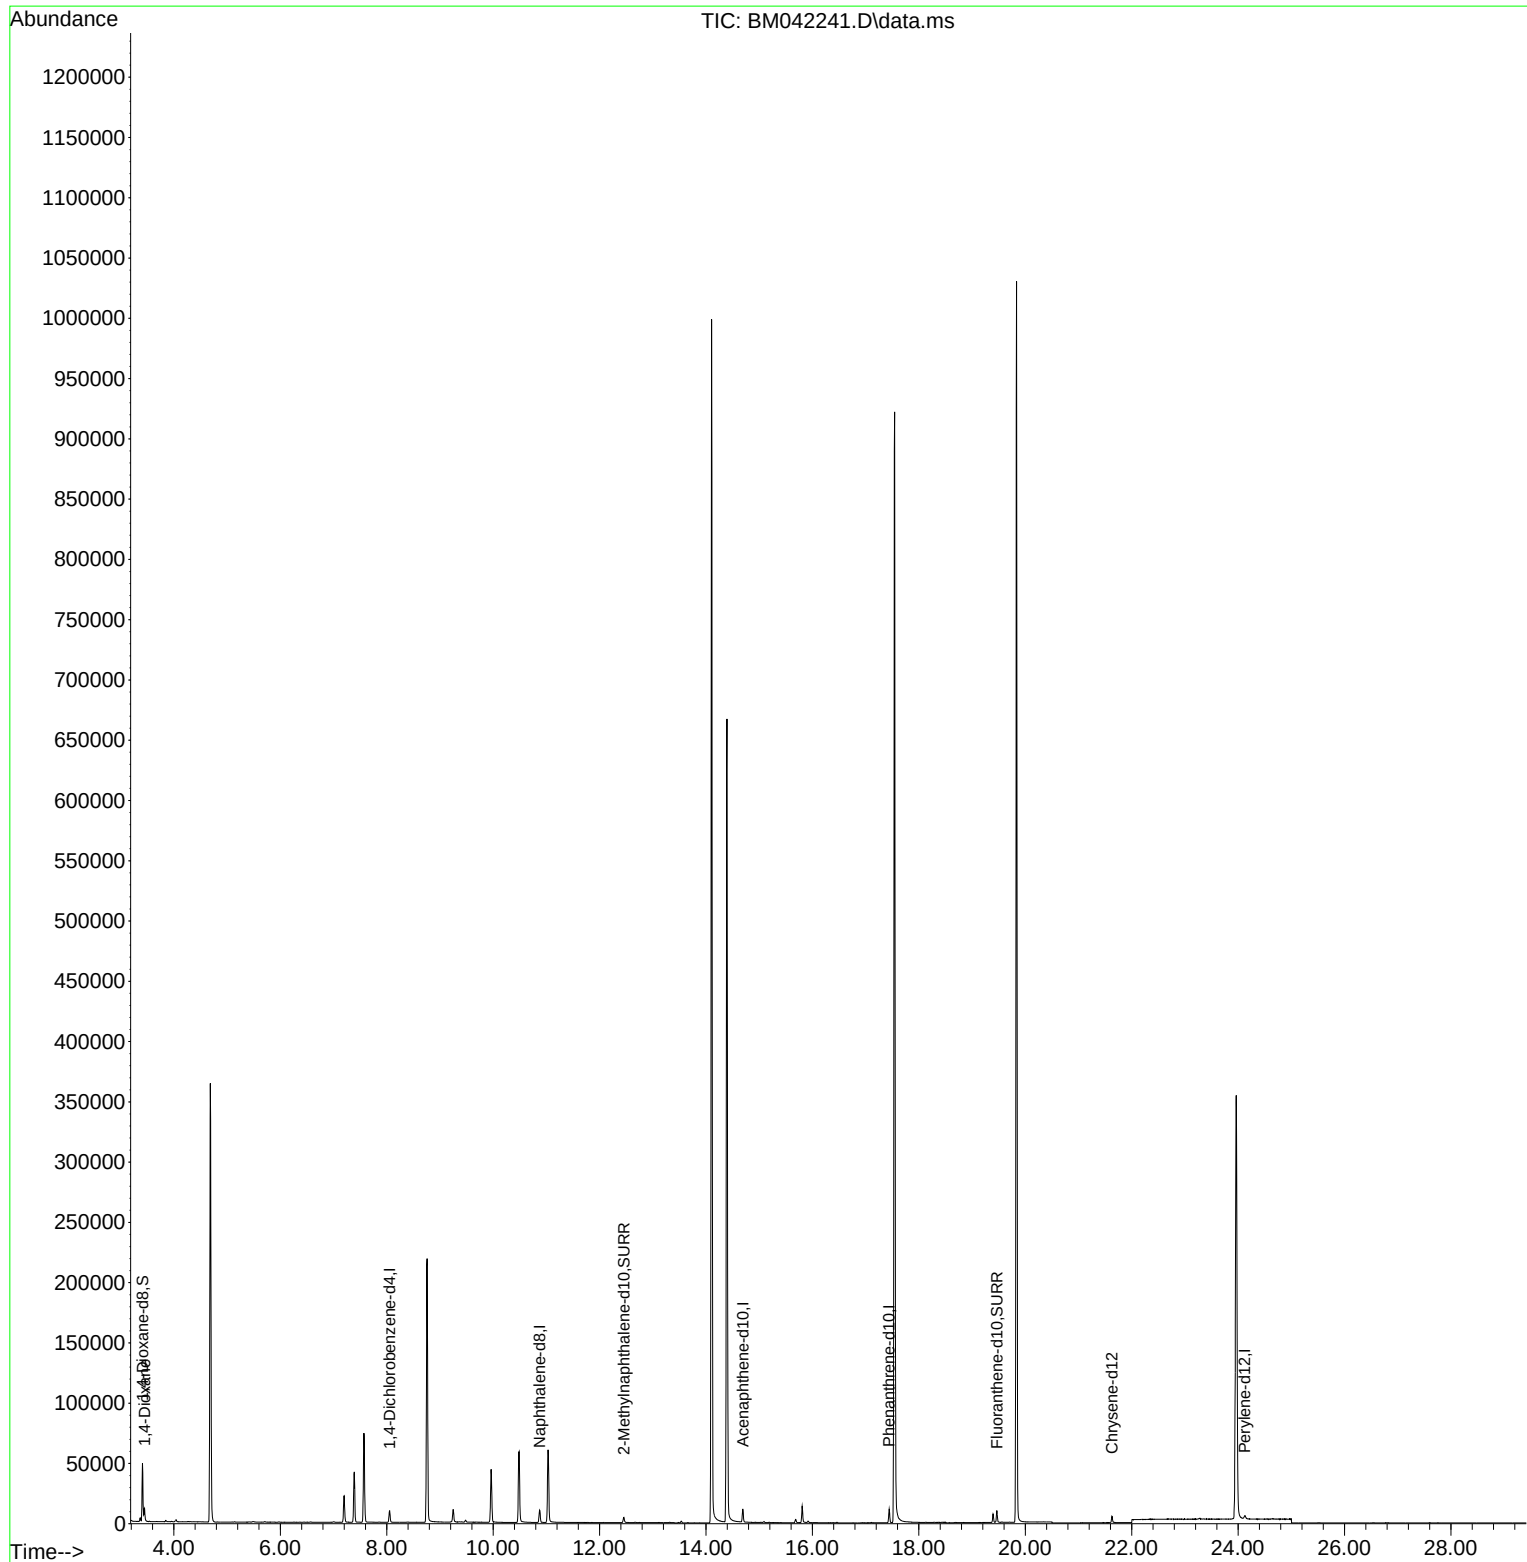

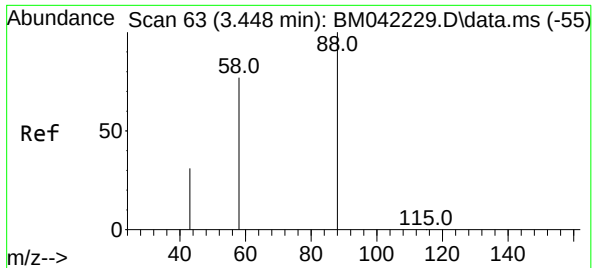

#2
 1,4-Dioxane
 Concen: 0.908 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM042241.D
 Acq: 10 Oct 2023 01:35

Instrument :
 BNA_M
 ClientSampleId :
 BBHC7

Tgt Ion:	88	Resp:	6031
Ion	Ratio	Lower	Upper
88	100		
43	41.1	52.1	78.1#
58	75.4	53.8	80.6

