

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
 Data File : BM042242.D
 Acq On : 10 Oct 2023 02:12
 Operator : MA/JU
 Sample : 04654-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK33

Quant Time: Oct 10 02:50:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 23:59:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4760	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	12486	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.694	164	4994	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.443	188	9780	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.629	240	4113	0.400	ng/ul	# 0.00
23) Perylene-d12	24.126	264	4596	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	24457	3.858	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	5672	0.331	ng/ul	0.00
18) Fluoranthene-d10	19.469	212	6632	0.429	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	4209	0.636	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100923\
Data File : BM042242.D
Acq On : 10 Oct 2023 02:12
Operator : MA/JU
Sample : 04654-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBK33

Quant Time: Oct 10 02:50:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 23:59:28 2023
Response via : Initial Calibration

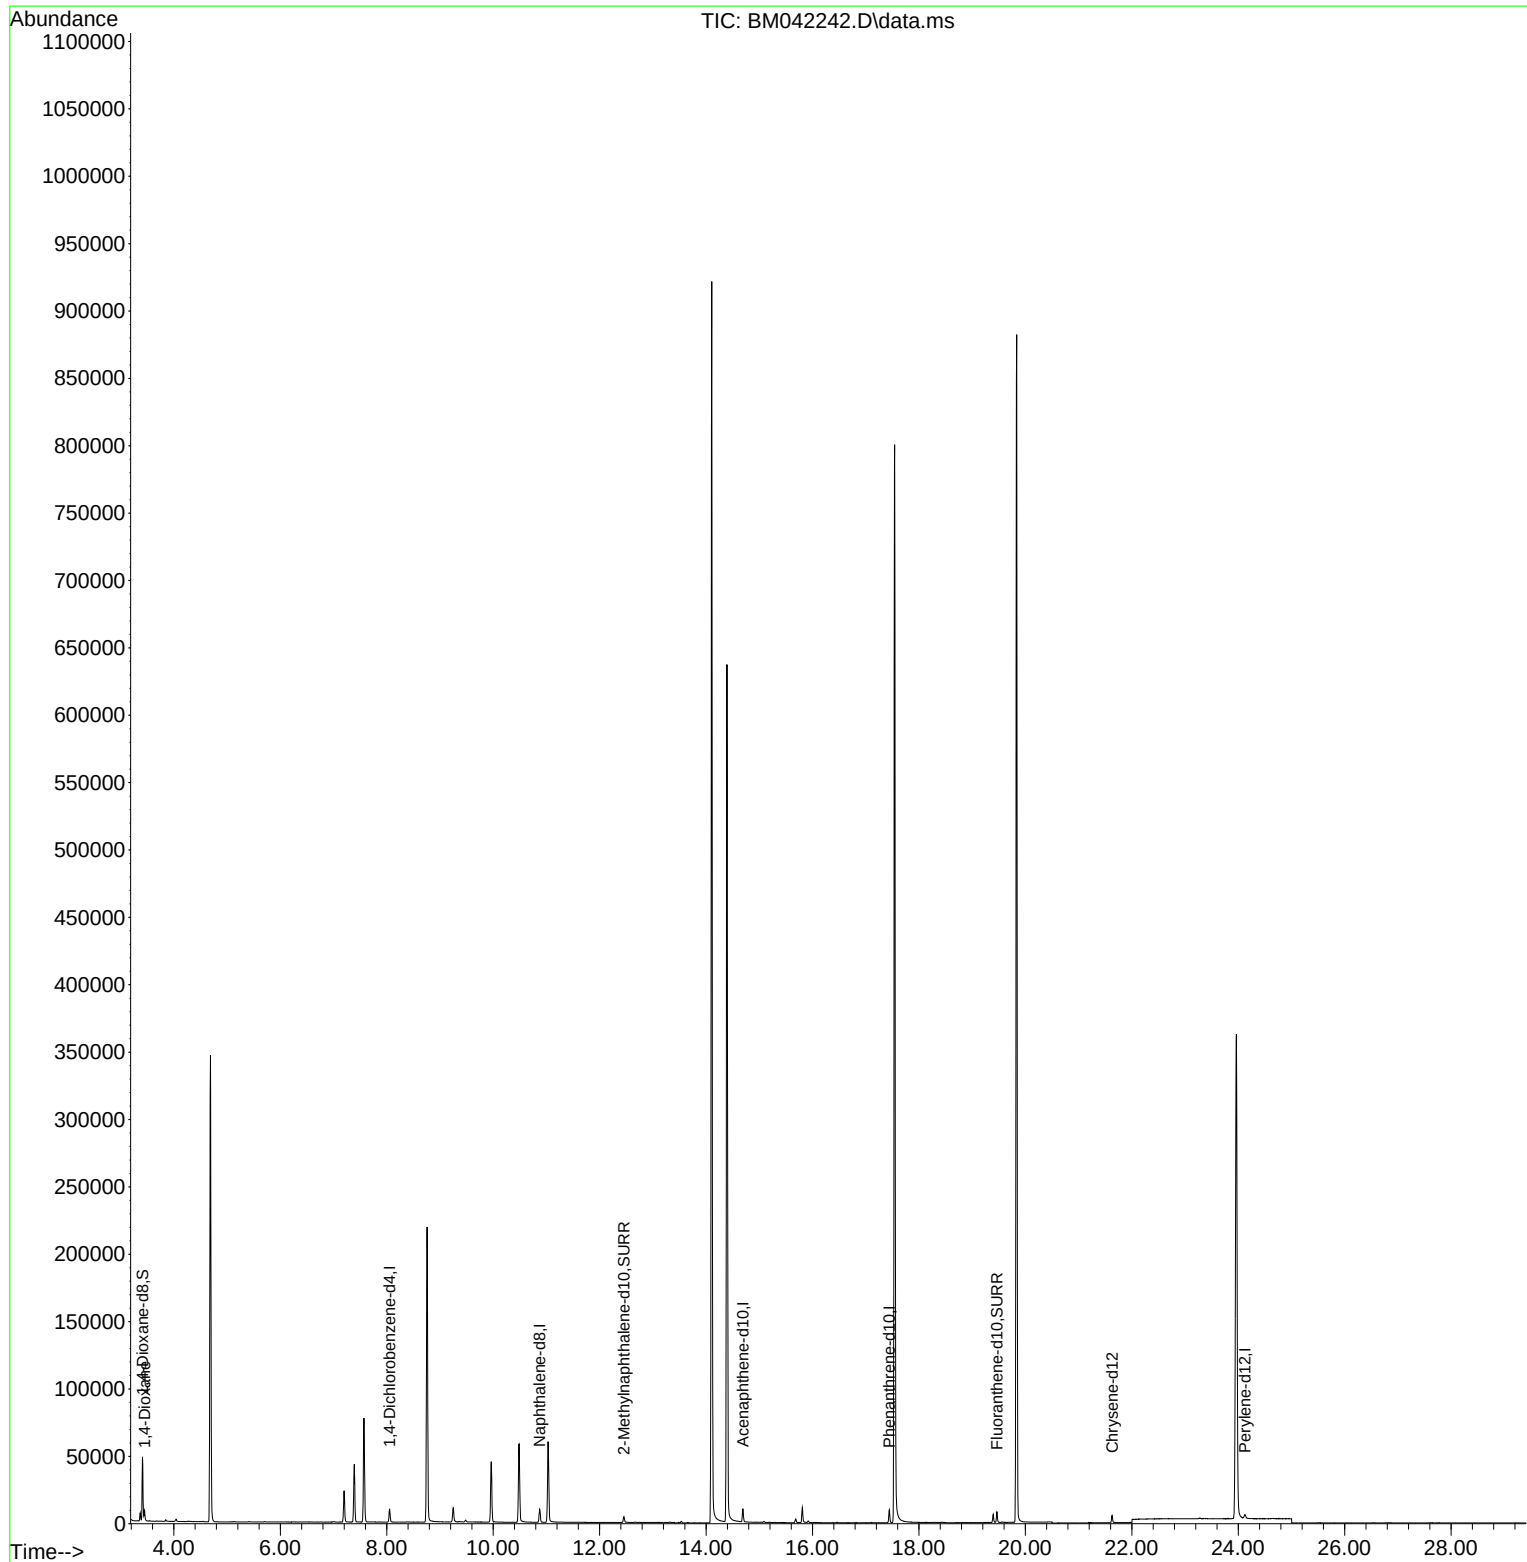

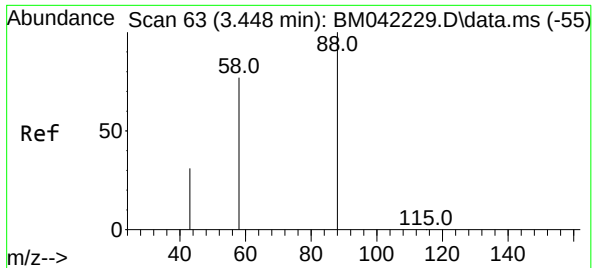

#2
 1,4-Dioxane
 Concen: 0.636 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BM042242.D
 Acq: 10 Oct 2023 02:12

Instrument :
 BNA_M
 ClientSampleId :
 BBK33

Tgt Ion:	88	Resp:	4209
Ion	Ratio	Lower	Upper
88	100		
43	42.3	52.1	78.1#
58	72.4	53.8	80.6

