

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042261.D
 Acq On : 10 Oct 2023 21:23
 Operator : MA/JU
 Sample : PB156057BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK057

Quant Time: Oct 11 00:47:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.026	152	4501	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	11771	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	4883	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	9305	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.594	240	3623	0.400	ng/ul	# 0.00
23) Perylene-d12	24.064	264	3548	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	43695	7.290	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	5386	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	6126	0.450	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.656	166	2345	0.089	ng/ul#	15
20) Pyrene	19.803	202	1762	0.060	ng/ul#	1
26) Benzo(a)pyrene	23.906	252	3066	0.170	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042261.D
Acq On : 10 Oct 2023 21:23
Operator : MA/JU
Sample : PB156057BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK057

Quant Time: Oct 11 00:47:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration




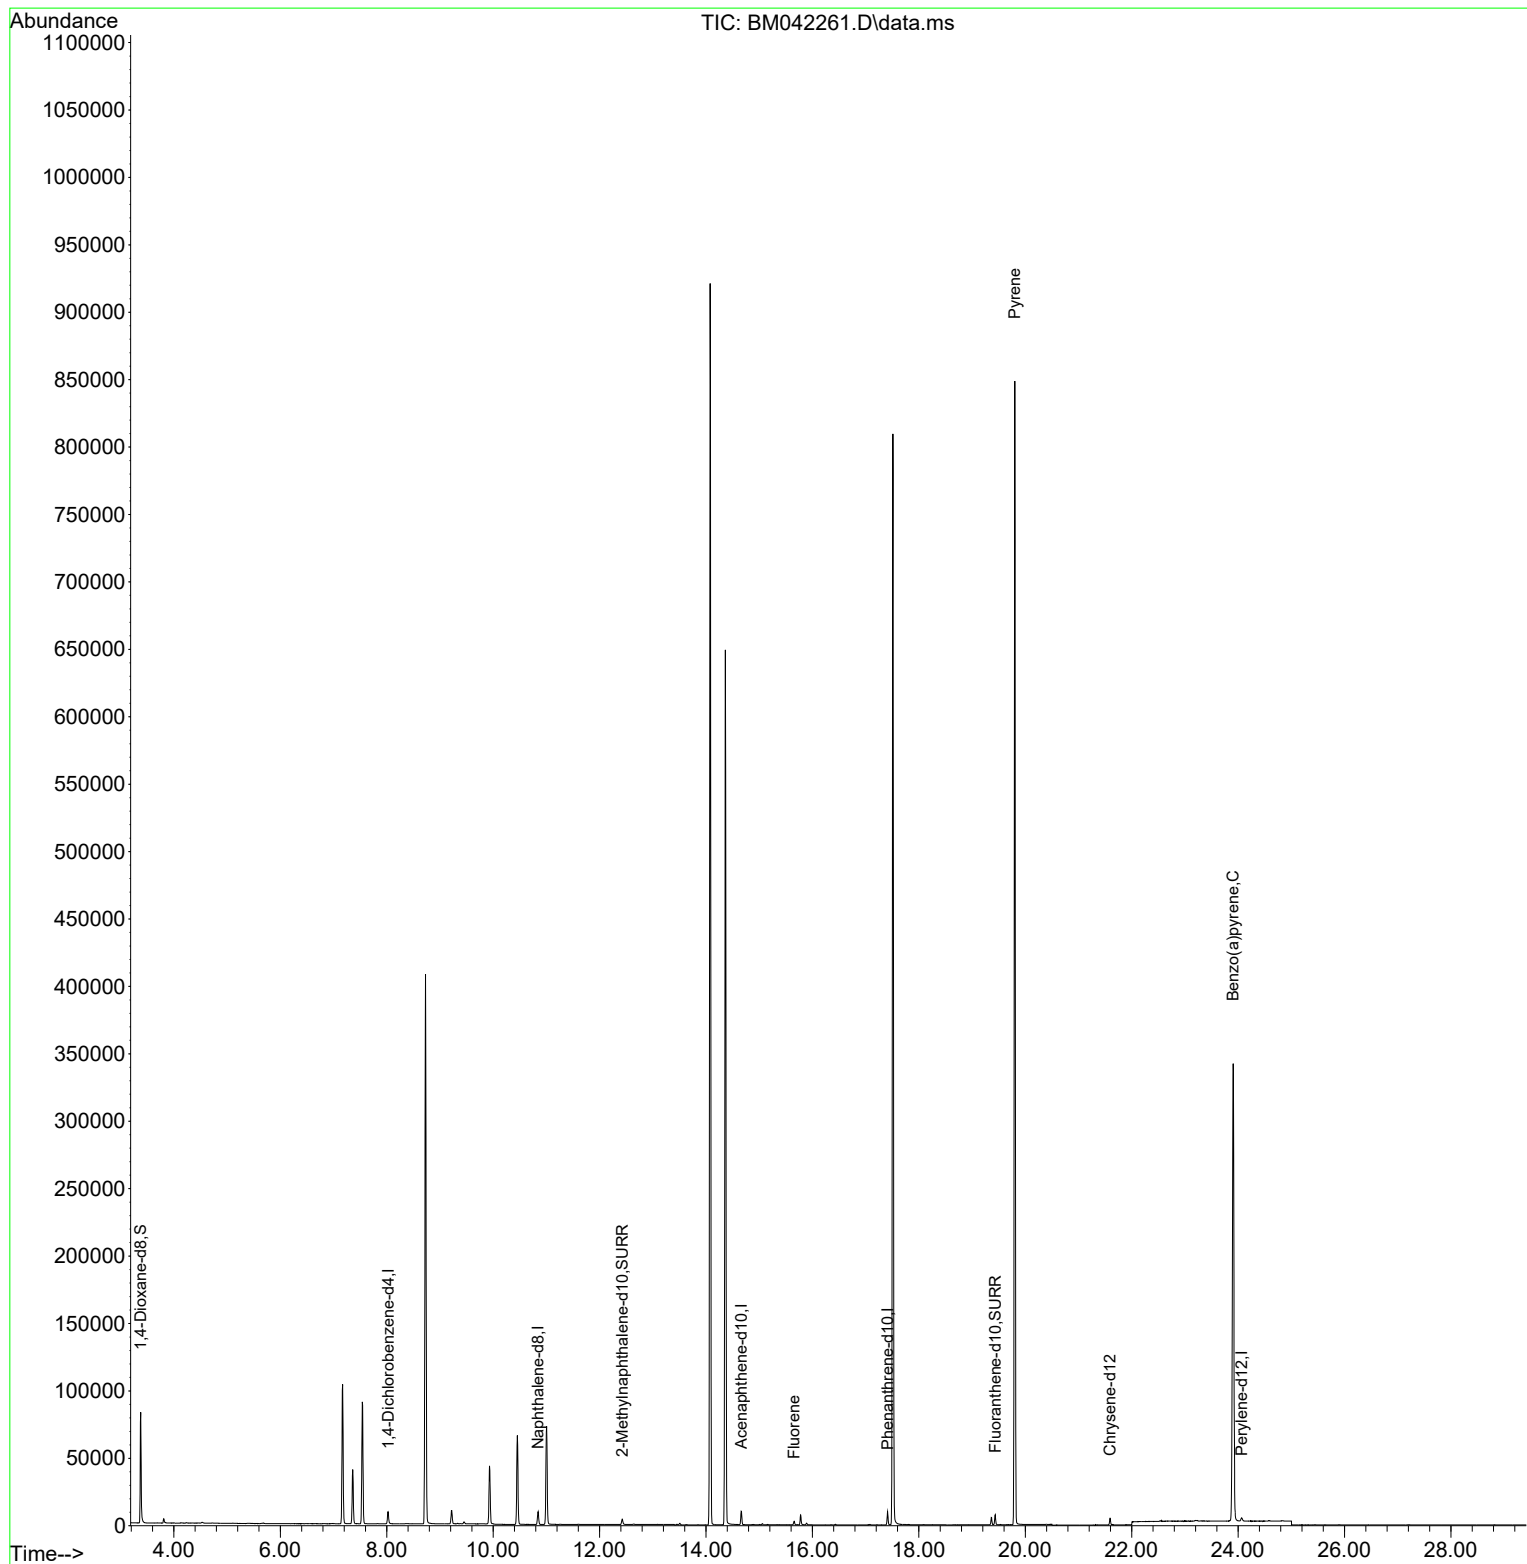


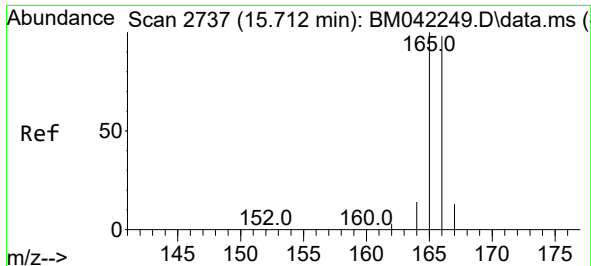

#12
 Fluorene
 Concen: 0.089 ng/ul
 RT: 15.656 min Scan# 21
 Delta R.T. -0.056 min
 Lab File: BM042261.D
 Acq: 10 Oct 2023 21:23




Instrument :
 BNA_M
 ClientSampleId :
 SBLK057


Tgt Ion:166 Resp: 2345
 Ion Ratio Lower Upper
 166 100
 165 9.0 78.4 117.6#
 167 33.9 11.5 17.3#

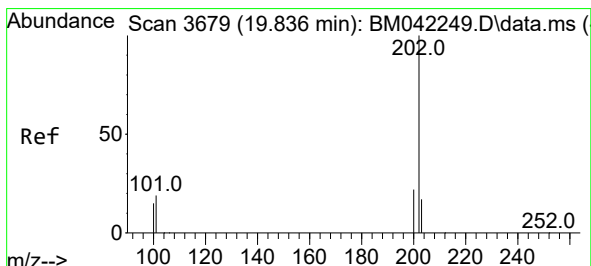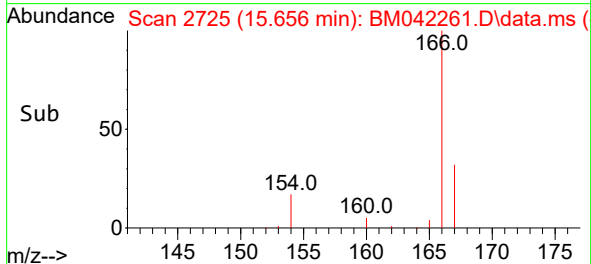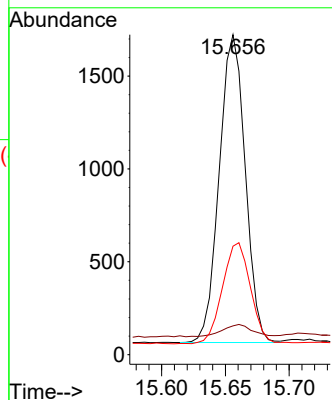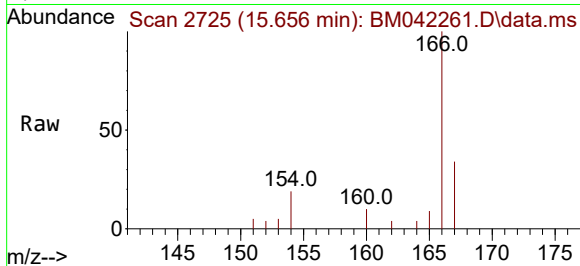

#20
 Pyrene
 Concen: 0.060 ng/ul
 RT: 19.803 min Scan# 3672
 Delta R.T. -0.033 min
 Lab File: BM042261.D
 Acq: 10 Oct 2023 21:23


Tgt Ion:202 Resp: 1762
 Ion Ratio Lower Upper
 202 100
 101 182.2 12.7 19.1#
 100 1358.3 9.9 14.9#

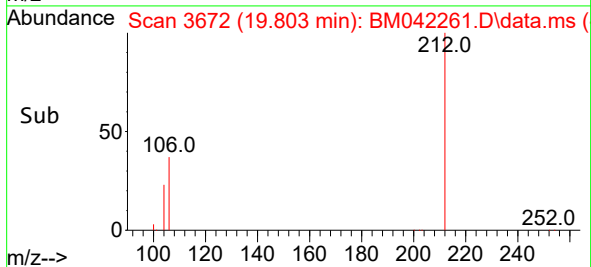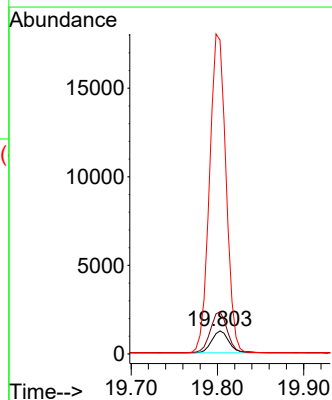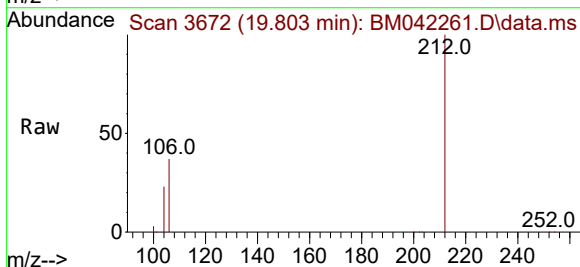

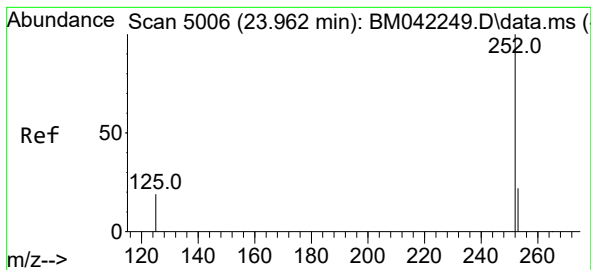

#26
Benzo(a)pyrene
Concen: 0.170 ng/ul
RT: 23.906 min Scan# 4987
Delta R.T. -0.056 min
Lab File: BM042261.D
Acq: 10 Oct 2023 21:23

Instrument :
BNA_M
ClientSampleId :
SBLK057

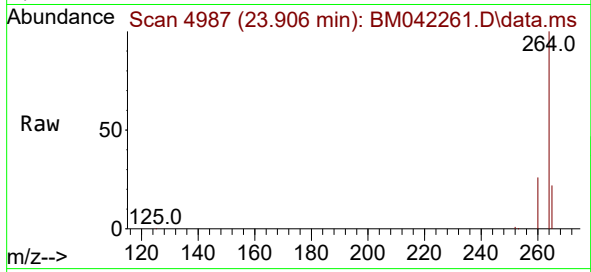

Tgt Ion:252 Resp: 3066
Ion Ratio Lower Upper
252 100
253 50.9 25.3 37.9#
125 51.1 23.2 34.8#

