

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042263.D
 Acq On : 10 Oct 2023 23:12
 Operator : MA/JU
 Sample : PB156094BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK094

Quant Time: Oct 11 00:48:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.026	152	5062	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	13067	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	5355	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	10040	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.594	240	3712	0.400	ng/ul	# 0.00
23) Perylene-d12	24.064	264	3702	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	33426	4.959	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	3660	0.204	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	3858	0.277	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	1381	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.904	252	2280	0.121	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042263.D
Acq On : 10 Oct 2023 23:12
Operator : MA/JU
Sample : PB156094BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK094

Quant Time: Oct 11 00:48:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration

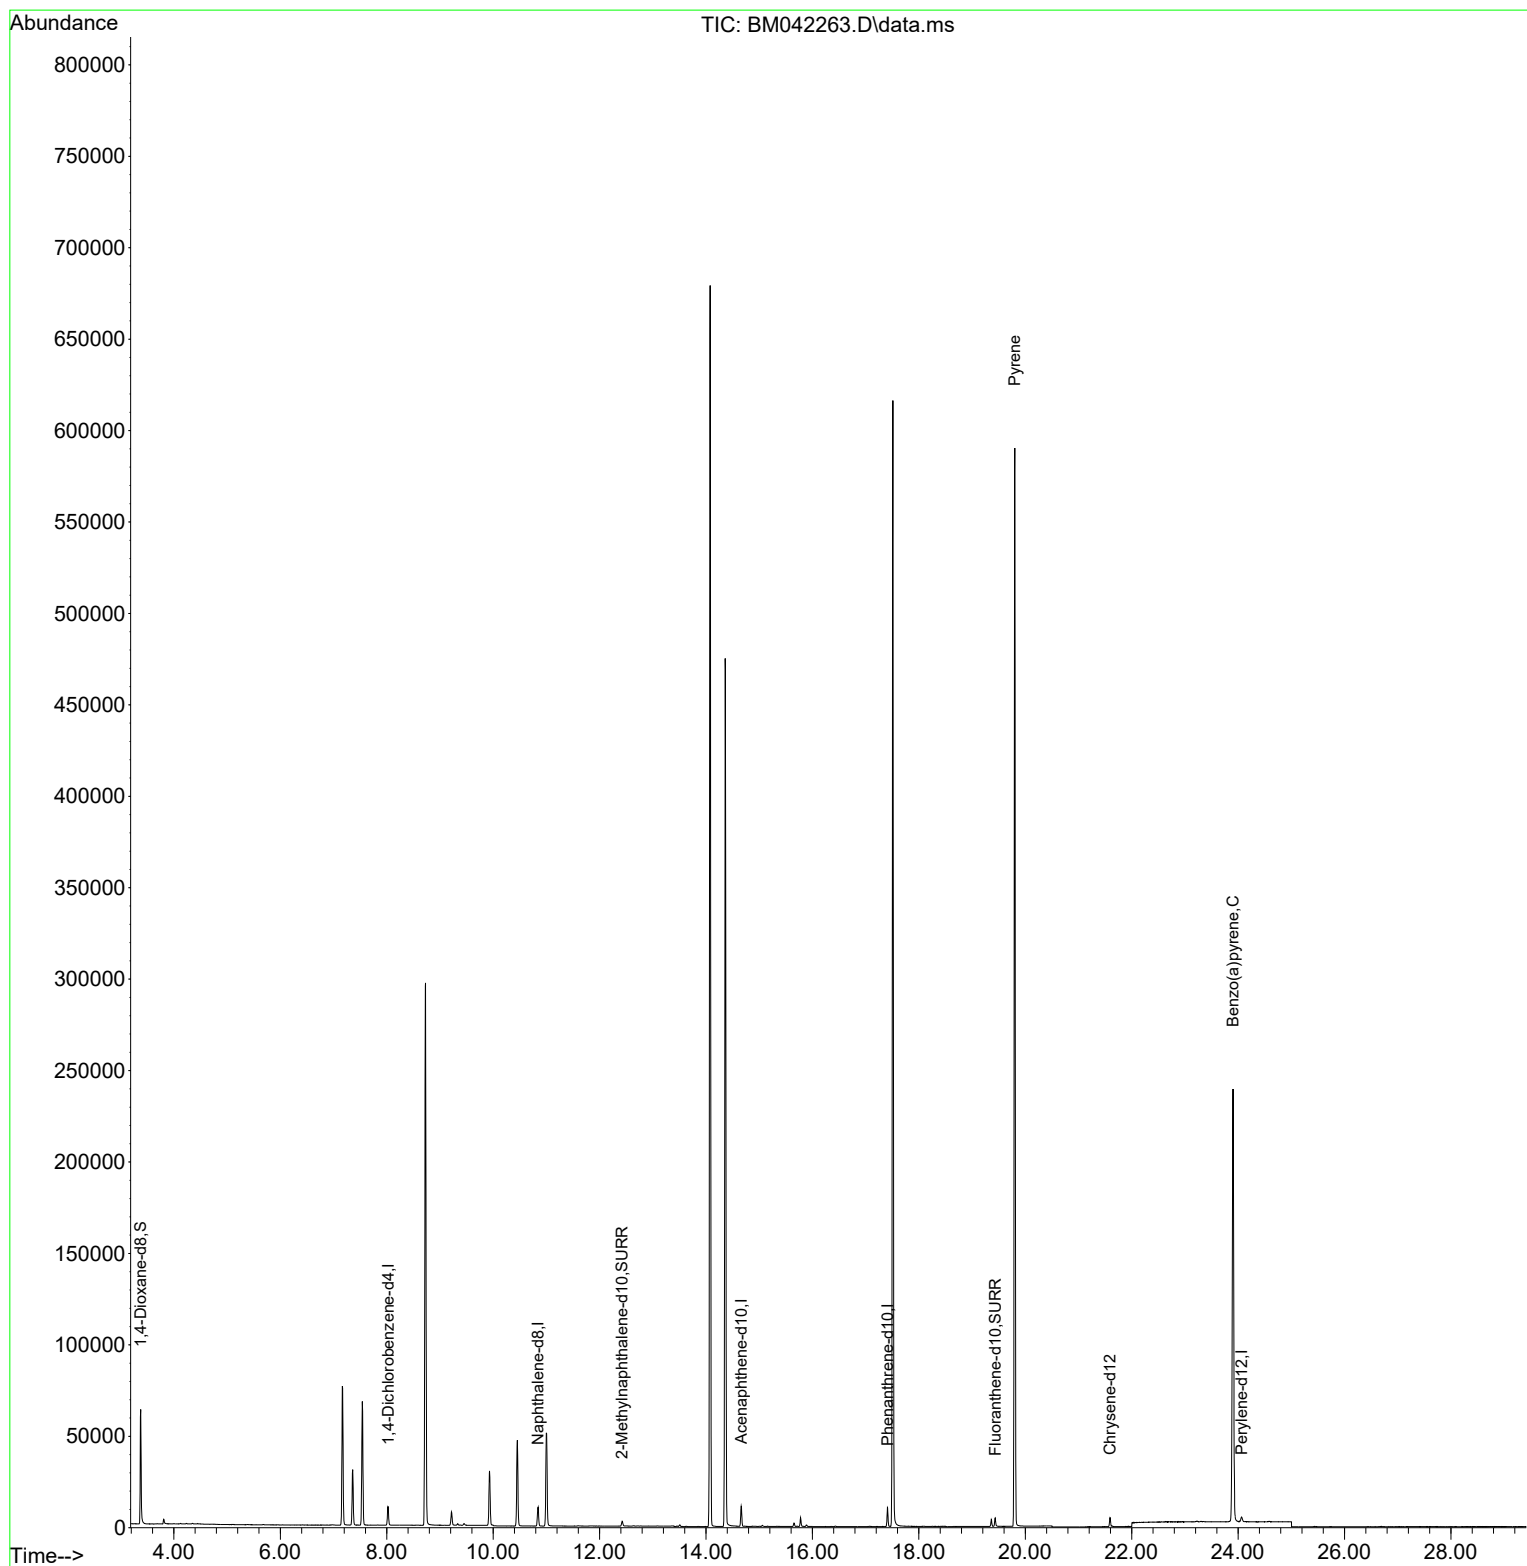

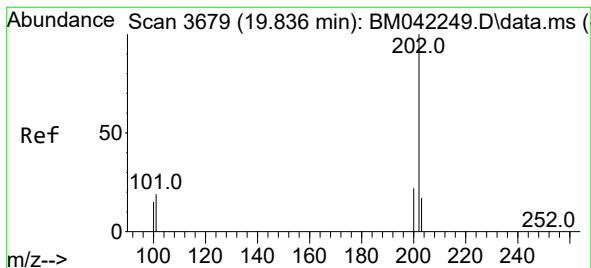

#20

Pyrene

Concen: 0.046 ng/ul

RT: 19.803 min Scan# 3

Delta R.T. -0.033 min

Lab File: BM042263.D

Acq: 10 Oct 2023 23:12

Instrument :

BNA_M

ClientSampleId :

SBLK094





Tgt Ion:202 Resp: 1381

Ion Ratio Lower Upper

202 100

101 181.5 12.7 19.1#

100 1315.4 9.9 14.9#

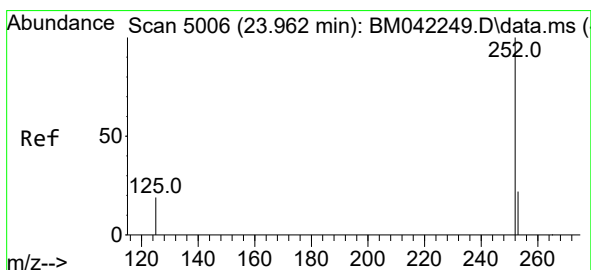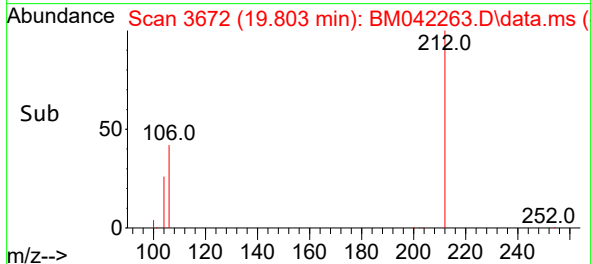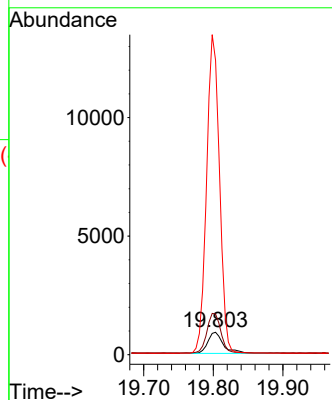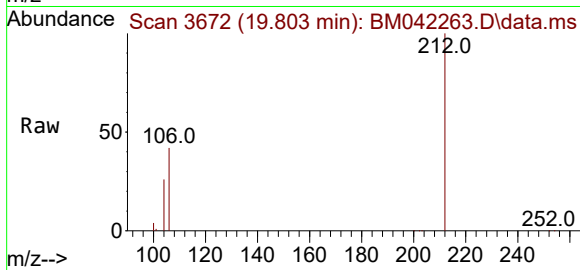

#26

Benzo(a)pyrene

Concen: 0.121 ng/ul

RT: 23.904 min Scan# 4986

Delta R.T. -0.058 min

Lab File: BM042263.D

Acq: 10 Oct 2023 23:12

Tgt Ion:252 Resp: 2280

Ion Ratio Lower Upper

252 100

253 55.9 25.3 37.9#

125 58.8 23.2 34.8#

