

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042264.D
 Acq On : 10 Oct 2023 23:48
 Operator : MA/JU
 Sample : PB156060BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK060

Quant Time: Oct 11 00:48:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.021	152	3779	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	9619	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	3951	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.413	188	8035	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.594	240	3294	0.400	ng/ul	# 0.00
23) Perylene-d12	24.064	264	3528	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	41361	8.219	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	4544	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	5853	0.473	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.656	166	2154	0.101	ng/ul#	15
20) Pyrene	19.803	202	1811	0.068	ng/ul#	1
26) Benzo(a)pyrene	23.906	252	3446	0.192	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042264.D
Acq On : 10 Oct 2023 23:48
Operator : MA/JU
Sample : PB156060BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK060

Quant Time: Oct 11 00:48:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration




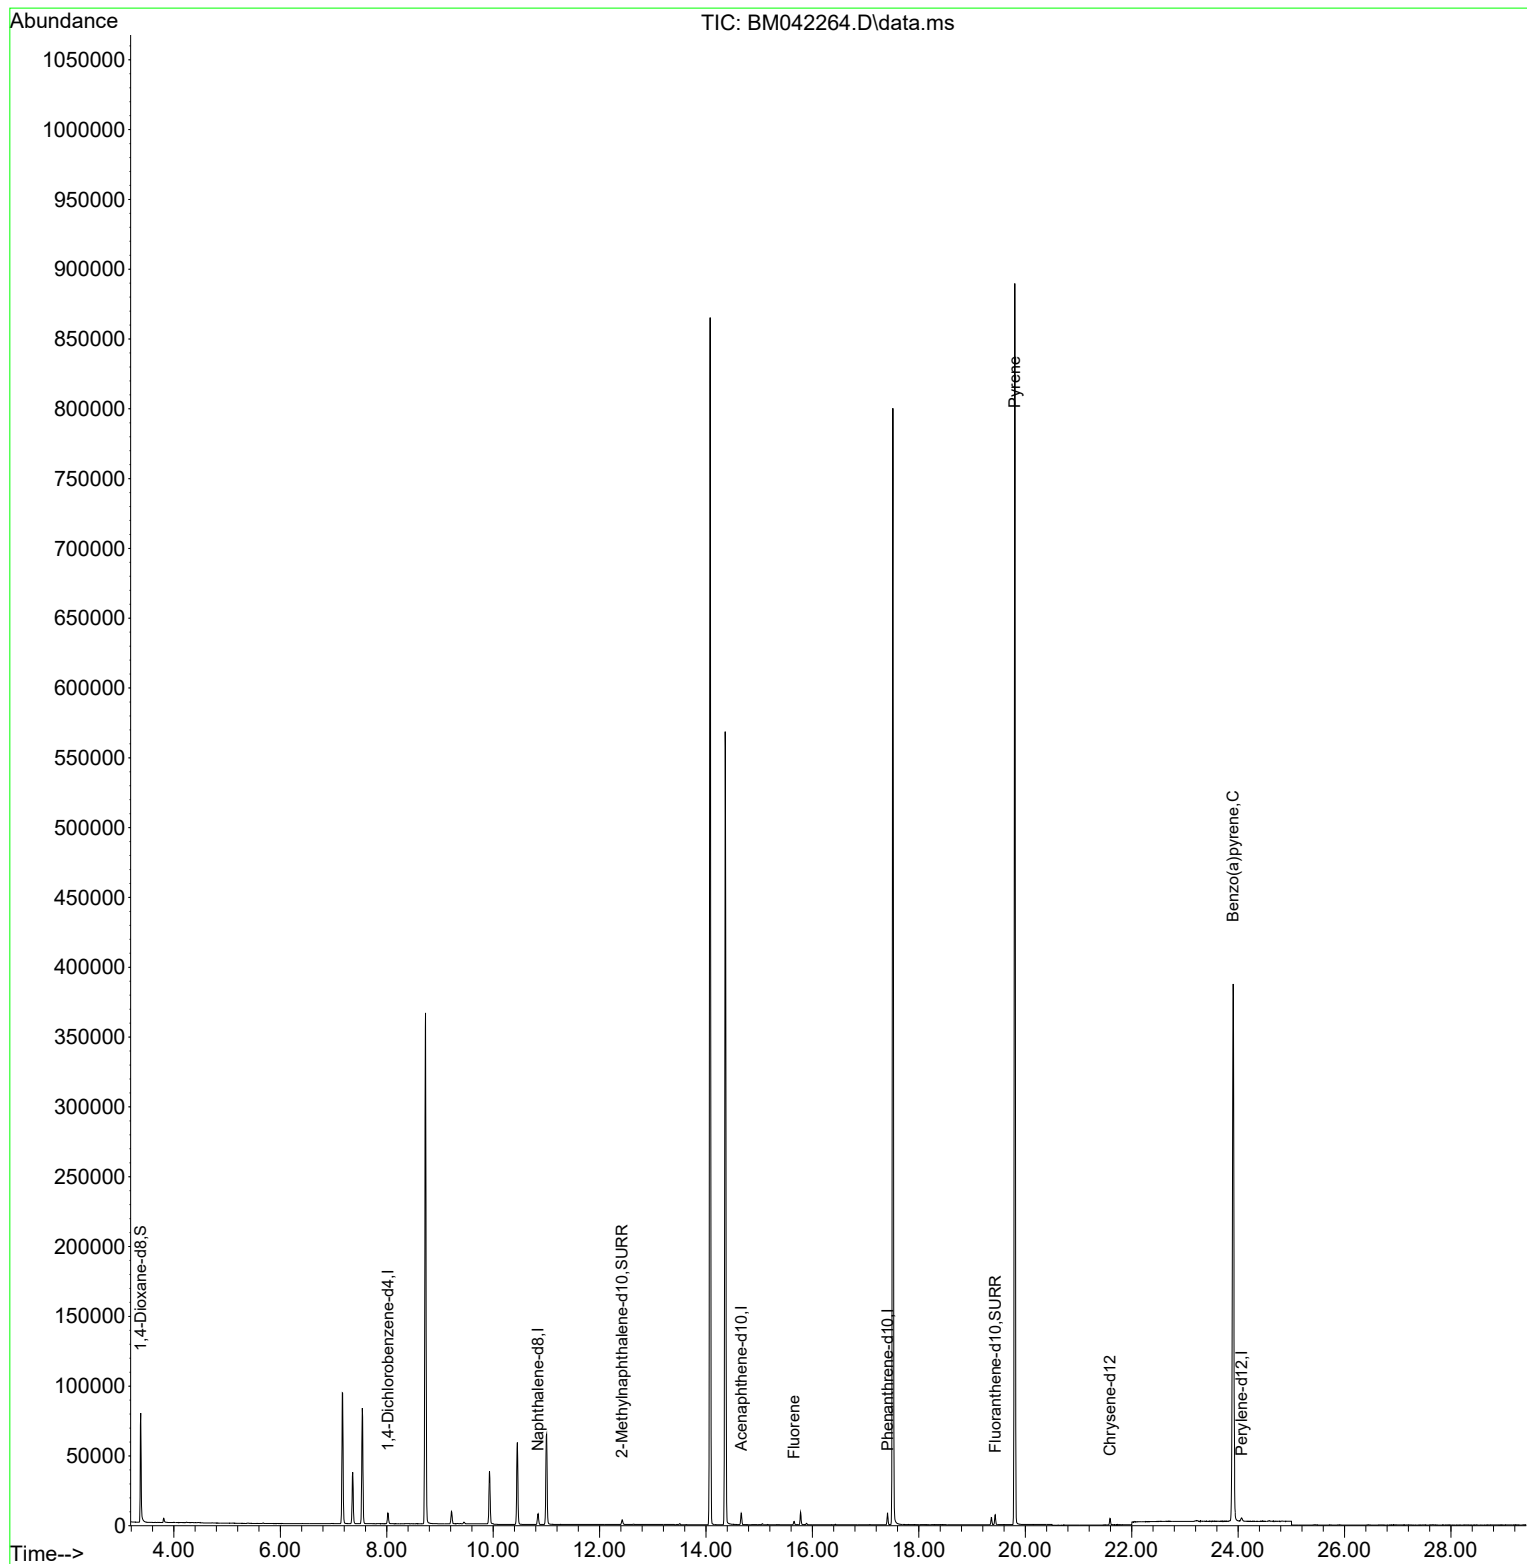


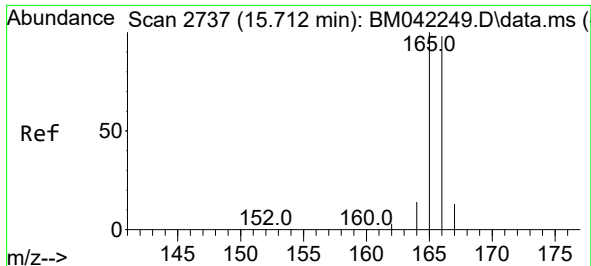

#12
Fluorene
Concen: 0.101 ng/ul
RT: 15.656 min Scan# 2154
Delta R.T. -0.056 min
Lab File: BM042264.D
Acq: 10 Oct 2023 23:48




Instrument :
BNA_M
ClientSampleId :
SBLK060


Tgt Ion:166 Resp: 2154
Ion Ratio Lower Upper
166 100
165 9.4 78.4 117.6#
167 35.4 11.5 17.3#

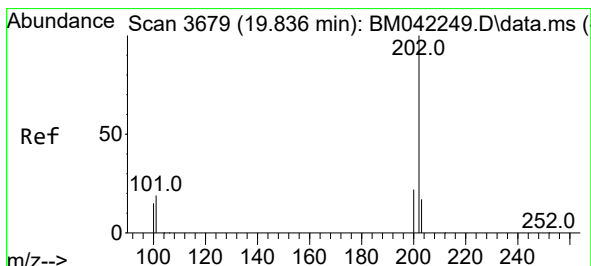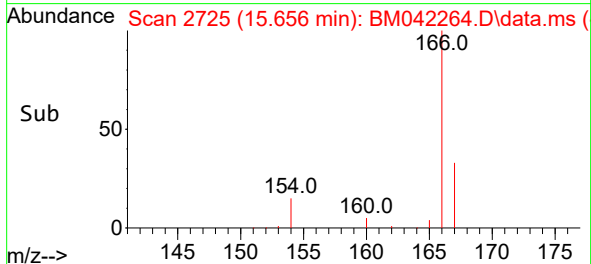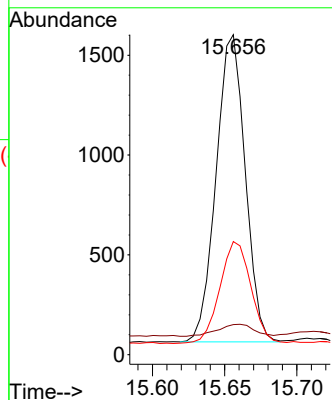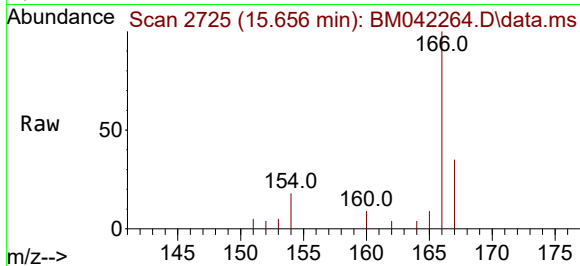

#20
Pyrene
Concen: 0.068 ng/ul
RT: 19.803 min Scan# 3672
Delta R.T. -0.033 min
Lab File: BM042264.D
Acq: 10 Oct 2023 23:48


Tgt Ion:202 Resp: 1811
Ion Ratio Lower Upper
202 100
101 185.1 12.7 19.1#
100 1396.6 9.9 14.9#

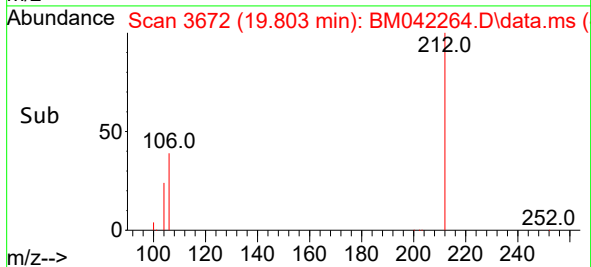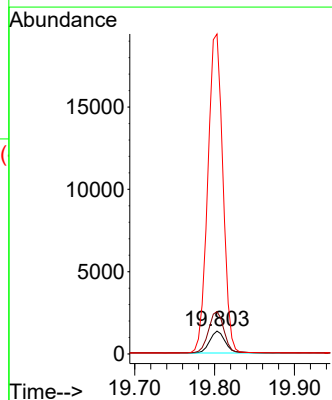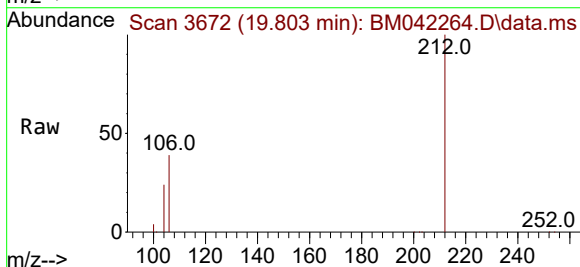

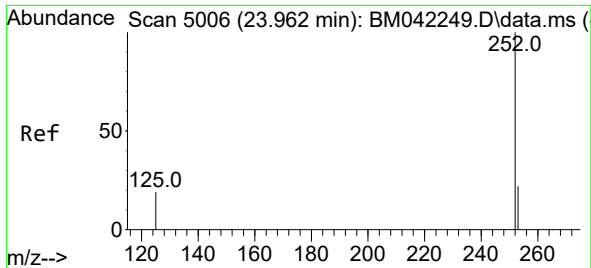

#26
Benzo(a)pyrene
Concen: 0.192 ng/ul
RT: 23.906 min Scan# 49
Delta R.T. -0.056 min
Lab File: BM042264.D
Acq: 10 Oct 2023 23:48

Instrument :
BNA_M
ClientSampleId :
SBLK060

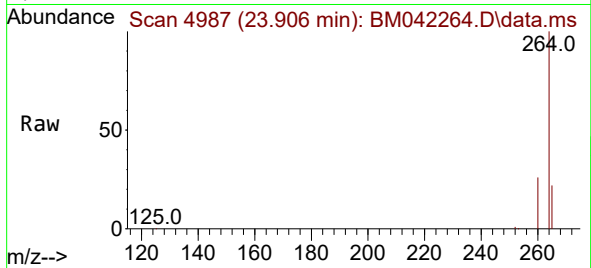

Tgt Ion:252 Resp: 3446
Ion Ratio Lower Upper
252 100
253 48.1 25.3 37.9#
125 49.1 23.2 34.8#

