

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042252.D
 Acq On : 10 Oct 2023 14:39
 Operator : MA/JU
 Sample : 04780-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH372

Quant Time: Oct 10 15:48:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.026	152	4252	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	11193	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	4451	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	8654	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.600	240	3706	0.400	ng/ul	# 0.00
23) Perylene-d12	24.079	264	3590	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.377	96	14264	2.519	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	4506	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	6468	0.465	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.414	88	4300	0.727	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042252.D
Acq On : 10 Oct 2023 14:39
Operator : MA/JU
Sample : 04780-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH372


Quant Time: Oct 10 15:48:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration

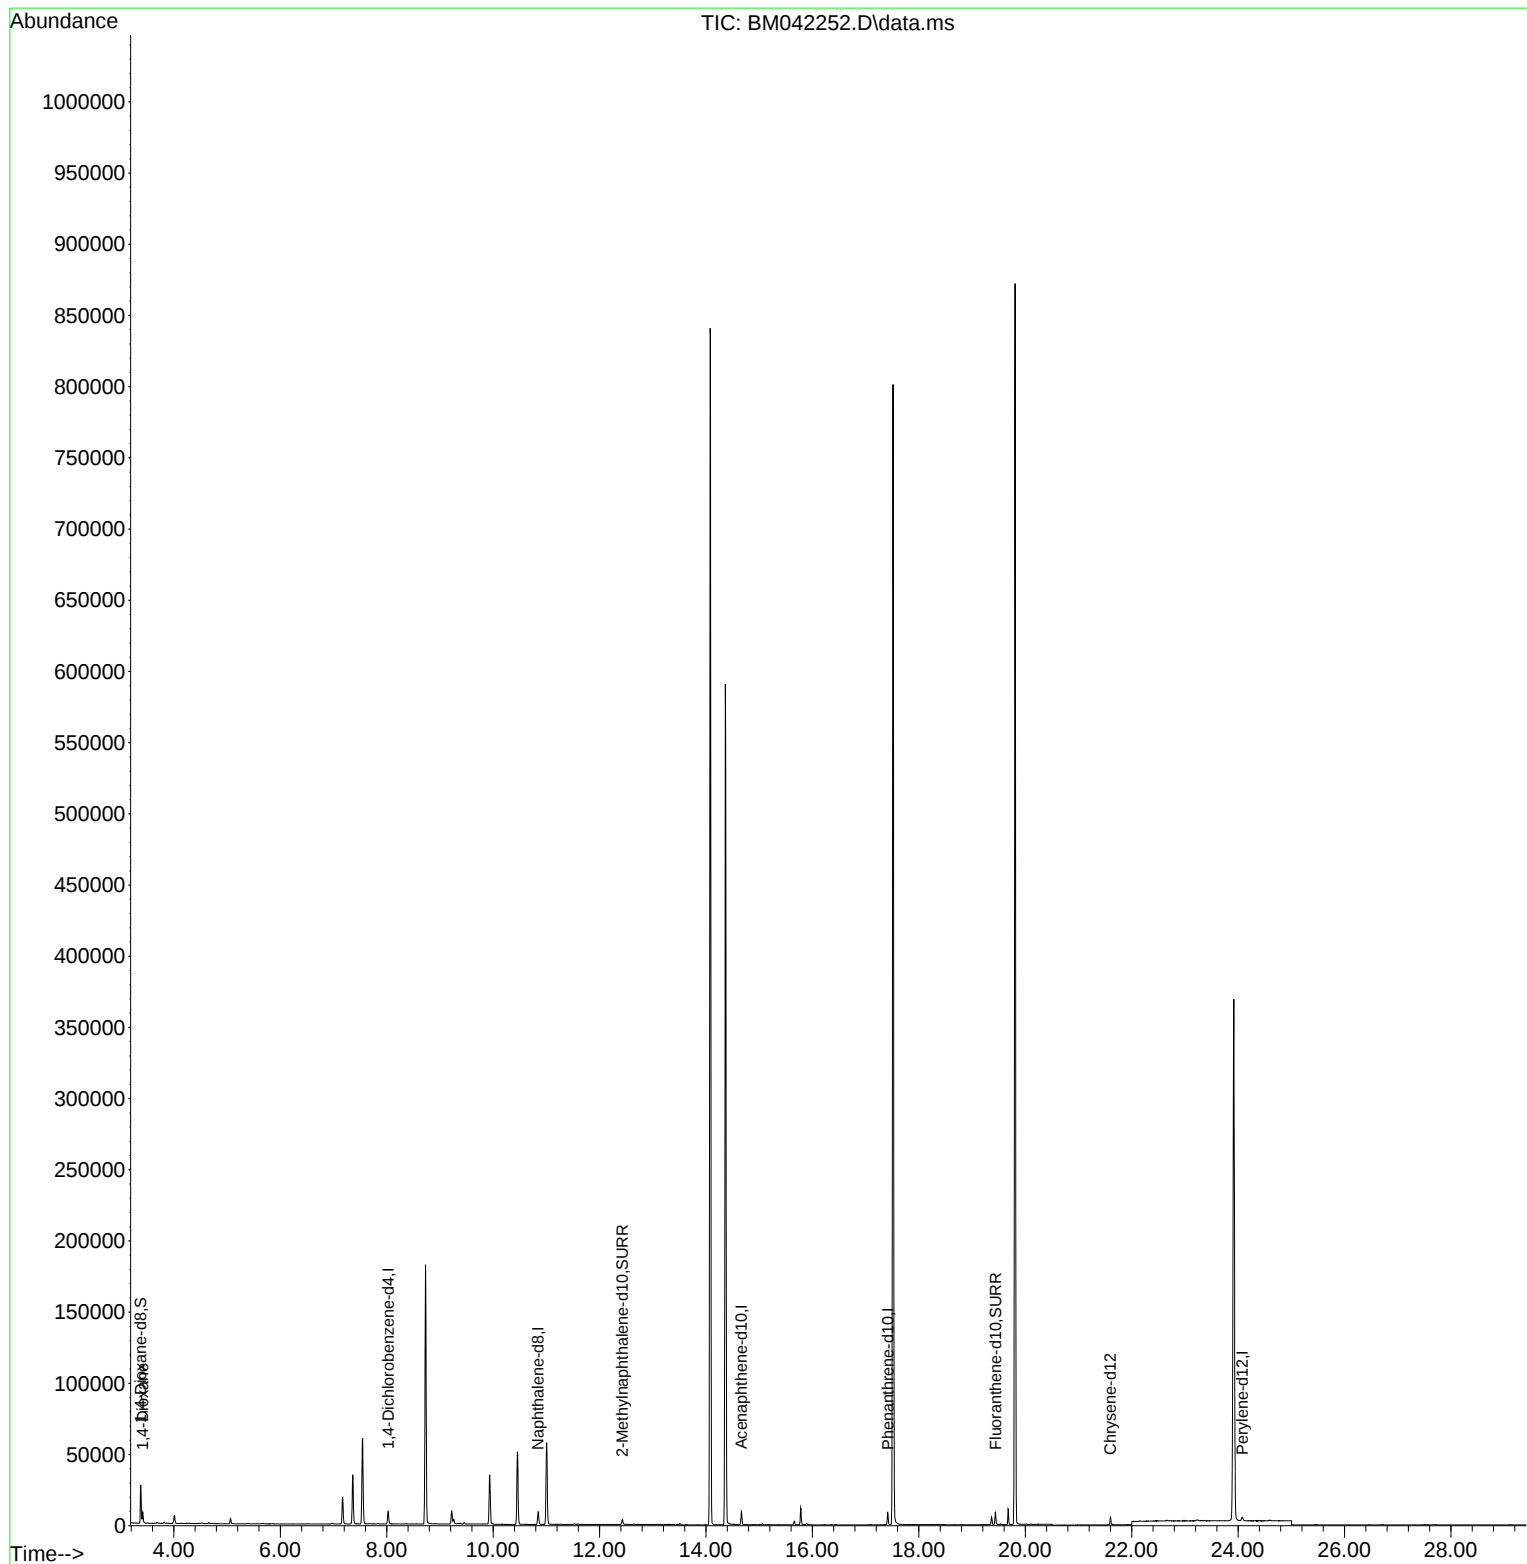

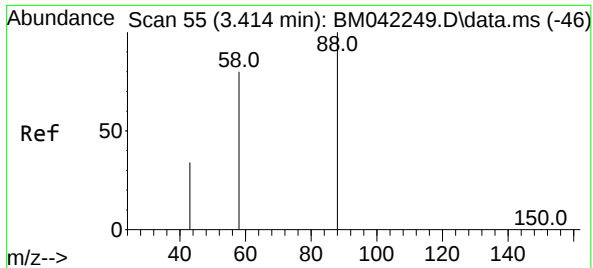

#2
1,4-Dioxane
Concen: 0.727 ng/ul
RT: 3.414 min Scan# 51
Delta R.T. 0.000 min
Lab File: BM042252.D
Acq: 10 Oct 2023 14:39

Instrument :
BNA_M
ClientSampleId :
BH372

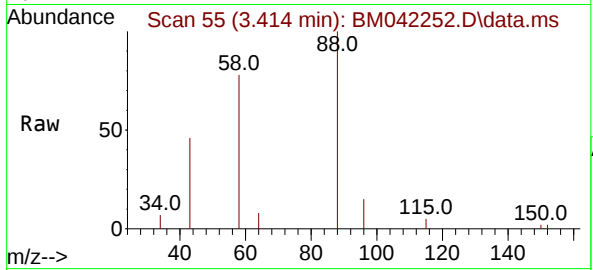

Tgt Ion: 88 Resp: 4300
Ion Ratio Lower Upper
88 100
43 45.7 52.1 78.1#
58 78.0 53.8 80.6

