

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042266.D
 Acq On : 11 Oct 2023 01:00
 Operator : MA/JU
 Sample : 04654-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBBW5

Quant Time: Oct 11 01:43:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.021	152	5713	0.400	ng/ul	0.00
4) Naphthalene-d8	10.840	136	14725	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.661	164	6131	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.409	188	12092	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.591	240	4849	0.400	ng/ul	# 0.00
23) Perylene-d12	24.064	264	4779	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	32398	4.258	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	6287	0.311	ng/ul	0.00
18) Fluoranthene-d10	19.431	212	8564	0.470	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.414	88	5025	0.632	ng/ul#	84
14) Pentachlorophenol	17.042	266	11819	2.156	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042266.D
Acq On : 11 Oct 2023 01:00
Operator : MA/JU
Sample : 04654-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBBW5

Quant Time: Oct 11 01:43:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration




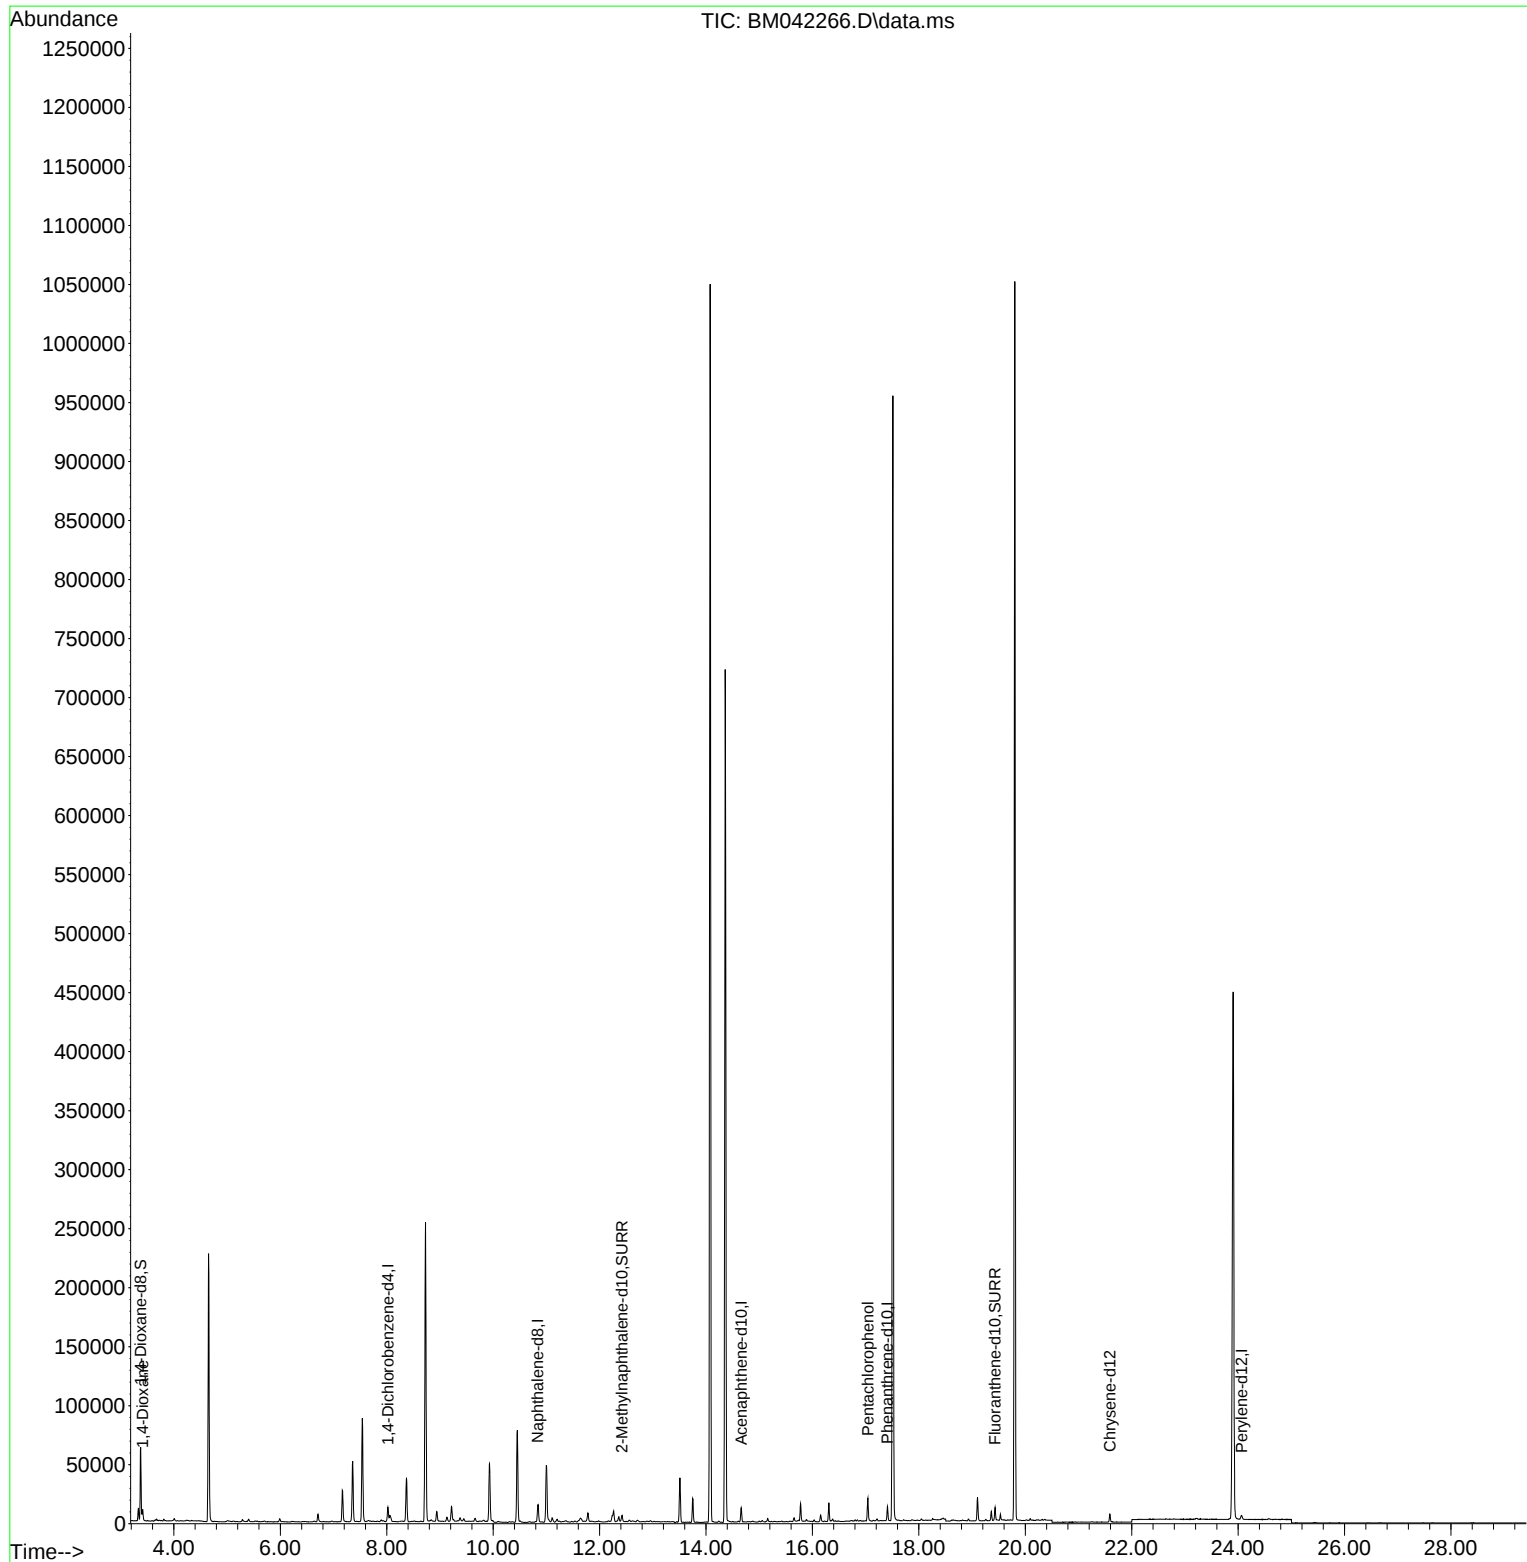


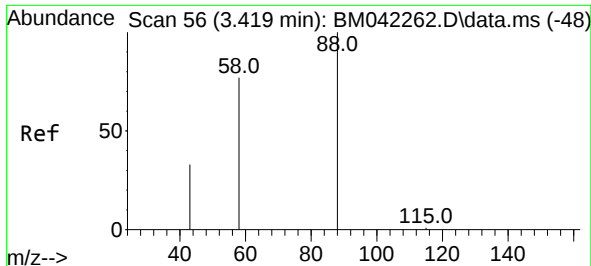

#2
 1,4-Dioxane
 Concen: 0.632 ng/ul
 RT: 3.414 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM042266.D
 Acq: 11 Oct 2023 01:00

Instrument :
 BNA_M
 ClientSampleId :
 BBBW5

Tgt Ion: 88 Resp: 5025
 Ion Ratio Lower Upper
 88 100
 43 50.0 52.1 78.1#
 58 77.2 53.8 80.6

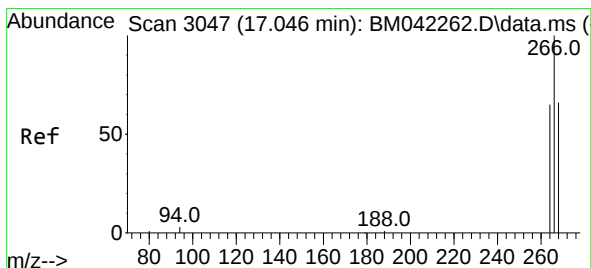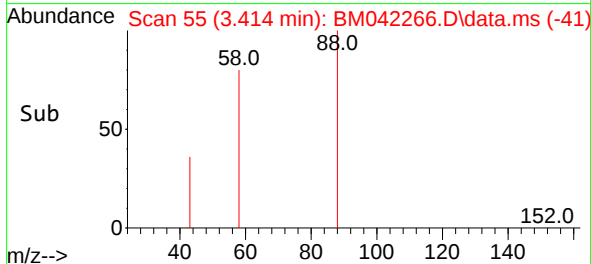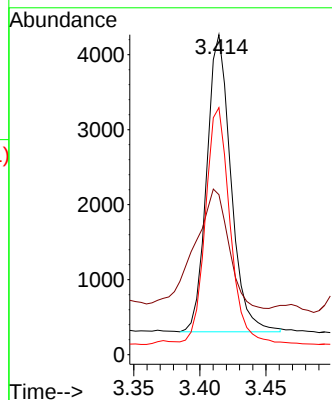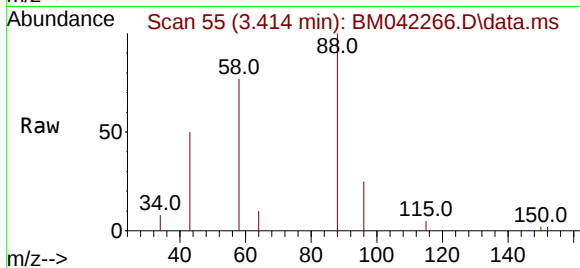

#14
 Pentachlorophenol
 Concen: 2.156 ng/ul
 RT: 17.042 min Scan# 3046
 Delta R.T. -0.008 min
 Lab File: BM042266.D
 Acq: 11 Oct 2023 01:00

Tgt Ion: 266 Resp: 11819
 Ion Ratio Lower Upper
 266 100
 264 62.6 51.1 76.7
 268 63.8 52.1 78.1

