

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042269.D
 Acq On : 11 Oct 2023 02:49
 Operator : MA/JU
 Sample : 04676-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK66

Quant Time: Oct 11 03:26:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.021	152	4323	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	11233	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	4533	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	8915	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.591	240	3803	0.400	ng/ul	# 0.00
23) Perylene-d12	24.064	264	3911	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	25667	4.458	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	4894	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.431	212	6707	0.470	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.414	88	9906	1.648	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042269.D
Acq On : 11 Oct 2023 02:49
Operator : MA/JU
Sample : 04676-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBK66

Quant Time: Oct 11 03:26:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration

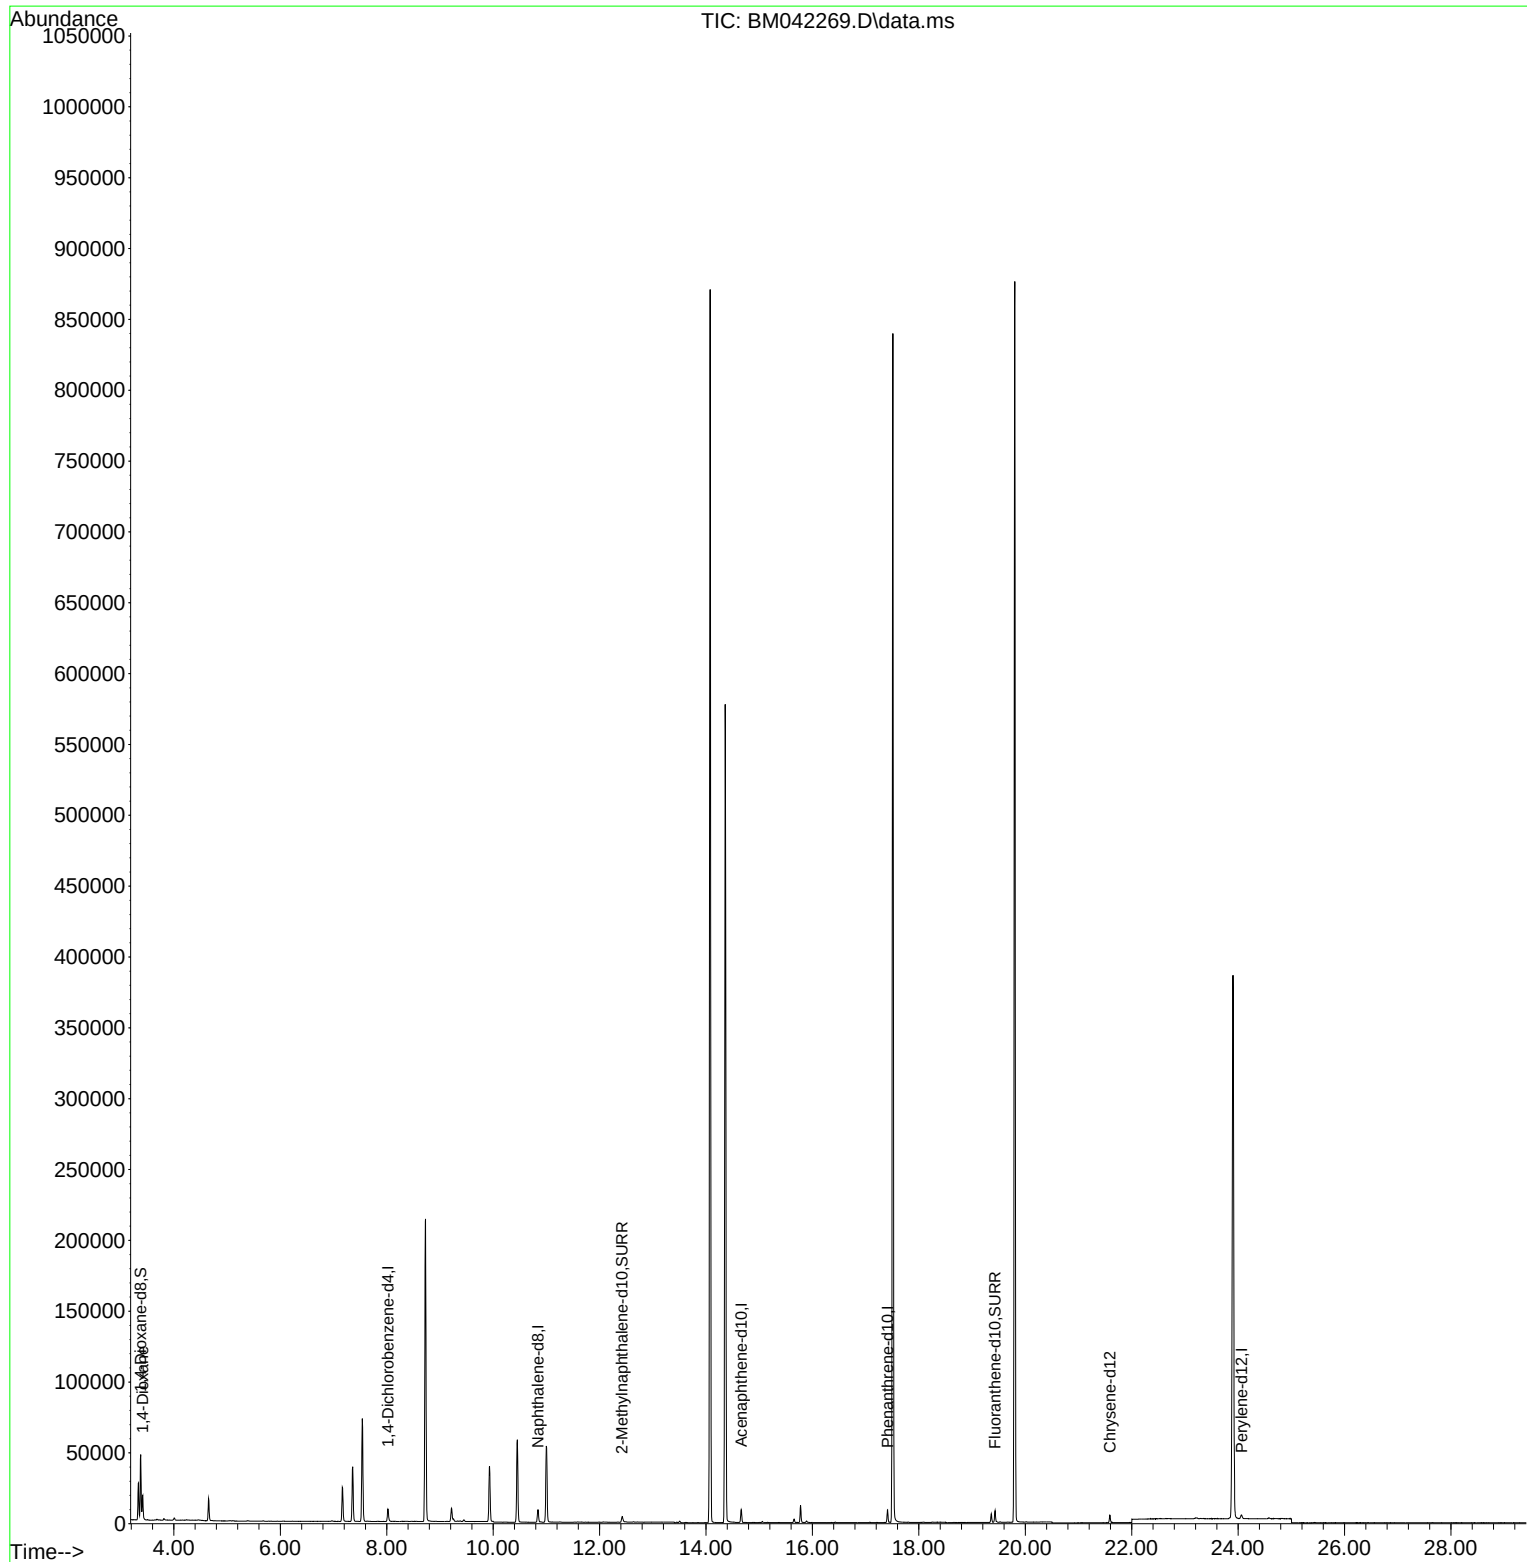

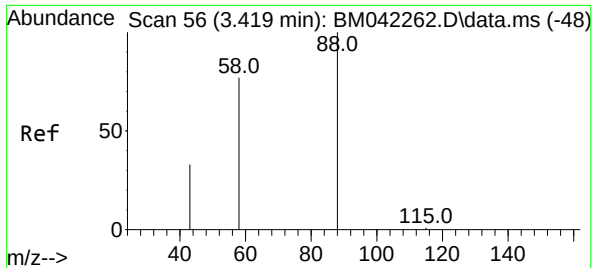

#2
 1,4-Dioxane
 Concen: 1.648 ng/ul
 RT: 3.414 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM042269.D
 Acq: 11 Oct 2023 02:49

Instrument :
 BNA_M
 ClientSampleId :
 BBK66

Tgt Ion: 88 Resp: 9906

Ion	Ratio	Lower	Upper
88	100		
43	37.1	52.1	78.1#
58	74.5	53.8	80.6

