

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
 Data File : BM042270.D
 Acq On : 11 Oct 2023 03:25
 Operator : MA/JU
 Sample : 04654-14DL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBBT9DL

Quant Time: Oct 11 04:22:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 14:01:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.021	152	4308	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	10921	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.661	164	4858	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	9424	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.591	240	4189	0.400	ng/ul	# 0.00
23) Perylene-d12	24.061	264	4195	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	1380	0.241	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	377	0.025	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	577	0.037	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.418	88	284	0.047	ng/ul#	78
14) Pentachlorophenol	17.041	266	2753	0.644	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101023\
Data File : BM042270.D
Acq On : 11 Oct 2023 03:25
Operator : MA/JU
Sample : 04654-14DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBBT9DL

Quant Time: Oct 11 04:22:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 14:01:53 2023
Response via : Initial Calibration




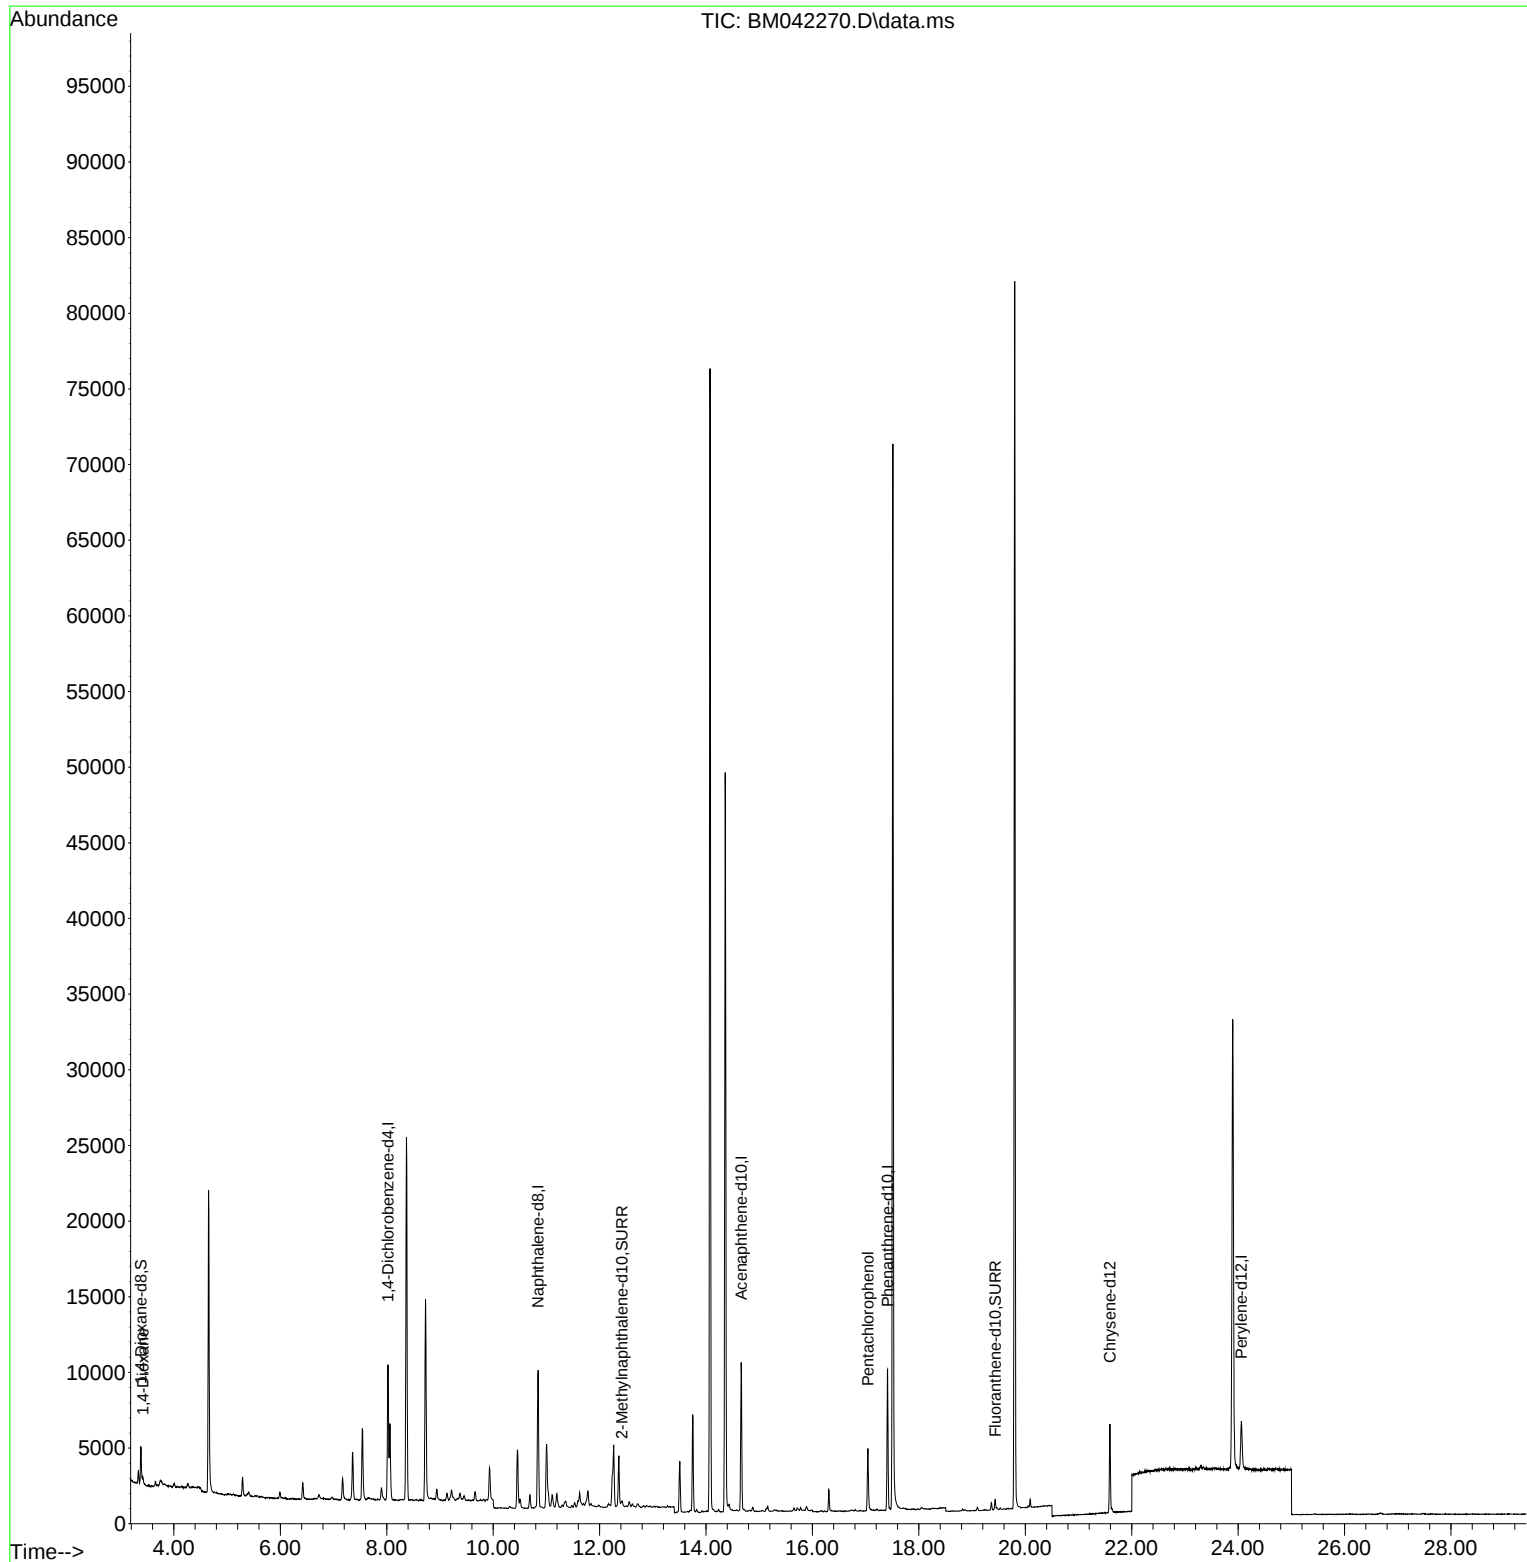


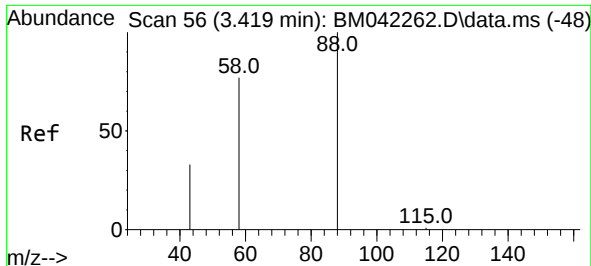

#2
1,4-Dioxane
Concen: 0.047 ng/ul
RT: 3.418 min Scan# 50
Delta R.T. 0.004 min
Lab File: BM042270.D
Acq: 11 Oct 2023 03:25

Instrument :
BNA_M
ClientSampleId :
BBBT9DL

Tgt Ion: 88 Resp: 284
Ion Ratio Lower Upper
88 100
43 68.9 52.1 78.1
58 35.5 53.8 80.6#

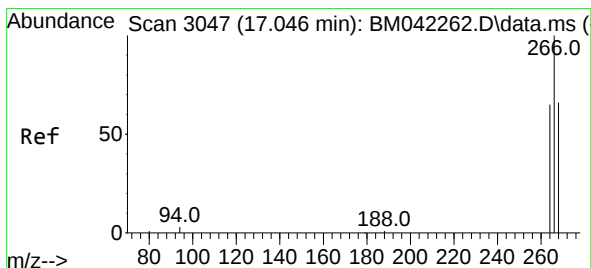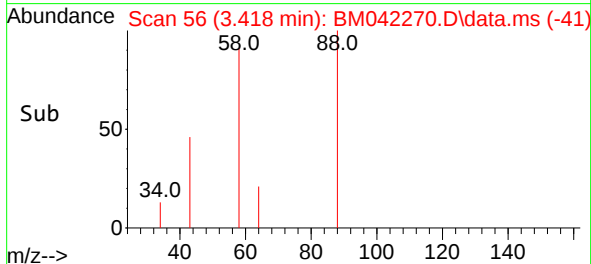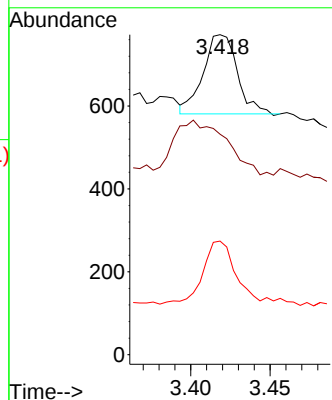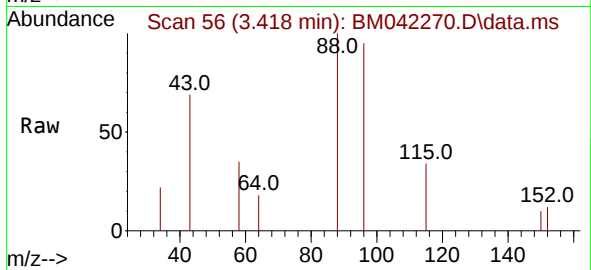

#14
Pentachlorophenol
Concen: 0.644 ng/ul
RT: 17.041 min Scan# 3046
Delta R.T. -0.009 min
Lab File: BM042270.D
Acq: 11 Oct 2023 03:25

Tgt Ion: 266 Resp: 2753
Ion Ratio Lower Upper
266 100
264 63.1 51.1 76.7
268 65.2 52.1 78.1

