




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 18:48:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

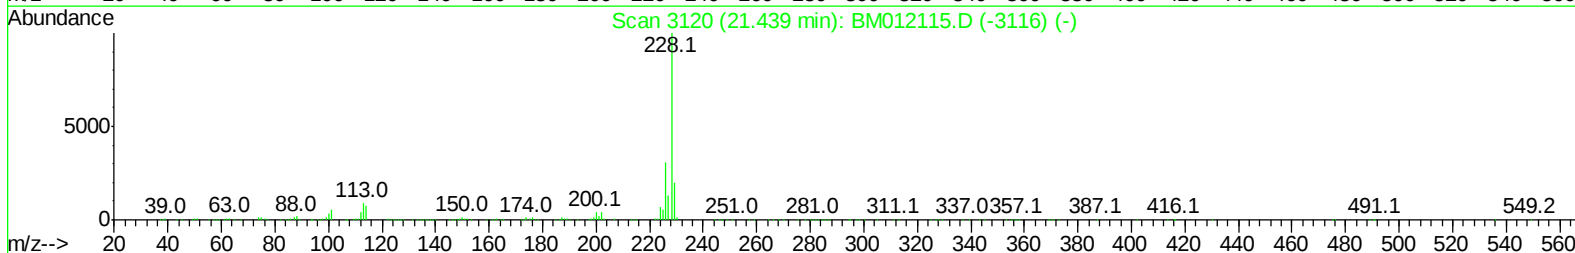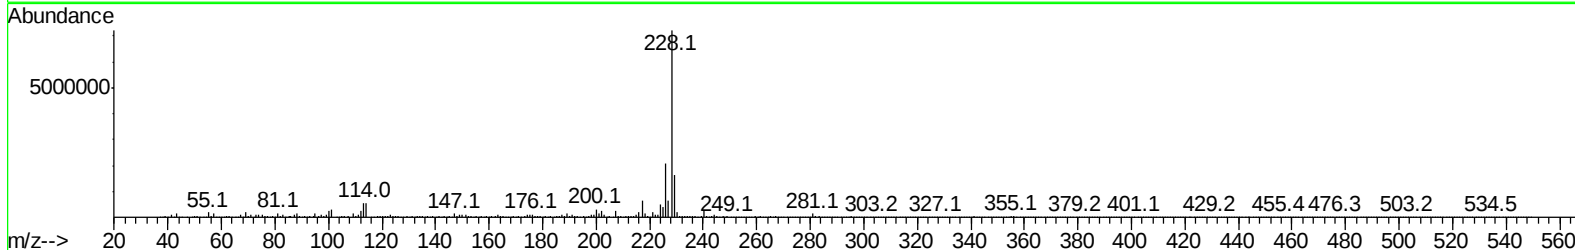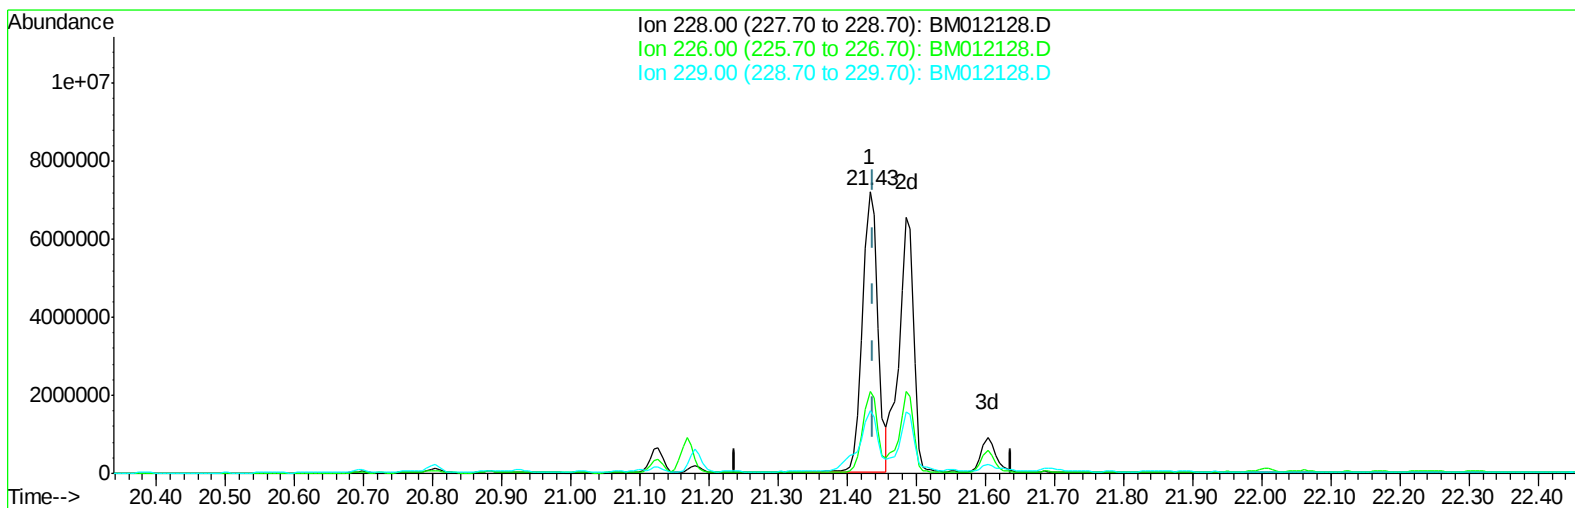

TIC: BM012128.D

(82) Chrysene

21.433min (-0.006) 121.10ng/ul

response 11108085

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	29.09
229.00	19.40	22.35
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 18:48:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

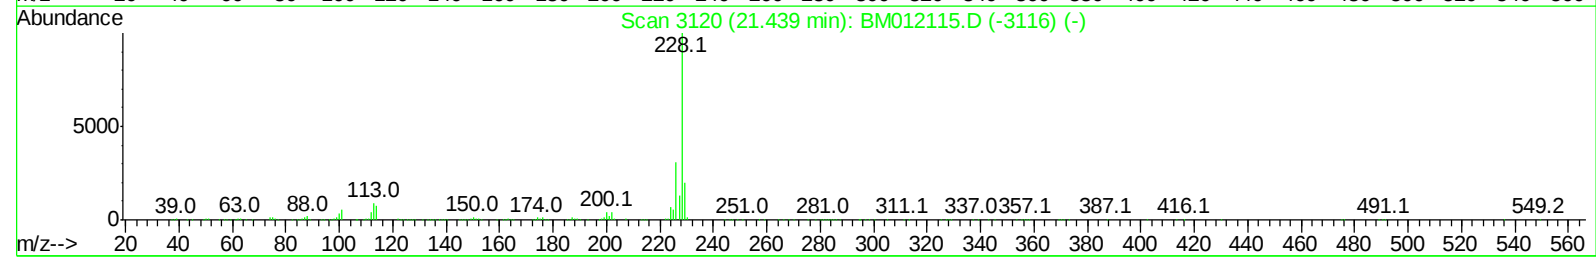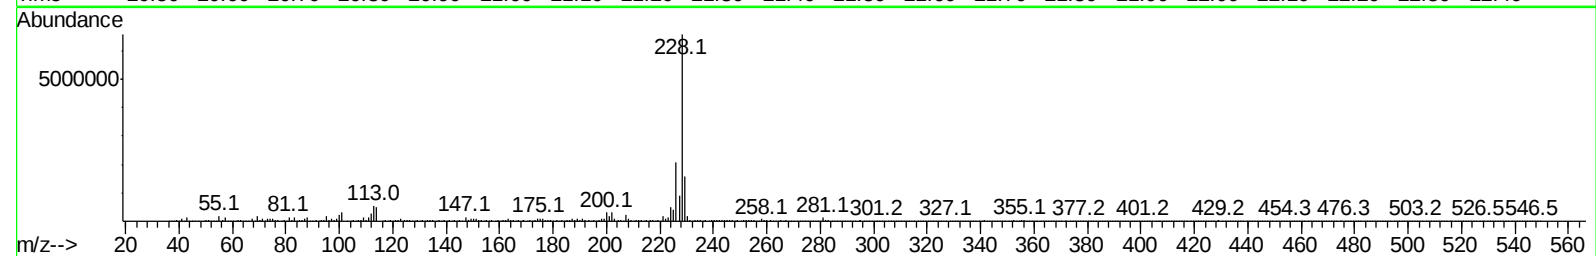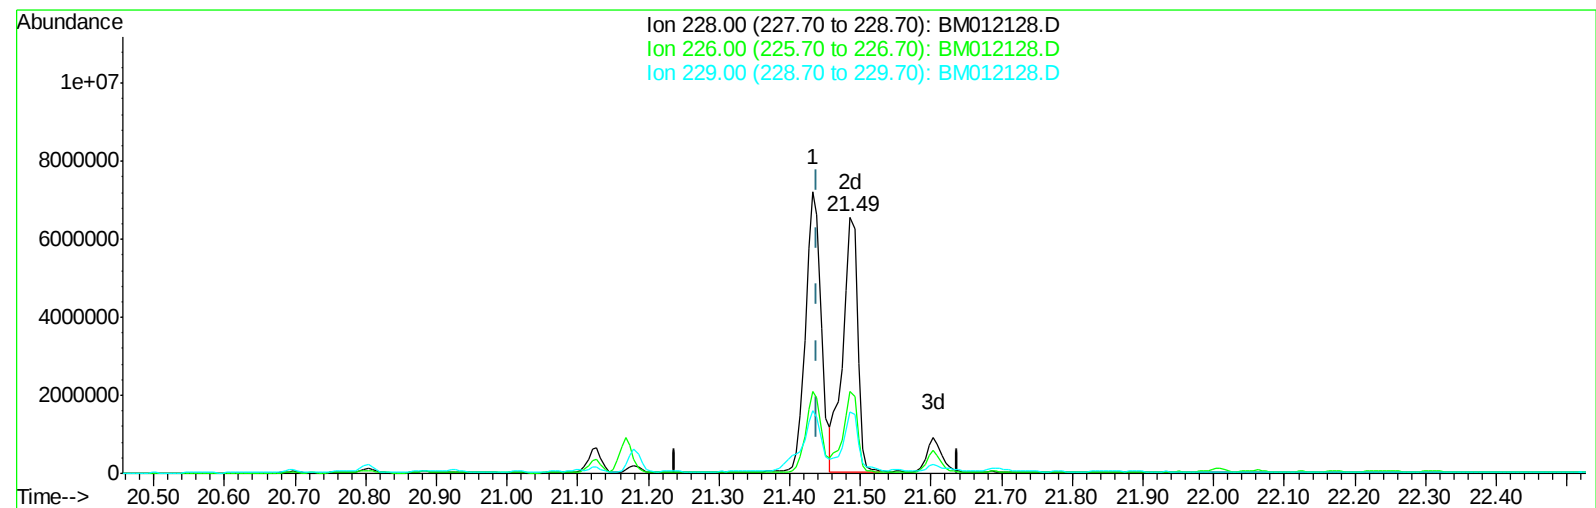

TIC: BM012128.D

(82) Chrysene

21.486min (+0.047) 104.56ng/ul m

response 9590866

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	31.81
229.00	19.40	23.98#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 18:48:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

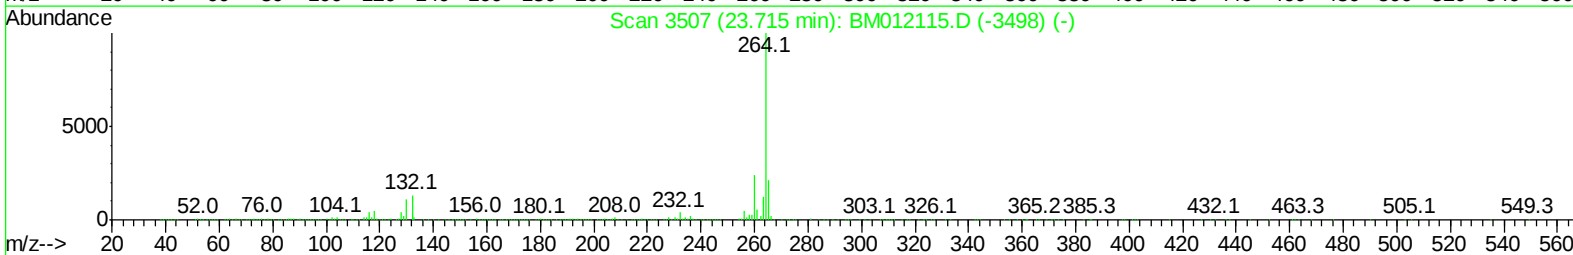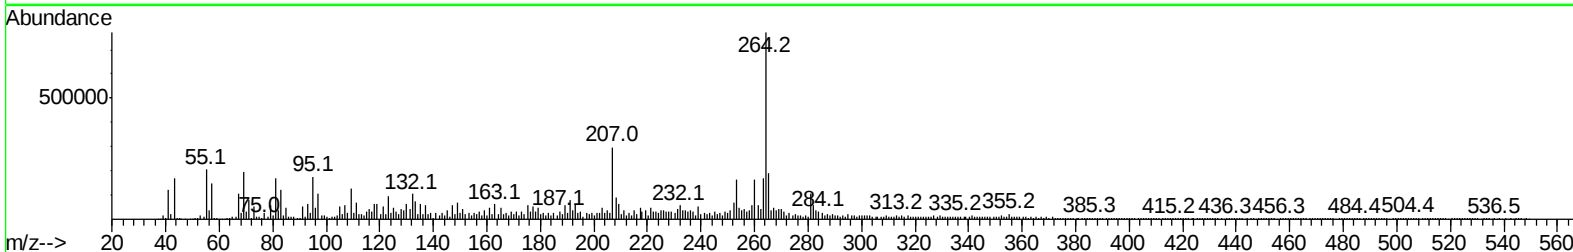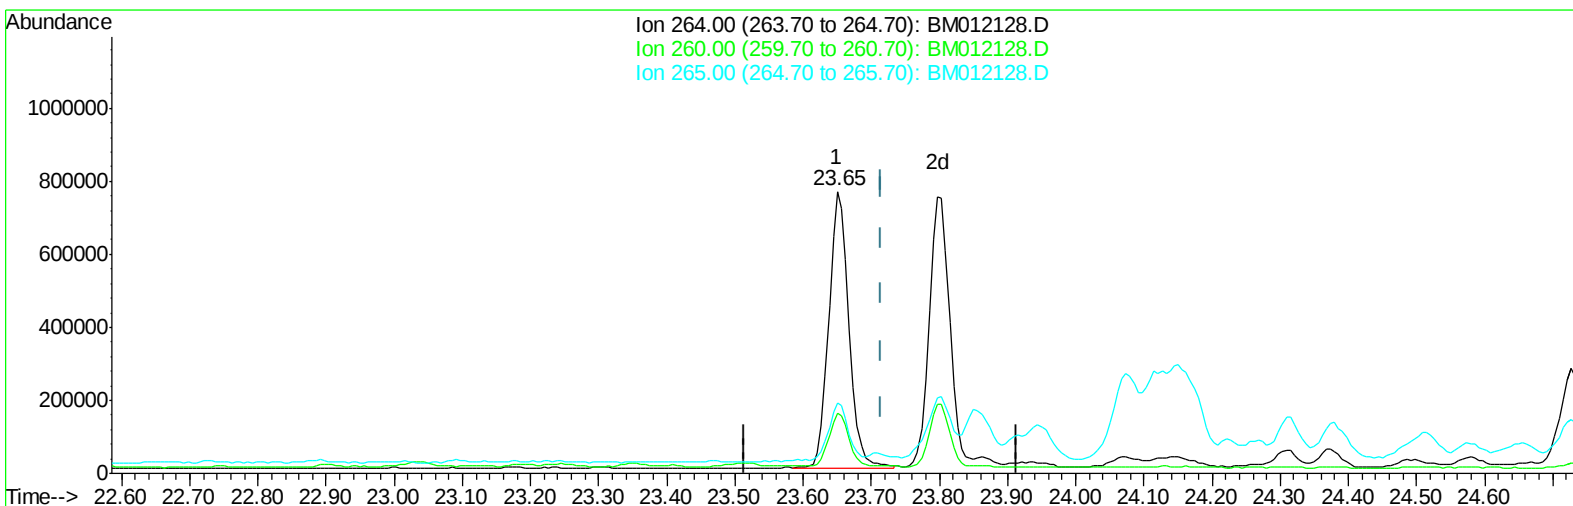

TIC: BM012128.D

(83) Perylene-d12 (I)

23.650min (-0.065) 20.00ng/ul

response 1559335

Ion	Exp%	Act%
264.00	100	100
260.00	24.20	21.54
265.00	22.50	24.86
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 18:48:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

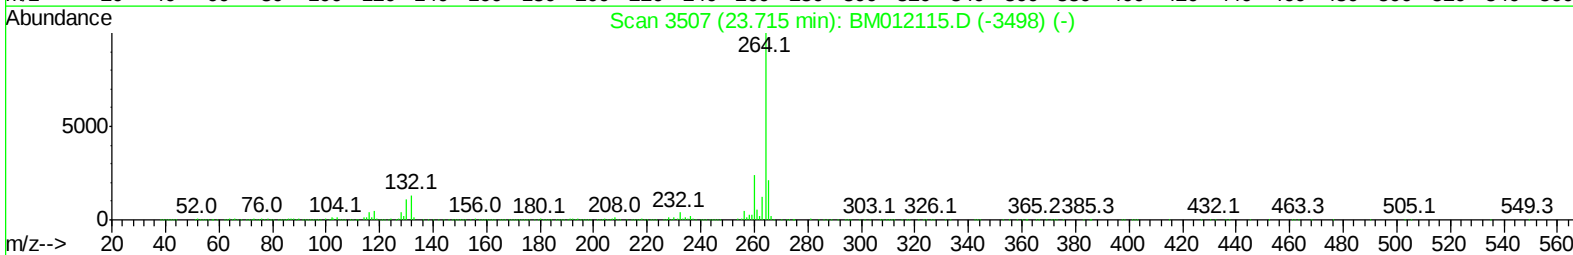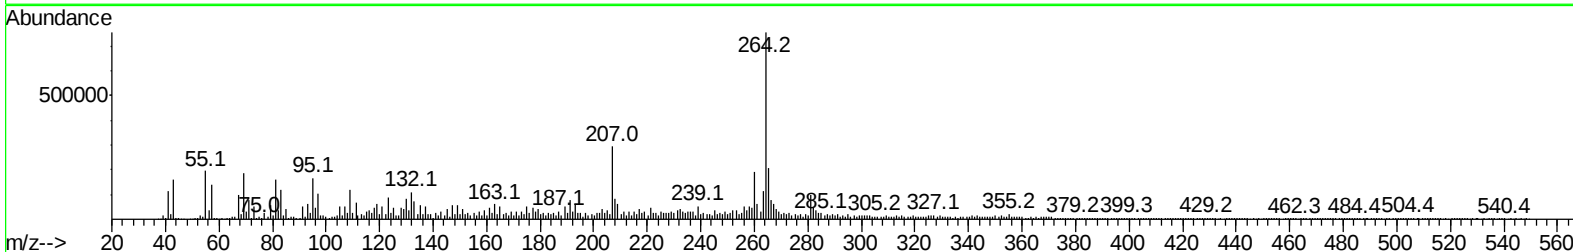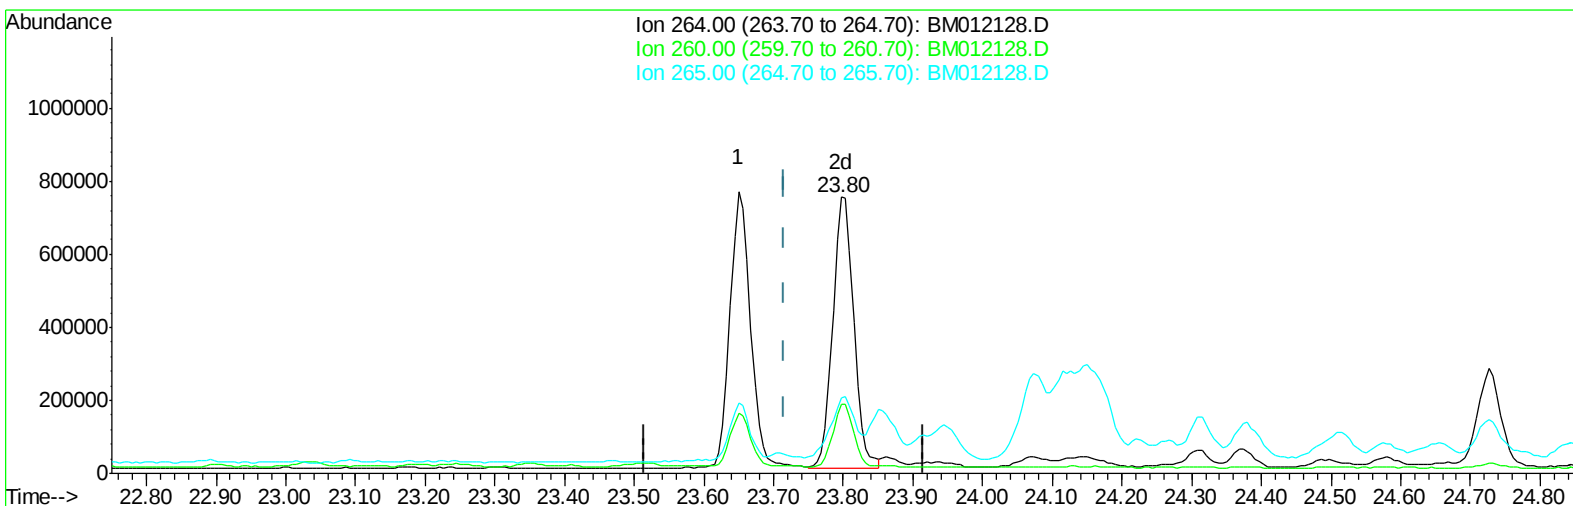

TIC: BM012128.D

(83) Perylene-d12 (I)

23.797min (+0.082) 20.00ng/ul m

response 1557753

Ion	Exp%	Act%
264.00	100	100
260.00	24.20	25.20
265.00	22.50	27.29#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

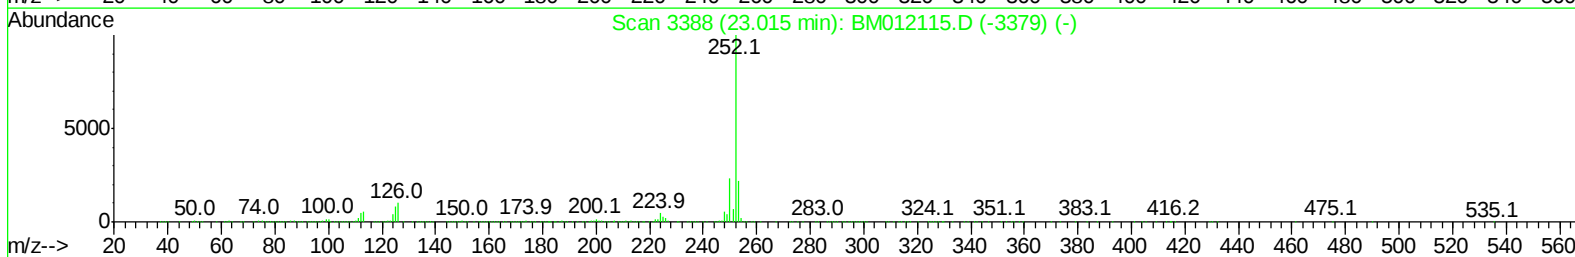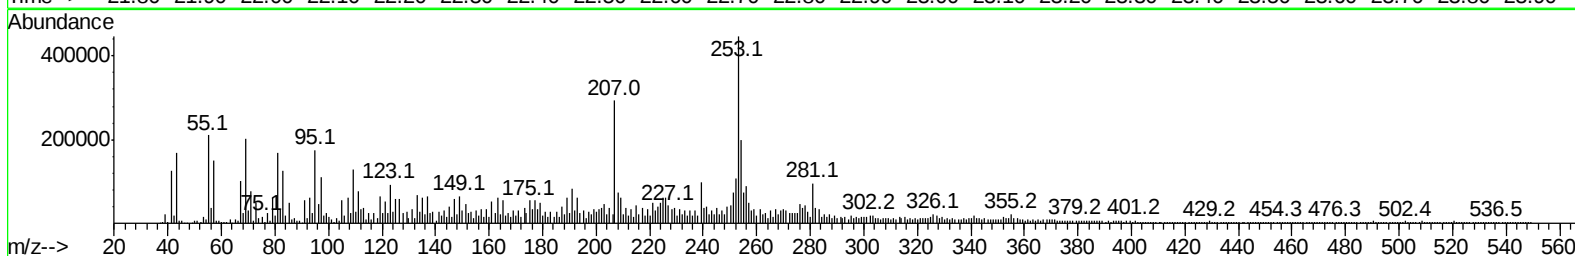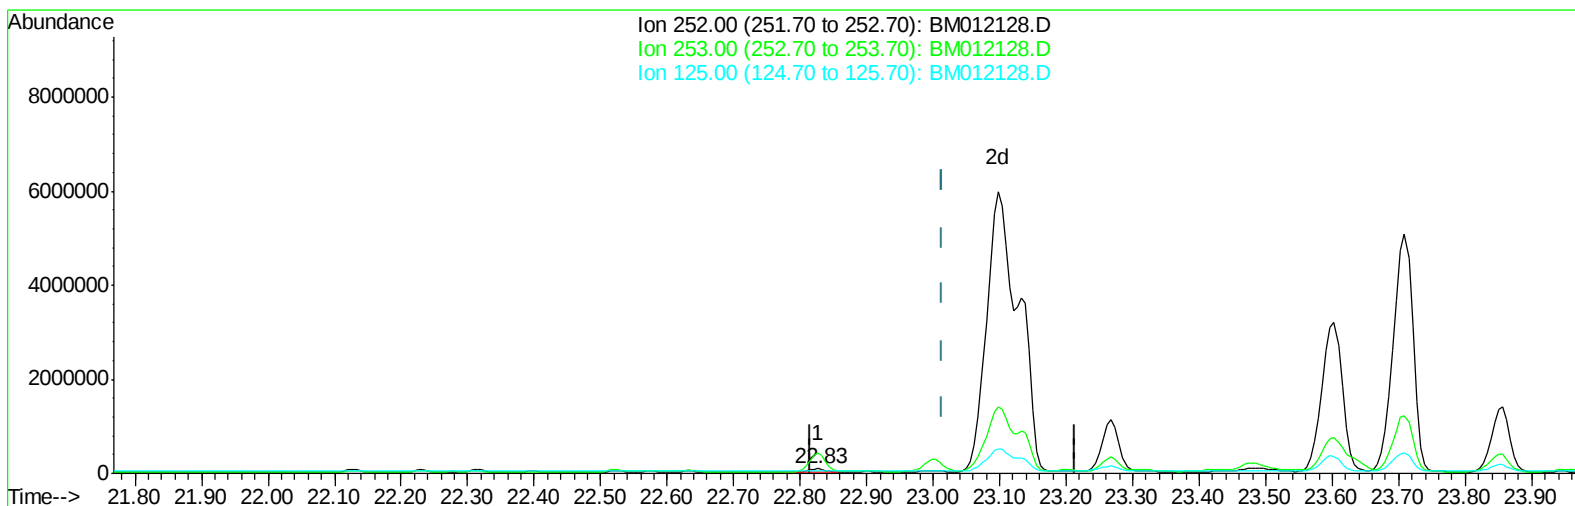

TIC: BM012128.D

(85) Benzo(b)fluoranthene
22.827min (-0.188) 1.43ng/ul
response 145389
Ion Exp% Act%
252.00 100 100
253.00 22.40 410.47#
125.00 4.50 54.48#
0.00 0.00 0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

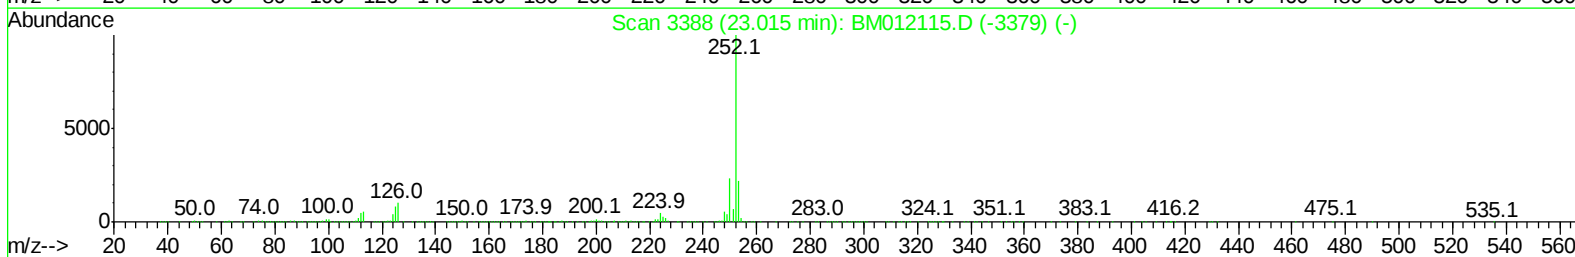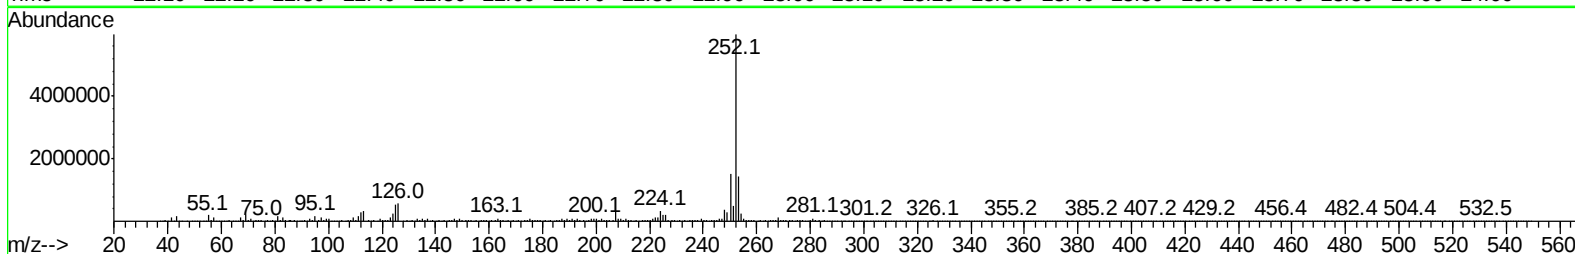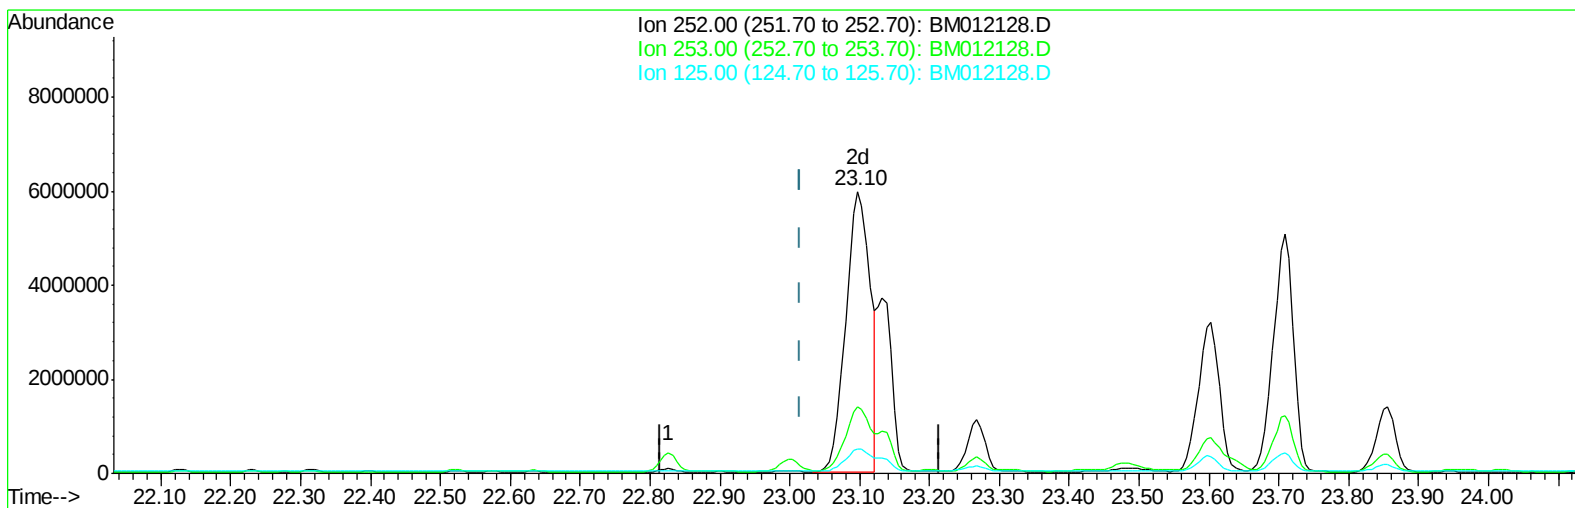

TIC: BM012128.D

(85) Benzo(b)fluoranthene

23.097min (+0.082) 143.09ng/ul m

response 14545585

Ion	Exp%	Act%
252.00	100	100
253.00	22.40	23.79
125.00	4.50	8.70#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

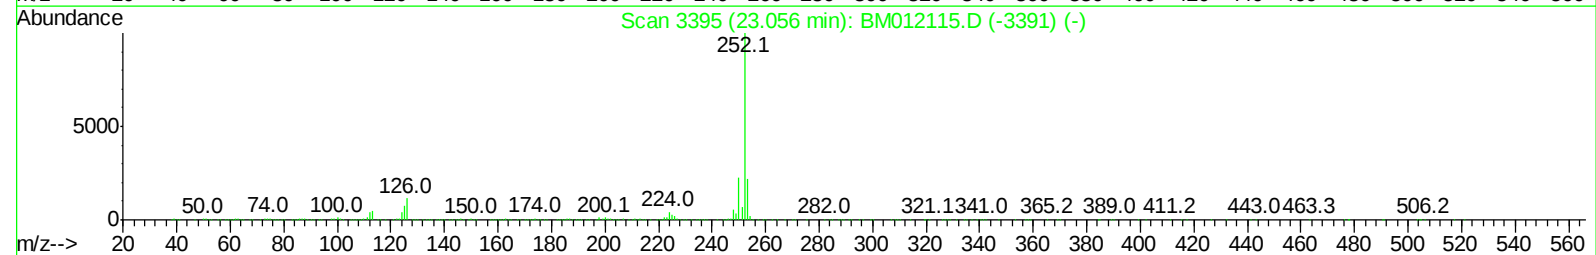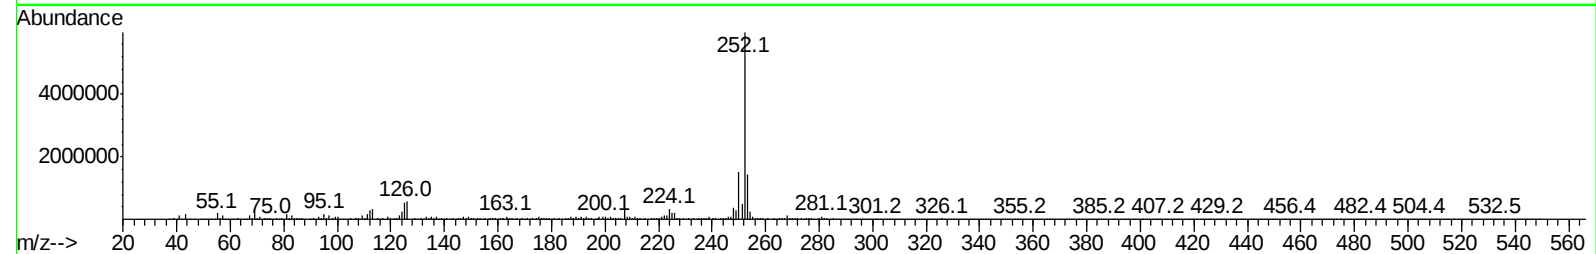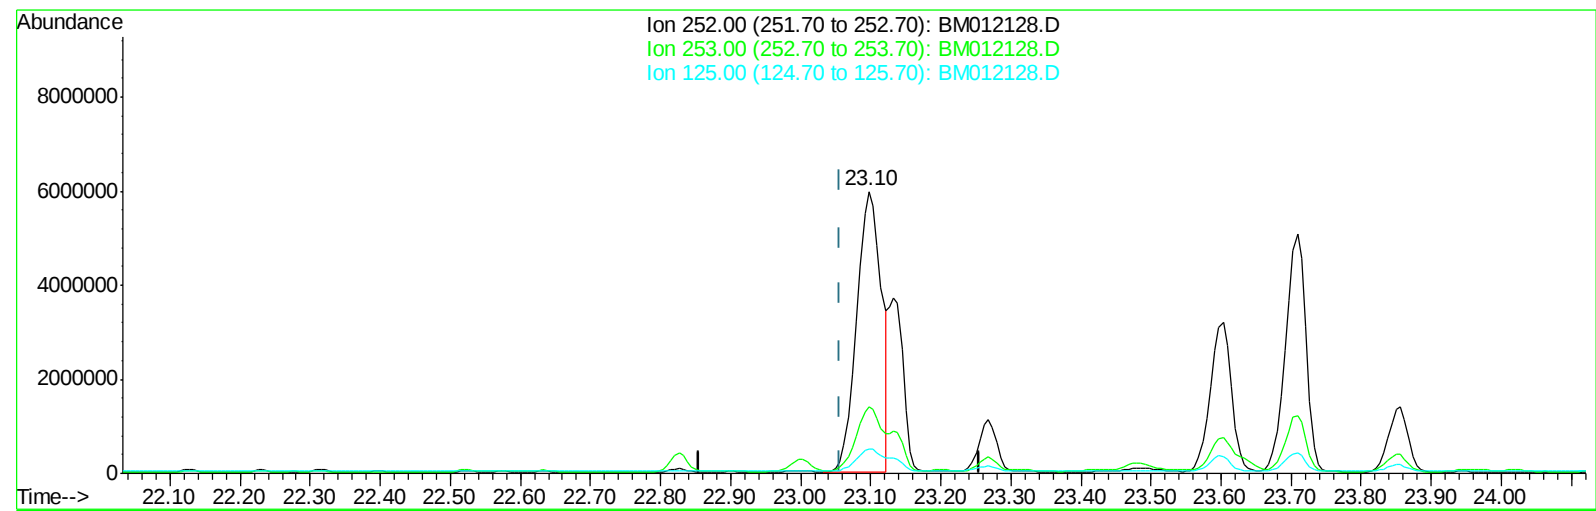

TIC: BM012128.D

(86) Benzo(k)fluoranthene

23.097min (+0.041) 147.67ng/ul

response 14466641

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.79
125.00	4.30	8.70#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

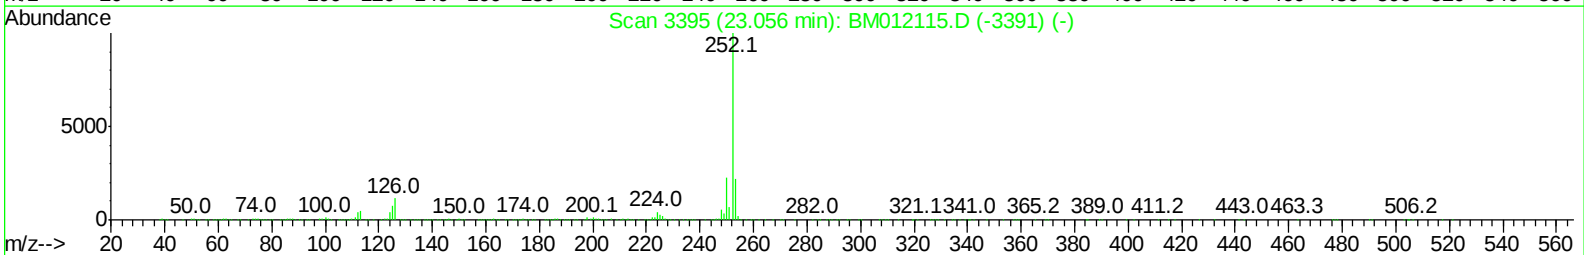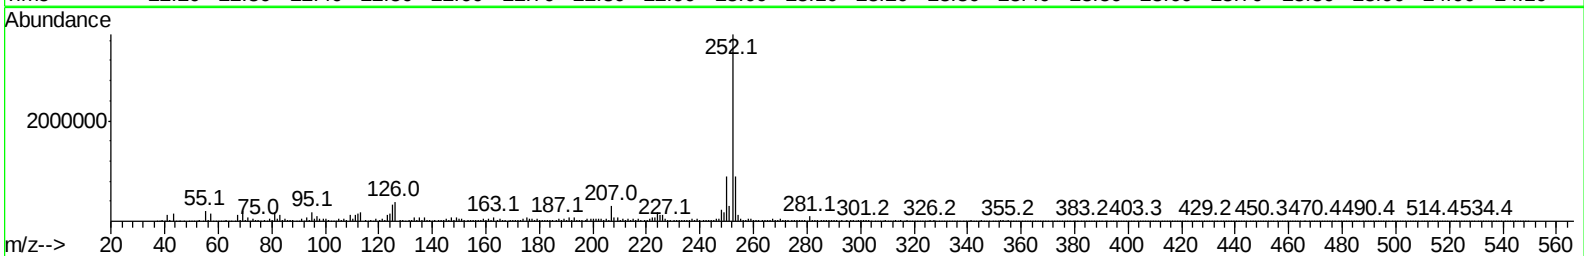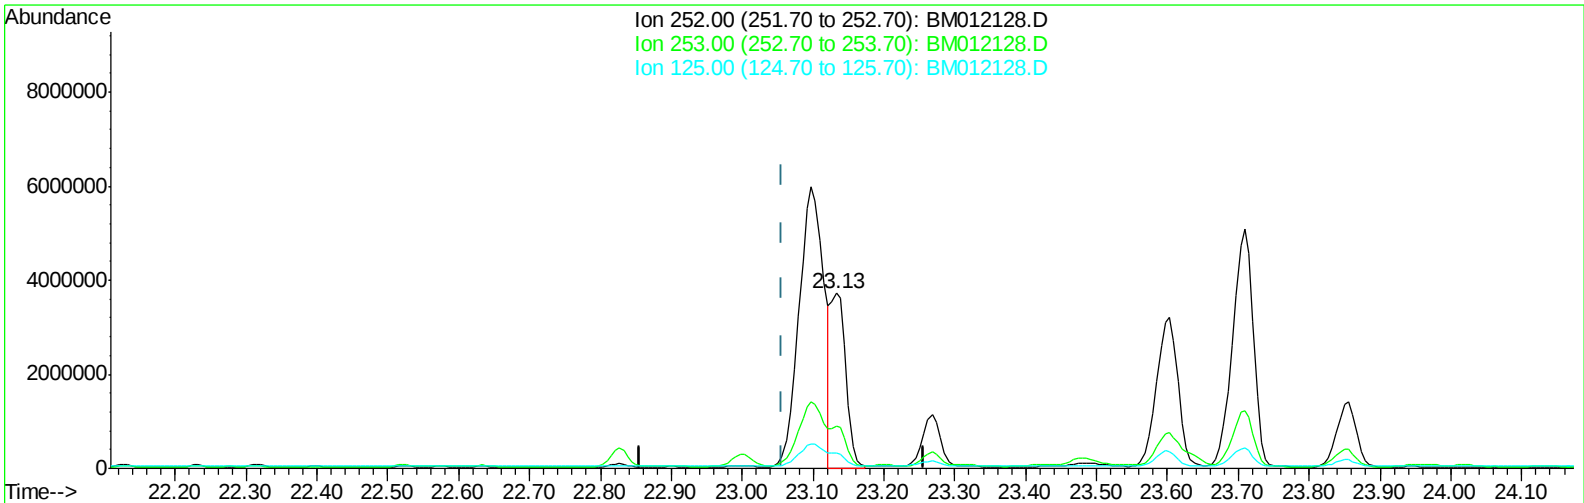

TIC: BM012128.D

(86) Benzo(k)fluoranthene

23.133min (+0.076) 55.78ng/ul m

response 5464707

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.26
125.00	4.30	8.64#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

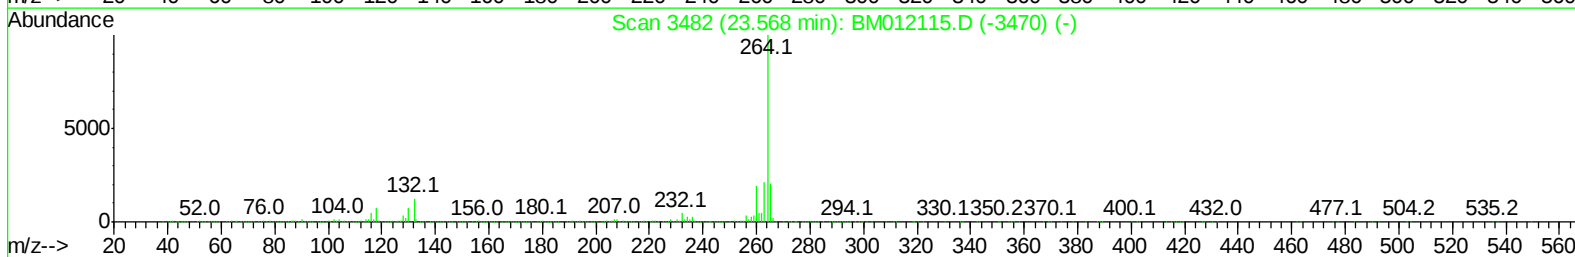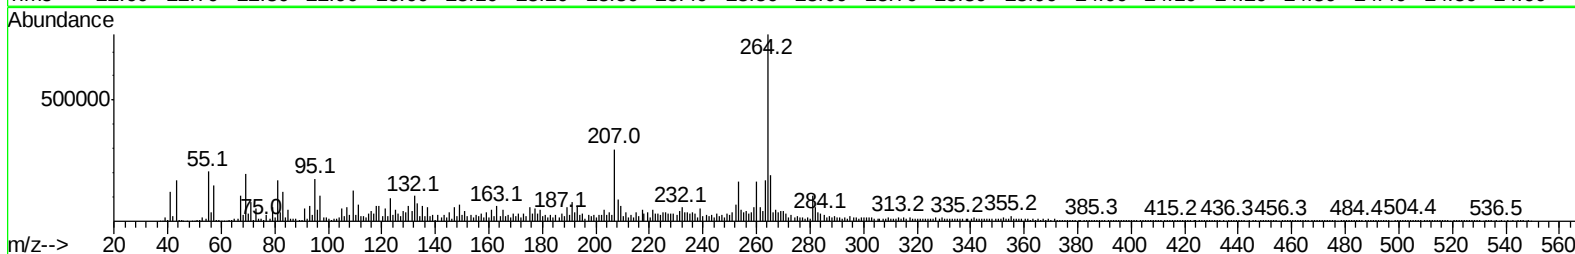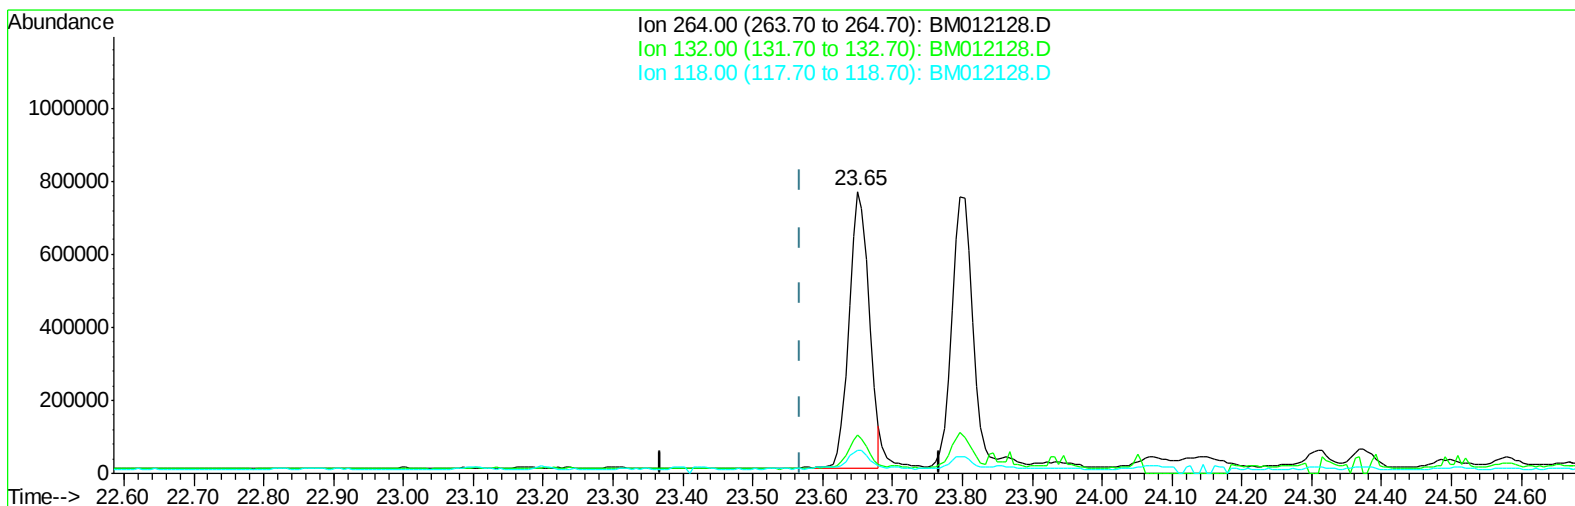

TIC: BM012128.D

(87) Benzo(a)pyrene-d12 (S)

23.650min (+0.082) 19.99ng/ul

response 1500911

Ion	Exp%	Act%
264.00	100	100
132.00	7.70	13.59#
118.00	5.30	8.32#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

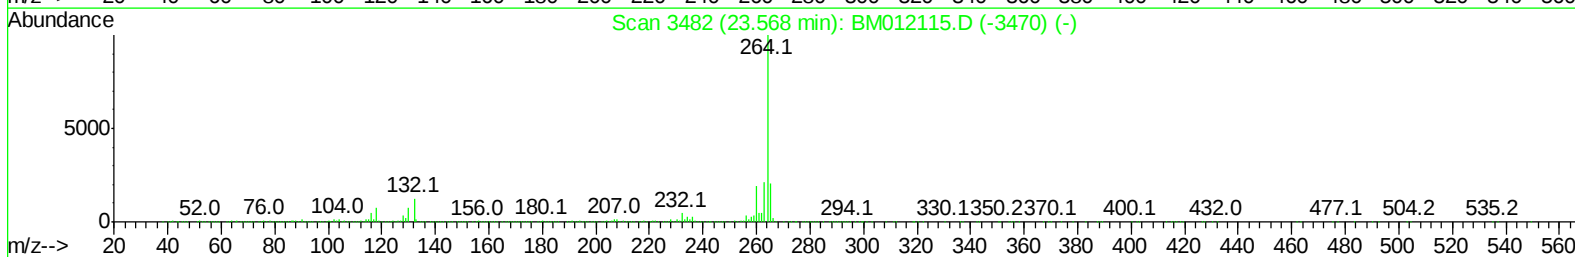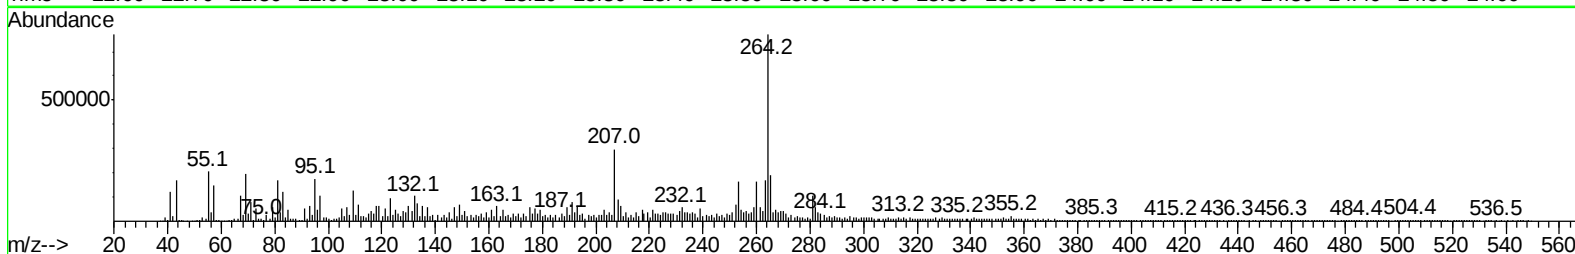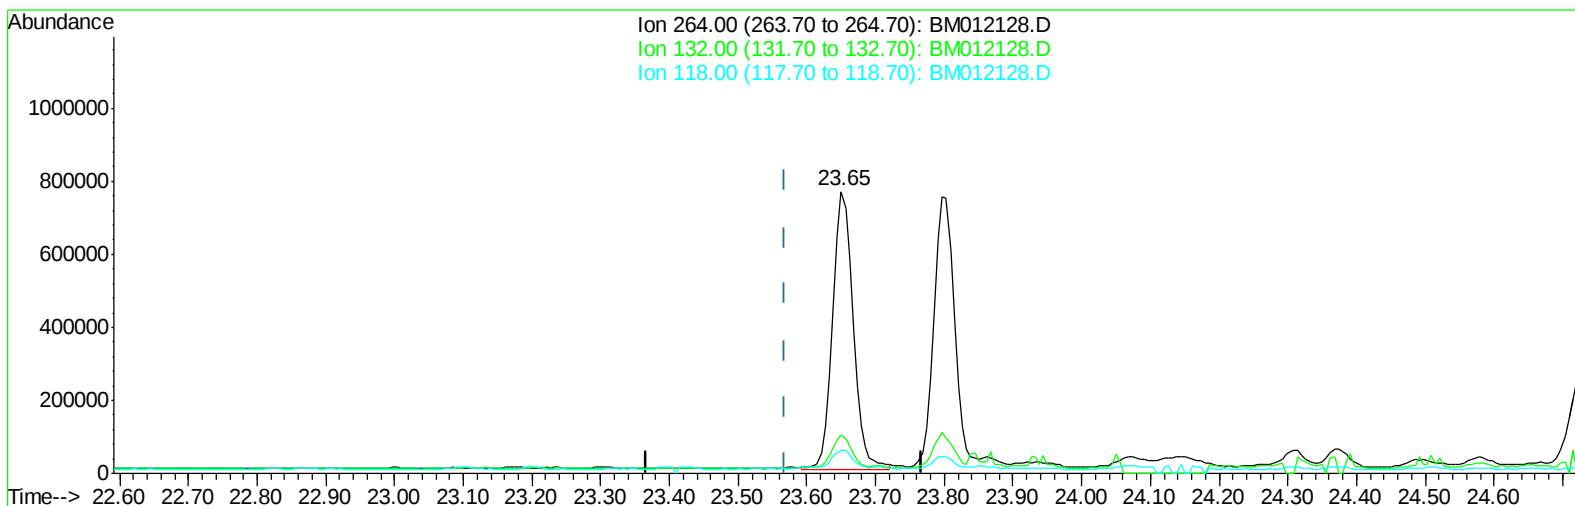

TIC: BM012128.D

(87) Benzo(a)pyrene-d12 (S)

23.650min (+0.082) 21.03ng/ul m

response 1579497

Ion	Exp%	Act%
264.00	100	100
132.00	7.70	13.59#
118.00	5.30	8.32#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

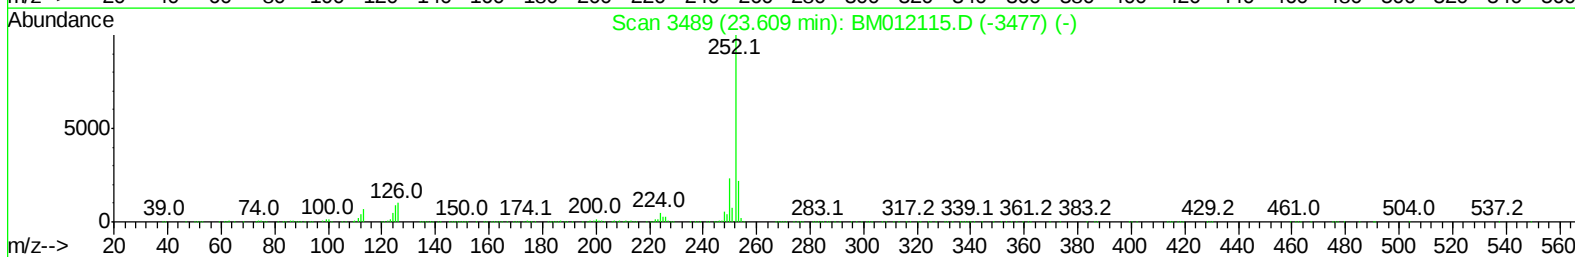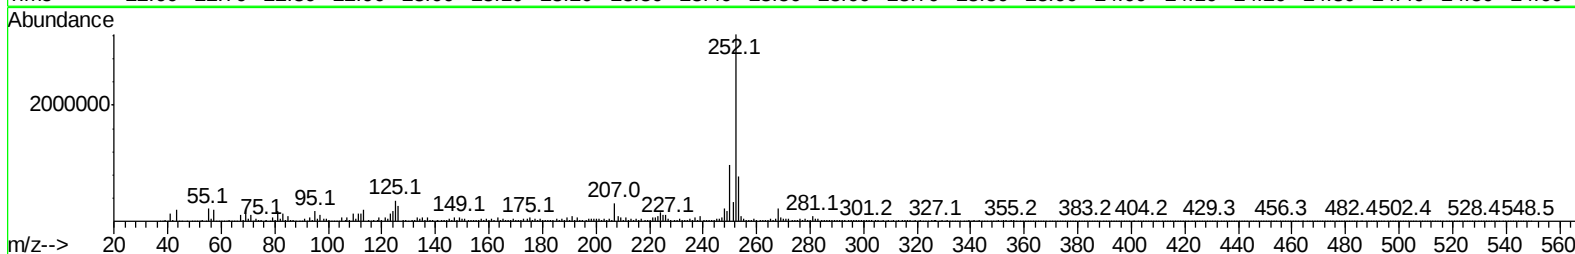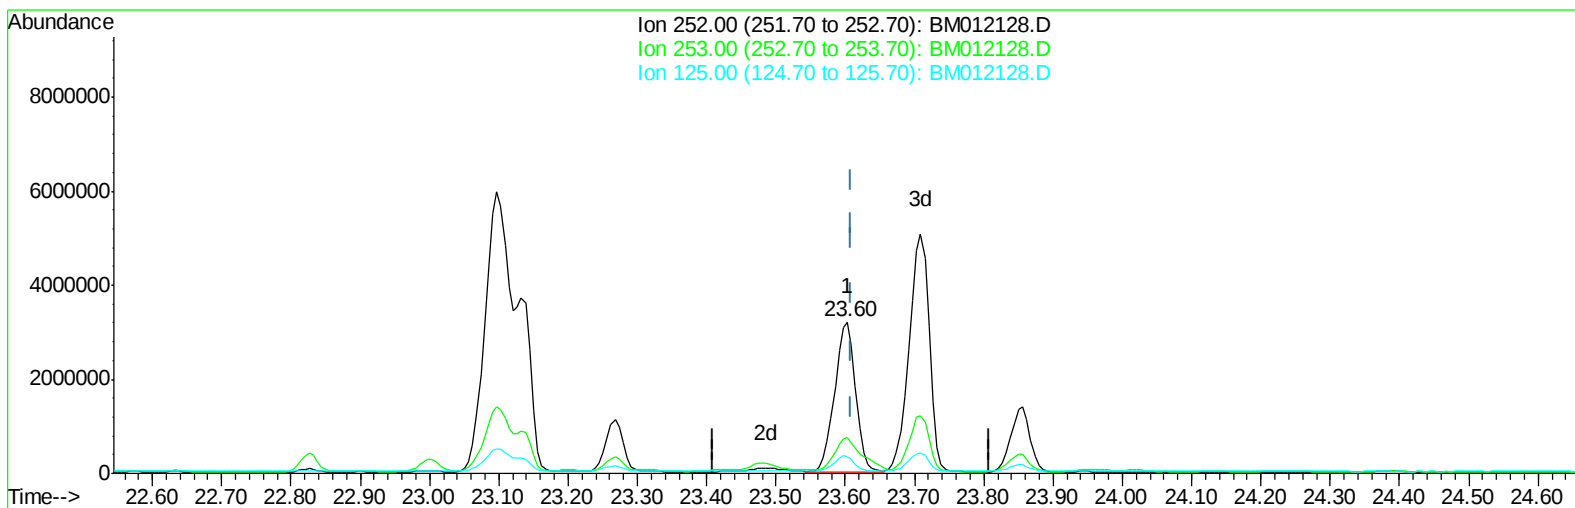

TIC: BM012128.D

(88) Benzo(a)pyrene (C)

23.603min (-0.006) 70.03ng/ul

response 6709932

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	23.72
125.00	5.00	11.30#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:52:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

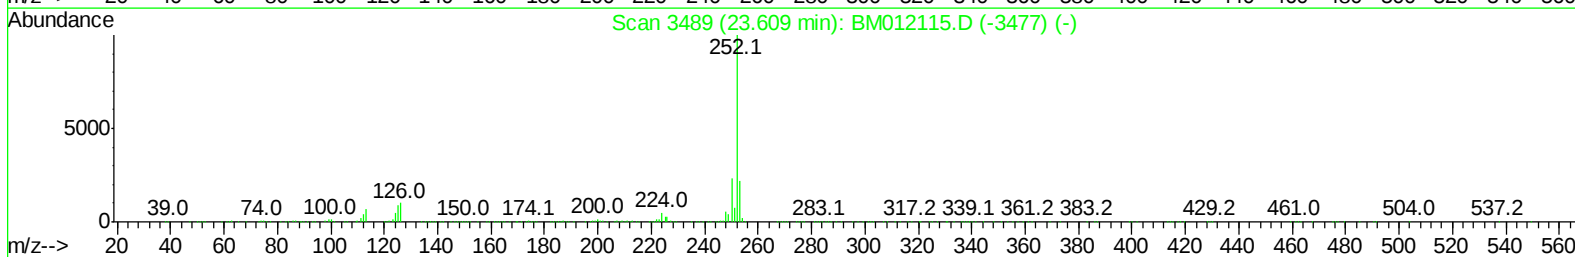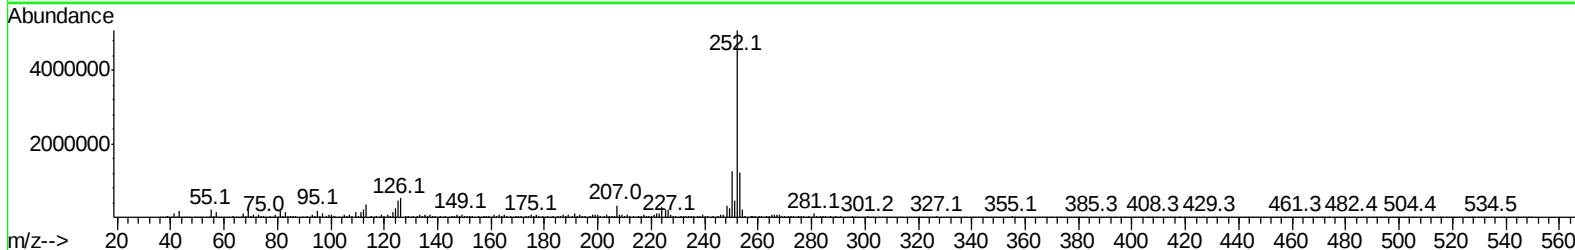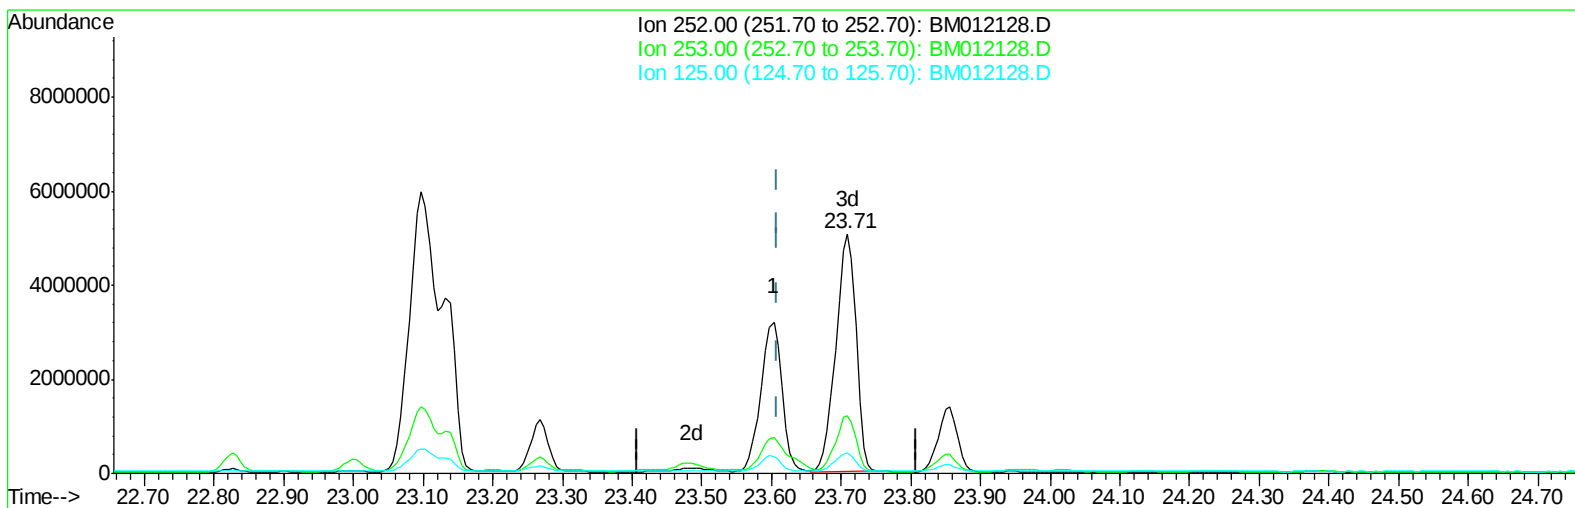

TIC: BM012128.D

(88) Benzo(a)pyrene (C)

23.709min (+0.100) 106.10ng/ul m

response 10166029

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	24.20
125.00	5.00	8.72#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:56:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

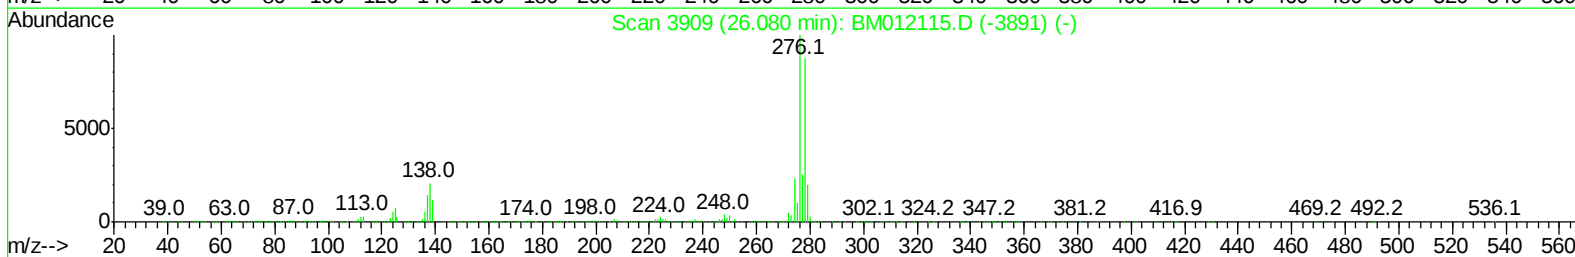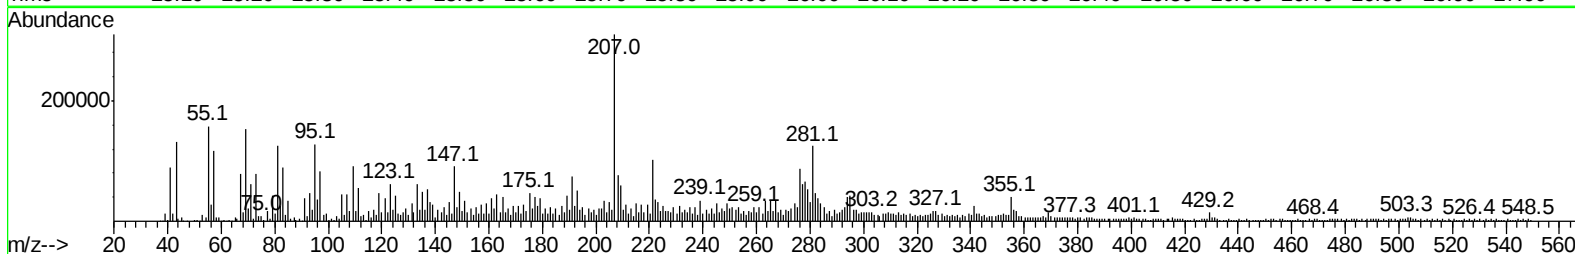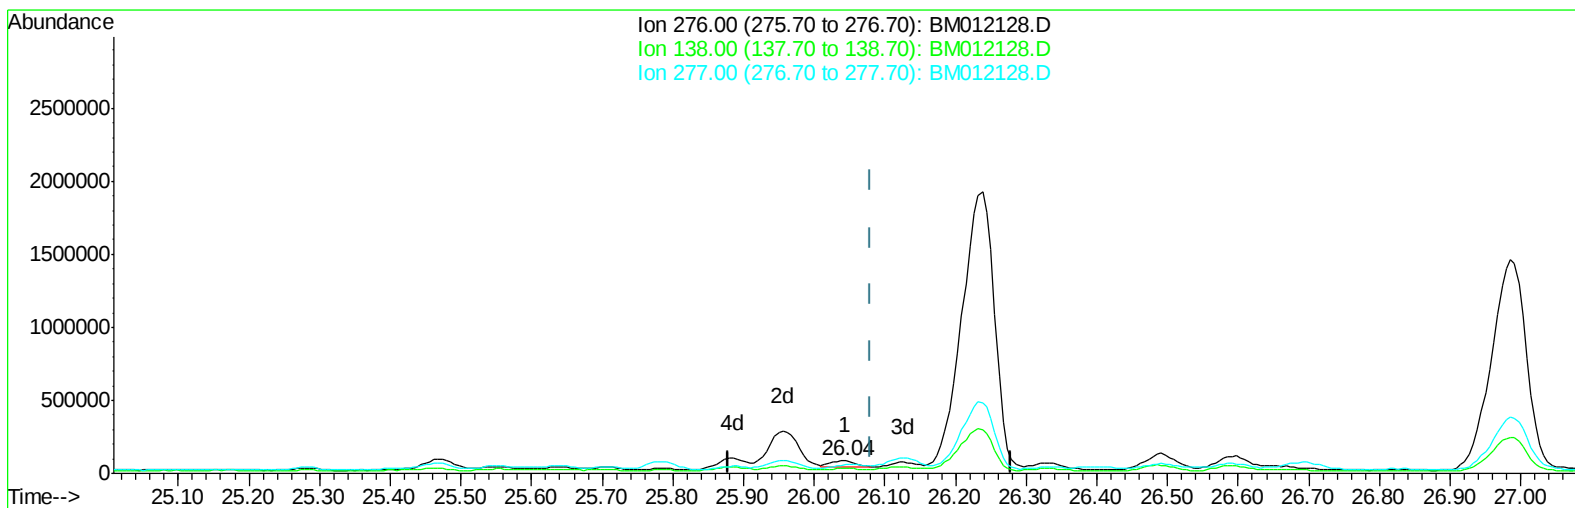

TIC: BM012128.D

(89) Indeno(1,2,3-cd)pyrene

26.044min (-0.035) 1.10ng/ul

response 112369

Ion	Exp%	Act%
276.00	100	100
138.00	11.60	37.47#
277.00	24.90	70.37#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:56:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

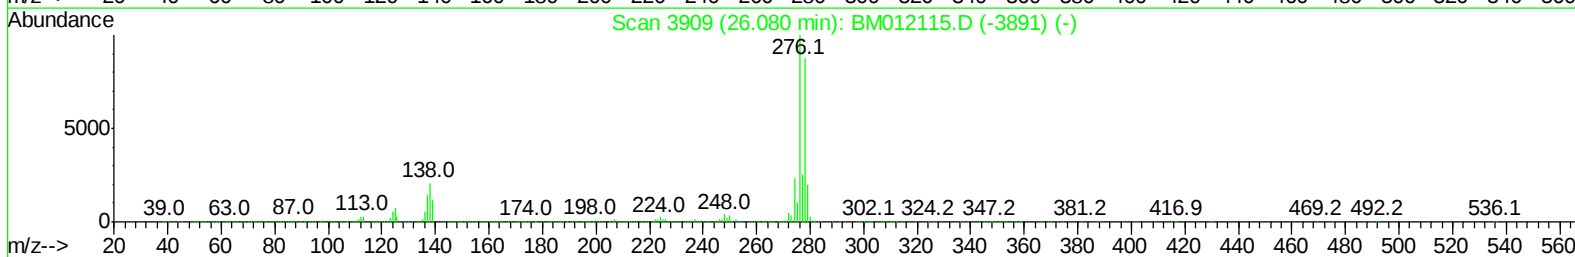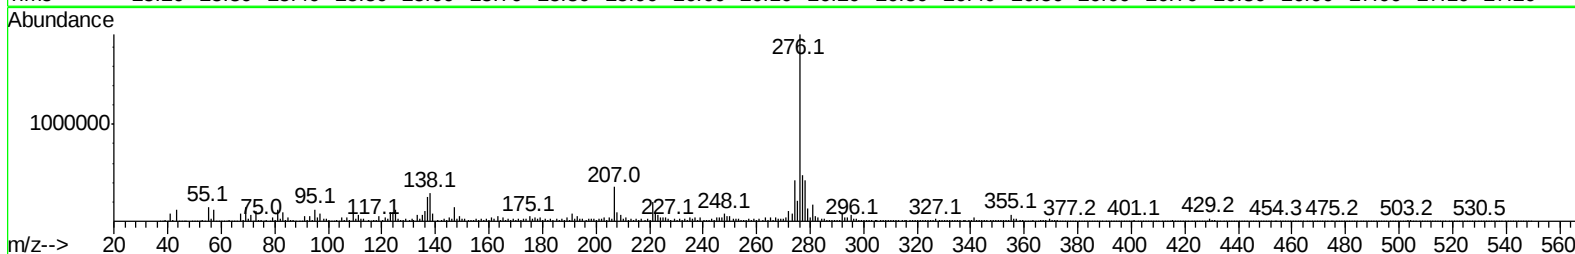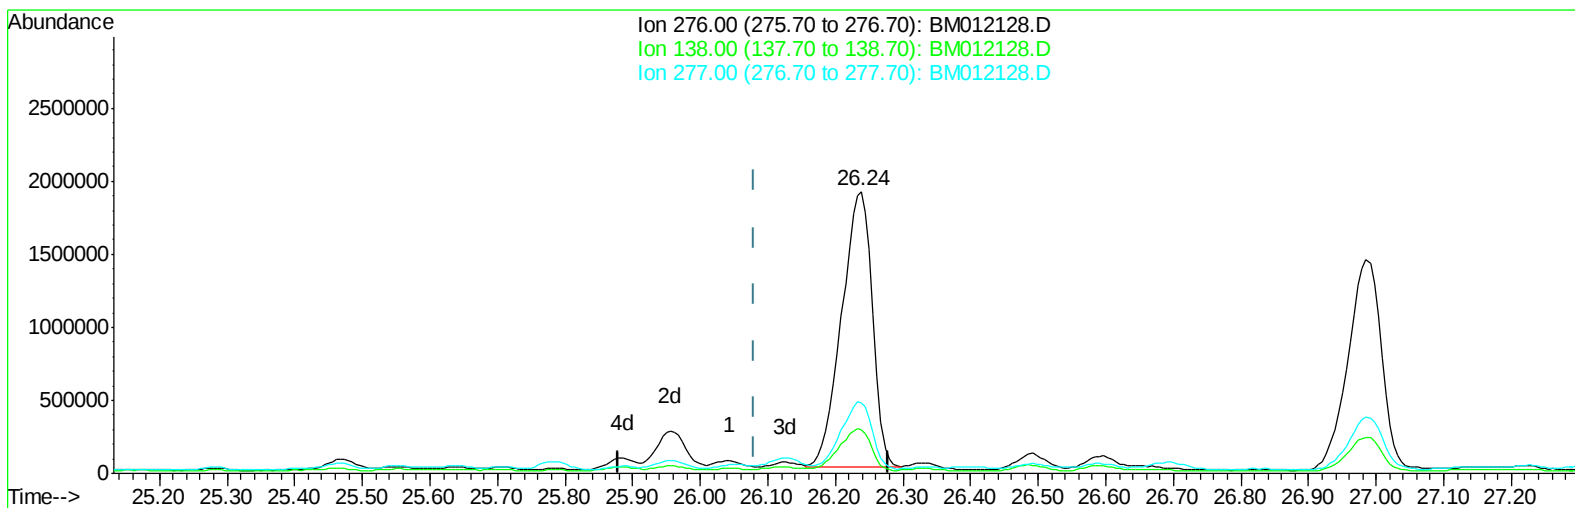

TIC: BM012128.D

(89) Indeno(1,2,3-cd)pyrene

26.238min (+0.159) 59.08ng/ul m

response 6011238

Ion	Exp%	Act%
276.00	100	100
138.00	11.60	15.31#
277.00	24.90	25.00
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:56:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

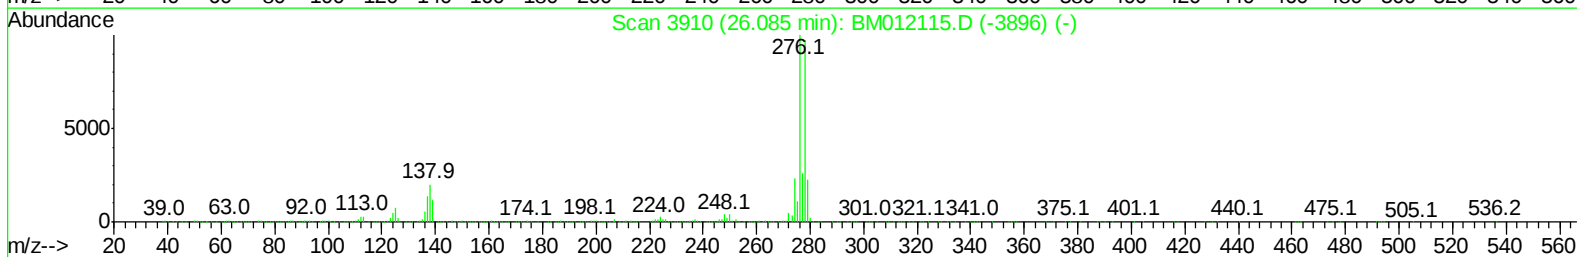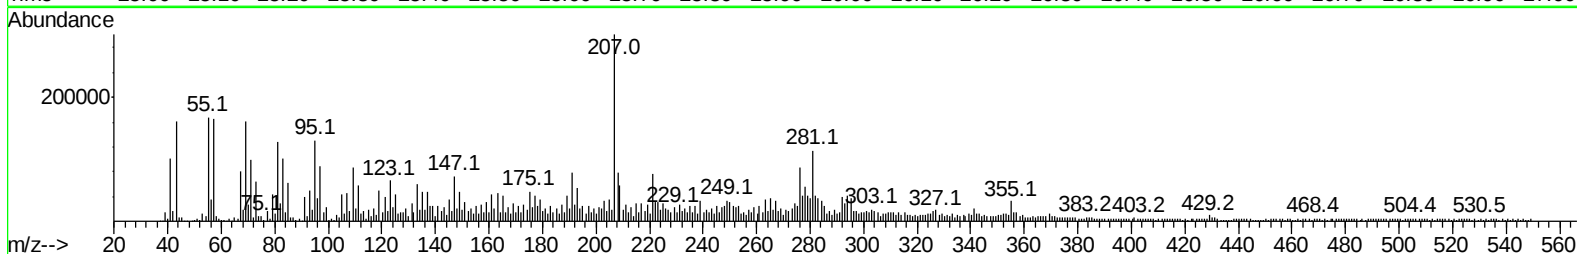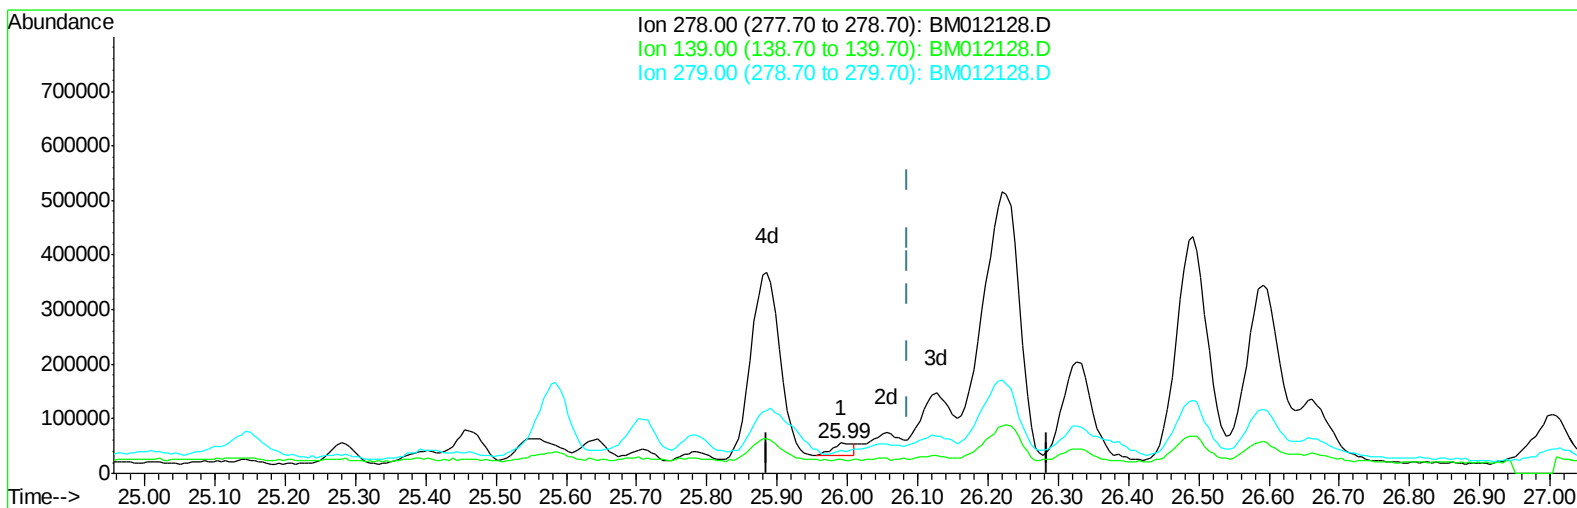

TIC: BM012128.D

(90) Dibenzo(a,h)anthracene

25.991min (-0.094) 0.50ng/ul

response 42951

Ion	Exp%	Act%
278.00	100	100
139.00	7.30	44.85#
279.00	23.20	74.50#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:56:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

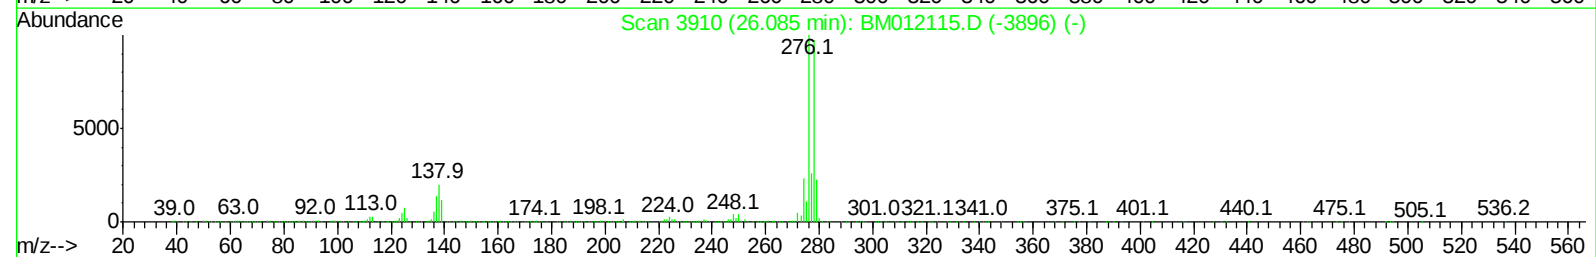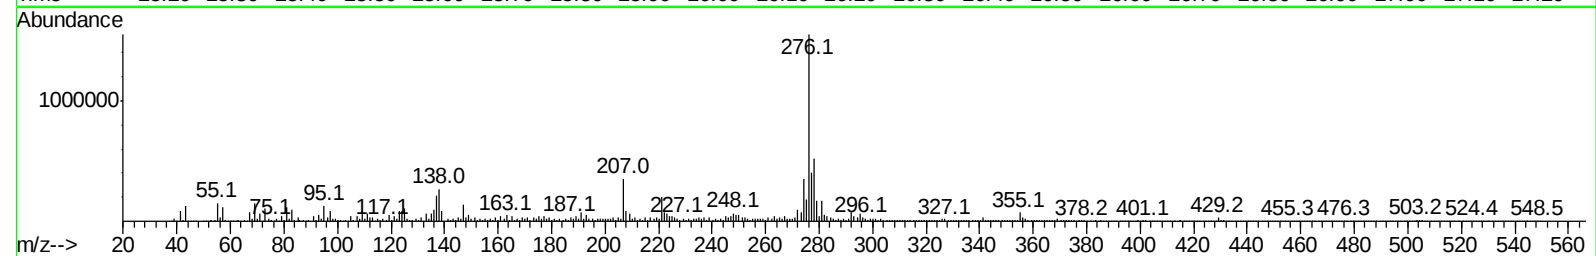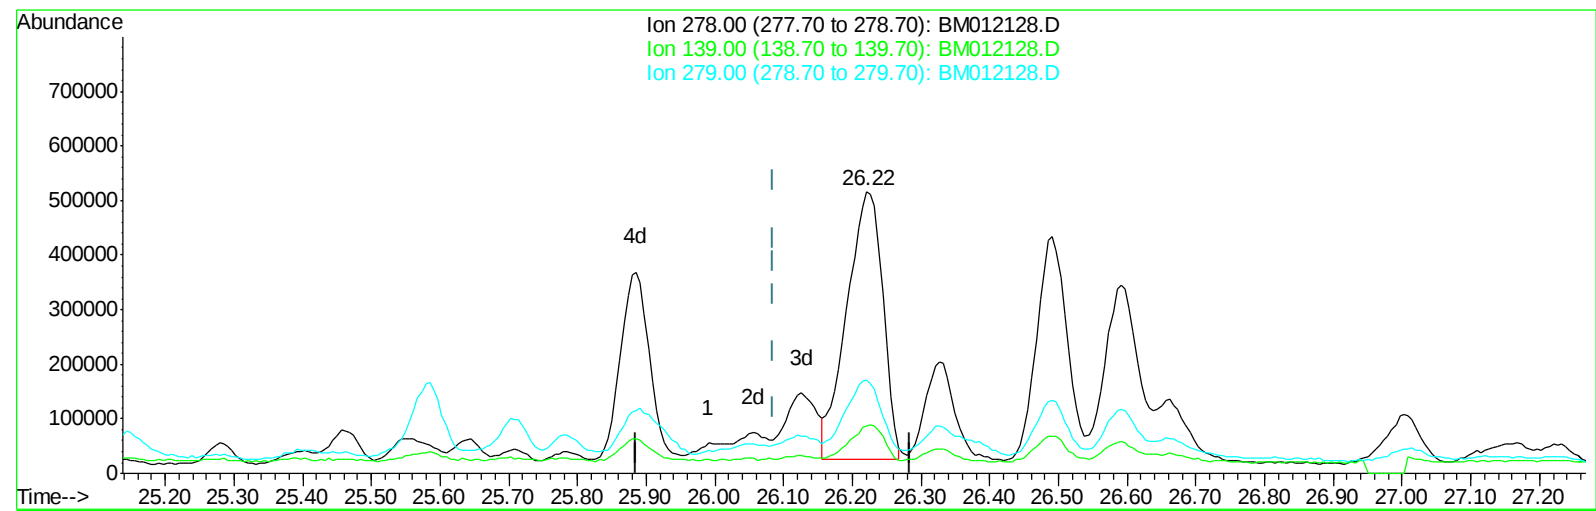

TIC: BM012128.D

(90) Dibenzo(a,h)anthracene

26.221min (+0.135) 20.93ng/ul m

response 1789788

Ion	Exp%	Act%
278.00	100	100
139.00	7.30	17.03#
279.00	23.20	33.34#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:56:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

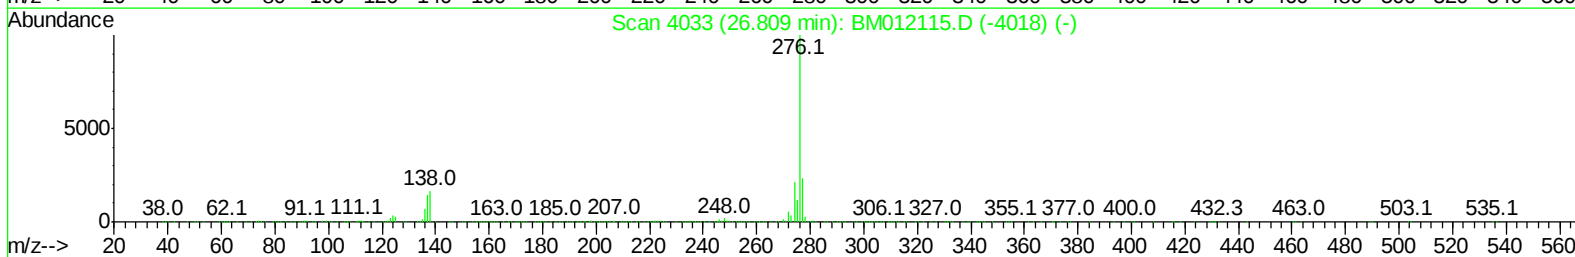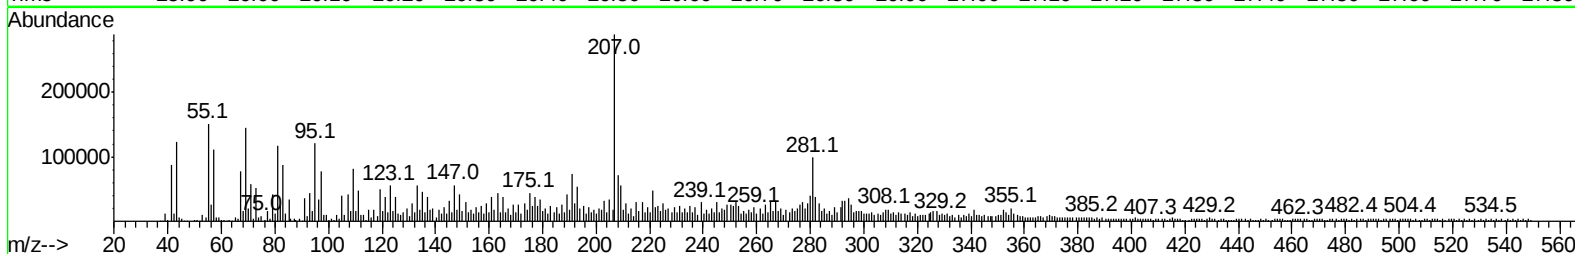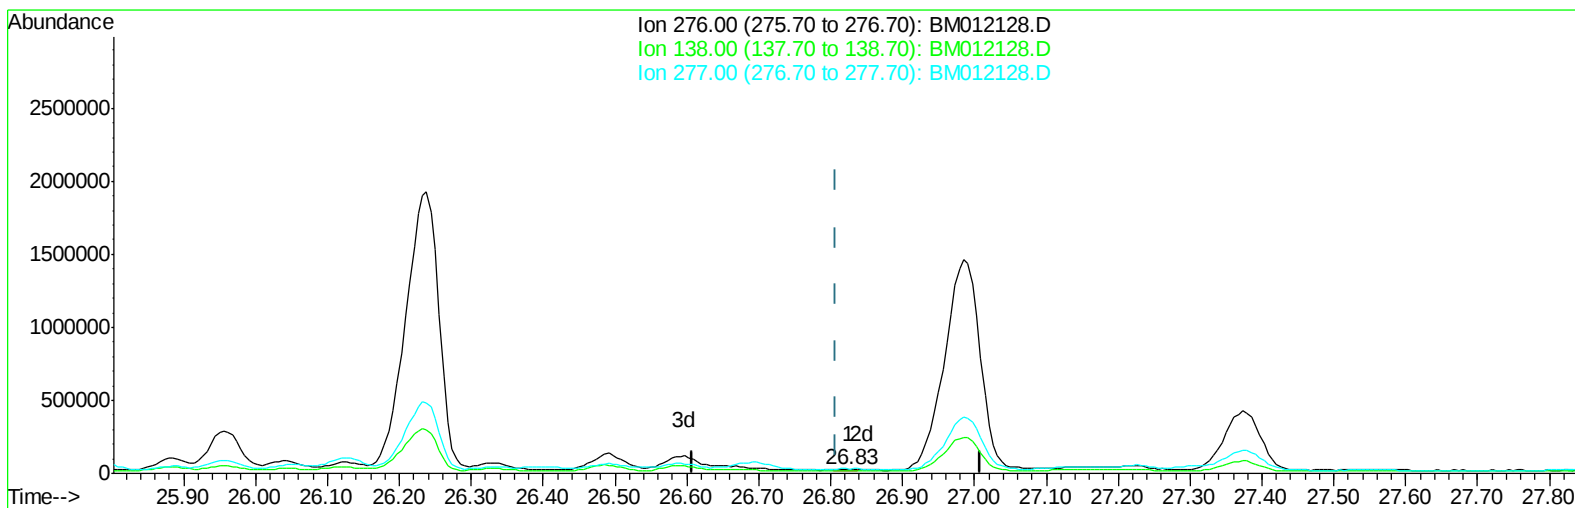

TIC: BM012128.D

(91) Benzo(g,h,i)perylene

26.826min (+0.017) 0.08ng/ul

response 6885

Ion	Exp%	Act%
276.00	100	100
138.00	10.60	67.31#
277.00	23.30	119.64#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:56:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

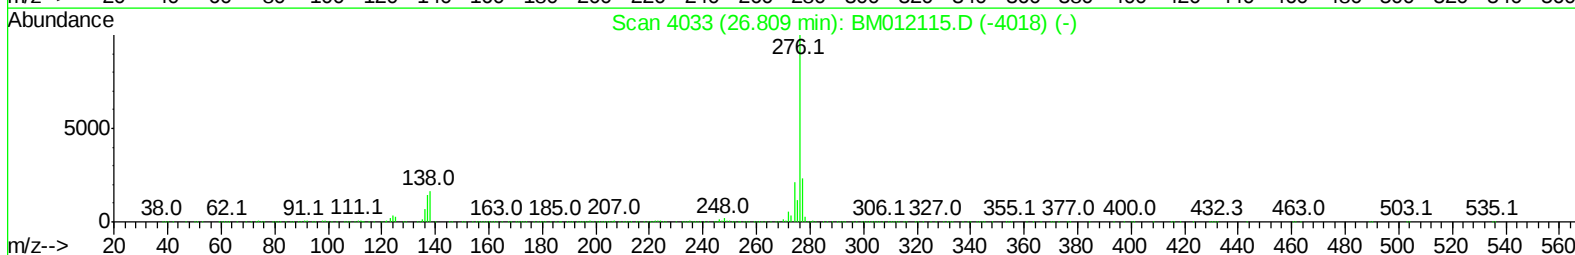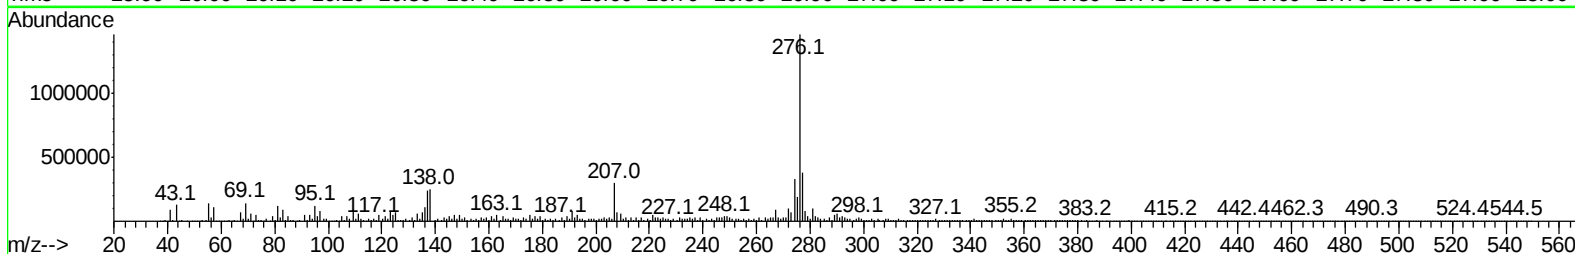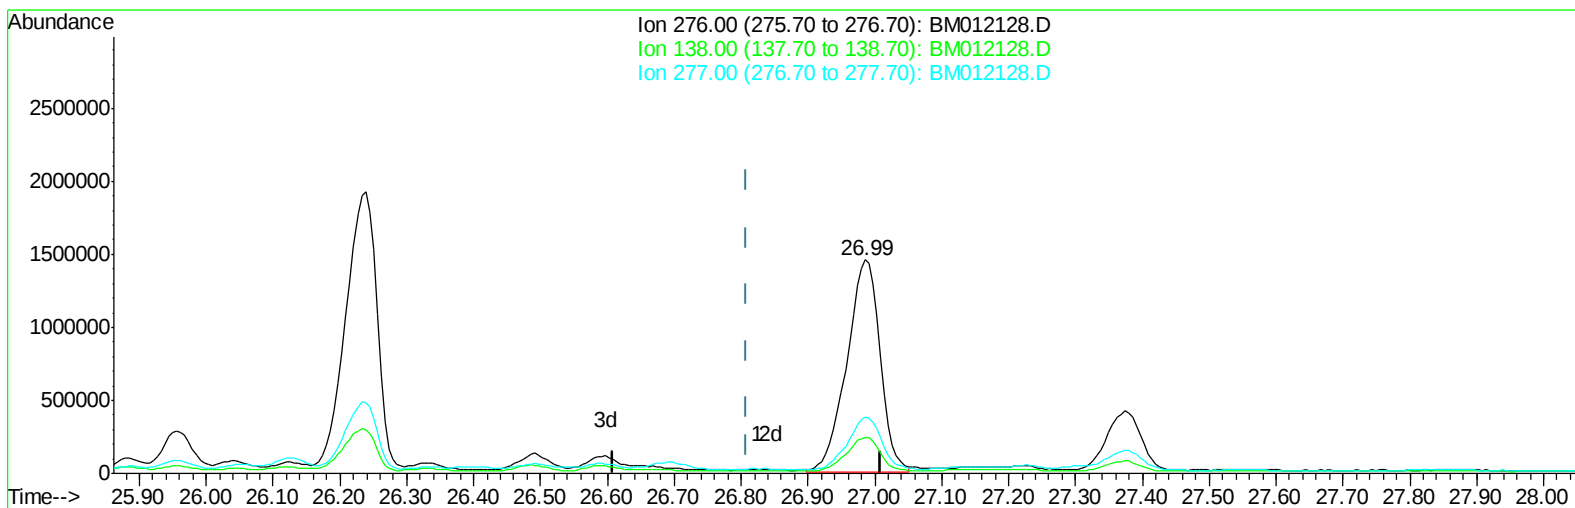

TIC: BM012128.D

(91) Benzo(g,h,i)perylene

26.985min (+0.176) 60.92ng/ul m

response 5076462

Ion	Exp%	Act%
276.00	100	100
138.00	10.60	16.84#
277.00	23.30	26.13
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
 Data File : BM012128.D
 Acq On : 13 Oct 2017 08:51
 Operator : SJ/JU
 Sample : I5568-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-29(0-1)-092917

Manual Integrations
 APPROVED

Sohil
 6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:58:10 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 13 04:53:53 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	296115	20.00	ng/ul	0.02
18) Naphthalene-d8	10.66	136	1143895	20.00	ng/ul	0.02
35) Acenaphthene-d10	14.51	164	573334	20.00	ng/ul	0.03
61) Phenanthrene-d10	17.26	188	1064346	20.00	ng/ul	0.03
75) Chrysene-d12	21.45	240	1501423	20.00	ng/ul	0.05
83) Perylene-d12	23.80	264	1557753m	20.00	ng/ul	0.08

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	18496	2.97	ng/uL	0.01
5) Phenol-d5	7.03	99	410235	17.07	ng/ul	0.04
7) Bis-(2-Chloroethyl)ether-d	7.17	67	255120	17.71	ng/ul	0.02
9) 2-Chlorophenol-d4	7.39	132	368355	18.08	ng/ul	0.03
13) 4-Methylphenol-d8	8.57	113	355576	17.19	ng/ul	0.03
19) Nitrobenzene-d5	9.02	128	176111	20.17	ng/ul	0.02
22) 2-Nitrophenol-d4	9.75	143	157898	15.48	ng/ul	0.03
26) 2,4-Dichlorophenol-d3	10.29	165	364009	18.69	ng/ul	0.04
29) 4-Chloroaniline-d4	10.80	131	252757	13.87	ng/ul	0.02
43) Dimethylphthalate-d6	13.91	166	1074733	21.21	ng/ul	0.02
46) Acenaphthylene-d8	14.20	160	1268012	20.67	ng/ul	0.03
51) 4-Nitrophenol-d4	14.74	143	81192	10.66	ng/ul	0.06
57) Fluorene-d10	15.50	176	814848	19.59	ng/ul	0.03
62) 4,6-Dinitro-2-methylphenol	15.66	200	268	0.04	ng/ul	0.05
70) Anthracene-d10	17.36	188	1134138	21.55	ng/ul	0.04
76) Pyrene-d10	19.66	212	1321469	17.34	ng/ul	0.04
87) Benzo(a)pyrene-d12	23.65	264	1579497m	21.03	ng/ul	0.08

Target Compounds

					Ovalue	
6) Phenol	7.06	94	53974	2.173	ng/ul#	86
11) 2-Methylphenol	8.30	108	46564	2.493	ng/ul	100
28) Naphthalene	10.71	128	88602	1.497	ng/ul	98
44) Dimethylphthalate	13.96	163	668443	13.167	ng/ul	99
49) Acenaphthene	14.57	153	189383	4.668	ng/ul	98
53) Dibenzofuran	14.90	168	94601	1.619	ng/ul	98
58) Fluorene	15.56	166	160207	3.302	ng/ul	96
69) Phenanthrene	17.30	178	2807880	46.375	ng/ul	98
71) Anthracene	17.39	178	924983	14.757	ng/ul	99
72) Carbazole	17.66	167	141850	2.674	ng/ul#	94
74) Fluoranthene	19.33	202	12145606	166.220	ng/ul#	88
77) Pyrene	19.69	202	11294931	113.911	ng/ul#	91
80) Benzo(a)anthracene	21.43	228	11108085	113.700	ng/ul	94
81) Bis(2-ethylhexyl)phthalate	21.32	149	232452	3.510	ng/ul#	93
82) Chrysene	21.49	228	9590866m	104.563	ng/ul	
85) Benzo(b)fluoranthene	23.10	252	14545585m	143.086	ng/ul	
86) Benzo(k)fluoranthene	23.13	252	5464707m	55.782	ng/ul	
88) Benzo(a)pyrene	23.71	252	10166029m	106.103	ng/ul	
89) Indeno(1,2,3-cd)pyrene	26.24	276	6011238m	59.080	ng/ul	
90) Dibenz(a,h)anthracene	26.22	278	1789788m	20.925	ng/ul	
91) Benzo(a,h,i)perylene	26.99	276	5076462m	60.917	ng/ul	

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:58:10 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM101217\
Data File : BM012128.D
Acq On : 13 Oct 2017 08:51
Operator : SJ/JU
Sample : I5568-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-29(0-1)-092917

Manual Integrations
APPROVED

Sohil
6/22/2018 4:49:03 PM

Quant Time: Oct 13 23:58:10 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 13 04:53:53 2017
Response via : Initial Calibration

