

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
 Data File : BM042282.D
 Acq On : 13 Oct 2023 11:51
 Operator : MA/JU
 Sample : PB156220BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	40	rVB	41348	64046	1.40%	0.144%
2	3.799	100	104	124	rBV	590684	967538	21.08%	2.174%
3	4.116	155	158	162	rVB2	6938	8459	0.18%	0.019%
4	7.157	668	675	688	rBV	732563	1124156	24.49%	2.526%
5	7.351	701	708	719	rVB	604424	961248	20.94%	2.160%
6	7.528	731	738	749	rVB	714216	1119376	24.39%	2.515%
7	8.010	812	820	829	rBV	526262	818210	17.83%	1.838%
8	8.716	931	940	955	rBV	903776	1406559	30.65%	3.160%
9	9.204	1016	1023	1037	rBV	712253	1169052	25.47%	2.627%
10	9.922	1137	1145	1155	rBV	599859	943723	20.56%	2.121%
11	10.445	1226	1234	1244	rBV	834842	1362638	29.69%	3.062%
12	10.833	1291	1300	1309	rBV	776988	1253020	27.30%	2.815%
13	10.992	1319	1327	1340	rBV	928079	1560015	33.99%	3.505%
14	12.416	1563	1569	1579	rVB3	11583	22097	0.48%	0.050%
15	13.498	1748	1753	1760	rVB2	9619	15177	0.33%	0.034%
16	14.068	1843	1850	1860	rBV	1792737	2351321	51.23%	5.283%
17	14.357	1892	1899	1910	rBV	1837970	2595656	56.55%	5.832%
18	14.657	1943	1950	1960	rVB	1189283	1720061	37.48%	3.865%
19	14.786	1967	1972	1976	rVB7	3804	5629	0.12%	0.013%
20	14.868	1978	1986	2005	rBV	886769	1308554	28.51%	2.940%
21	15.645	2111	2118	2125	rBV	2321847	3255859	70.94%	7.316%
22	15.774	2134	2140	2151	rBV	920773	1163703	25.35%	2.615%
23	15.886	2153	2159	2164	rVB6	8487	12796	0.28%	0.029%
24	17.409	2411	2418	2424	rBV	1479015	2078387	45.28%	4.670%
25	17.509	2427	2435	2450	rBV	2533910	3579332	77.99%	8.043%
26	18.251	2558	2561	2566	rBV6	4994	7253	0.16%	0.016%
27	19.362	2746	2750	2754	rVB	24819	32975	0.72%	0.074%
28	19.433	2757	2762	2766	rBV	31804	40356	0.88%	0.091%
29	19.521	2775	2777	2782	rBV6	5141	7526	0.16%	0.017%
30	19.668	2800	2802	2806	rBV5	9550	10256	0.22%	0.023%
31	19.798	2818	2824	2835	rBV	3223231	4291543	93.50%	9.643%
32	21.592	3124	3129	3137	rBV	1845389	2249972	49.02%	5.056%
33	23.909	3515	3523	3534	rVB	2331180	4589752	100.00%	10.313%
34	24.068	3543	3550	3561	rBV	1202033	2408286	52.47%	5.411%

Sum of corrected areas: 44504531

Instrument :

BNA_M

ClientSampleId :




SBLK220

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042282.D
Acq On : 13 Oct 2023 11:51
Operator : MA/JU
Sample : PB156220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

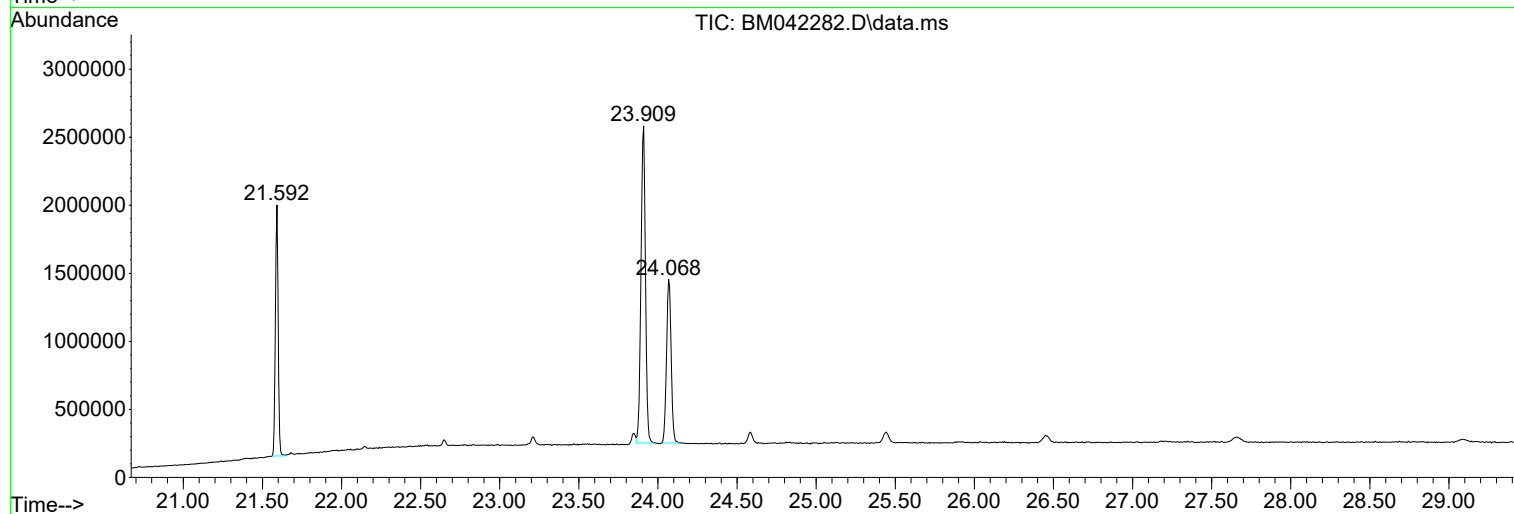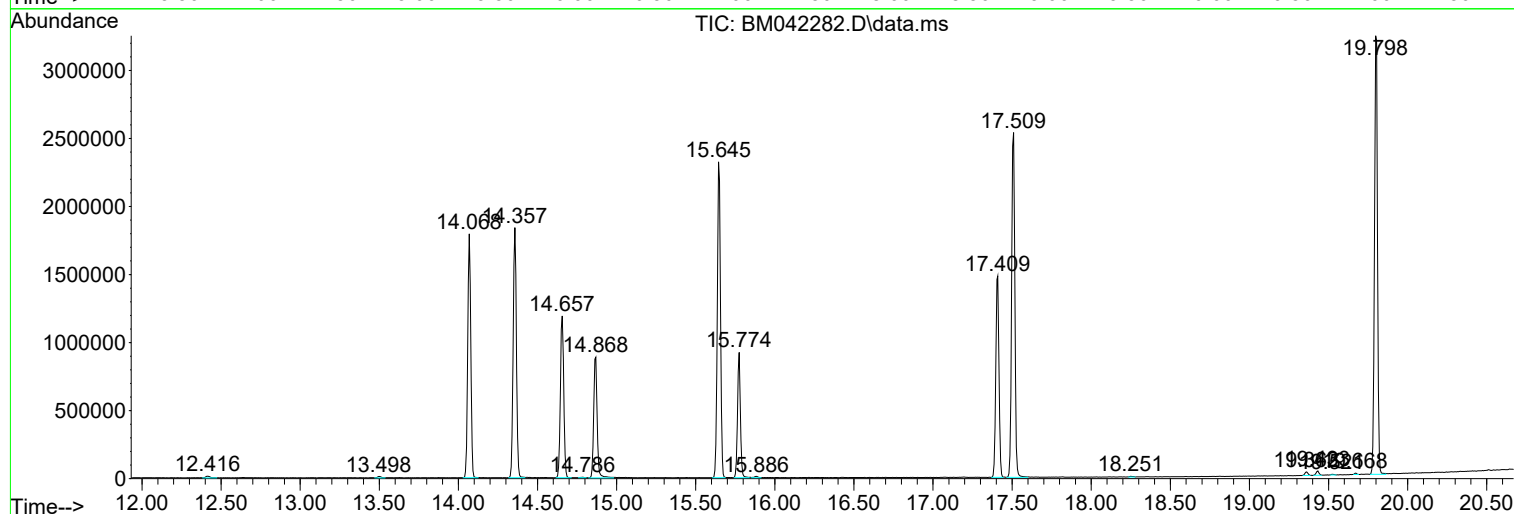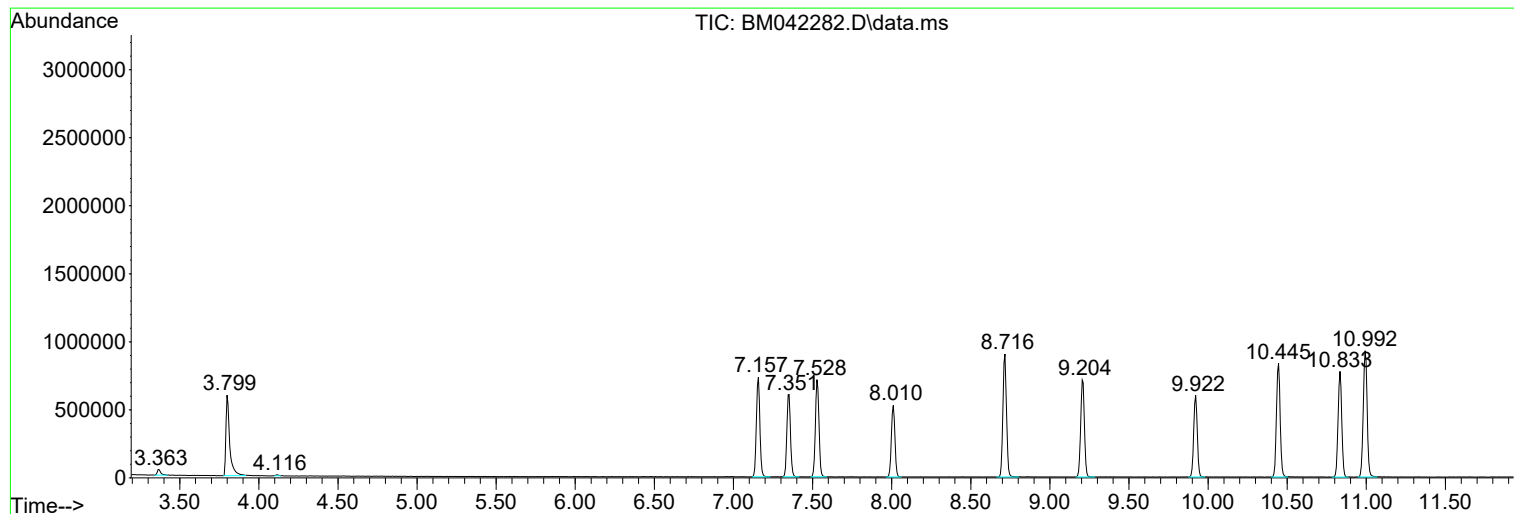

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042282.D
Acq On : 13 Oct 2023 11:51
Operator : MA/JU
Sample : PB156220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042282.D
Acq On : 13 Oct 2023 11:51
Operator : MA/JU
Sample : PB156220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc