

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
 Data File : BM042286.D
 Acq On : 13 Oct 2023 16:44
 Operator : MA/JU
 Sample : PB156222BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042286.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	44	rVB	56067	89672	1.89%	0.181%
2	3.799	100	104	125	rBV	778301	1225233	25.77%	2.469%
3	4.116	154	158	164	rVB2	11756	16628	0.35%	0.034%
4	7.151	668	674	687	rBV	914250	1408631	29.63%	2.839%
5	7.345	700	707	716	rVB	761944	1170726	24.62%	2.359%
6	7.528	731	738	749	rBV	866319	1346724	28.33%	2.714%
7	8.004	812	819	827	rBV	523836	840826	17.69%	1.694%
8	8.710	933	939	949	rBV	1087753	1699879	35.76%	3.426%
9	9.204	1014	1023	1036	rBV	879647	1421112	29.89%	2.864%
10	9.922	1137	1145	1153	rBV	722199	1168712	24.58%	2.355%
11	10.439	1226	1233	1245	rBV	992889	1656874	34.85%	3.339%
12	10.833	1292	1300	1308	rBV	777620	1280631	26.94%	2.581%
13	10.992	1319	1327	1343	rBV	1145718	1879095	39.52%	3.787%
14	12.416	1564	1569	1575	rBV	16202	26201	0.55%	0.053%
15	13.504	1748	1754	1761	rVB2	12598	19829	0.42%	0.040%
16	14.069	1844	1850	1860	rBV	2057796	2708206	56.96%	5.458%
17	14.357	1889	1899	1908	rBV	2154997	3012127	63.36%	6.070%
18	14.657	1943	1950	1958	rVB	1193154	1743096	36.66%	3.513%
19	14.863	1977	1985	2004	rBV	1023407	1488447	31.31%	3.000%
20	15.445	2078	2084	2089	rBV6	3713	6297	0.13%	0.013%
21	15.645	2112	2118	2125	rBV	2761884	3797740	79.88%	7.654%
22	15.774	2134	2140	2153	rBV	1021921	1332375	28.02%	2.685%
23	15.880	2153	2158	2165	rVB4	11145	19167	0.40%	0.039%
24	17.409	2412	2418	2425	rBV	1494348	2076235	43.67%	4.184%
25	17.509	2428	2435	2448	rBV	2951015	4119312	86.65%	8.302%
26	18.251	2556	2561	2567	rVB9	6097	10252	0.22%	0.021%
27	18.809	2654	2656	2661	rVB3	4475	5202	0.11%	0.010%
28	19.362	2746	2750	2754	rBV	27996	36198	0.76%	0.073%
29	19.433	2758	2762	2768	rVB	30042	40510	0.85%	0.082%
30	19.674	2800	2803	2805	rBV2	6430	5699	0.12%	0.011%
31	19.803	2819	2825	2836	rBV	3597292	4714122	99.16%	9.500%
32	21.592	3124	3129	3137	rBV	1751775	2190867	46.08%	4.415%
33	23.909	3516	3523	3535	rVB2	2413410	4754238	100.00%	9.581%
34	24.074	3544	3551	3561	rVB	1138662	2310040	48.59%	4.655%

Sum of corrected areas: 49620903

Instrument :

BNA_M

ClientSampleId :




SBLK222

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042286.D
Acq On : 13 Oct 2023 16:44
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

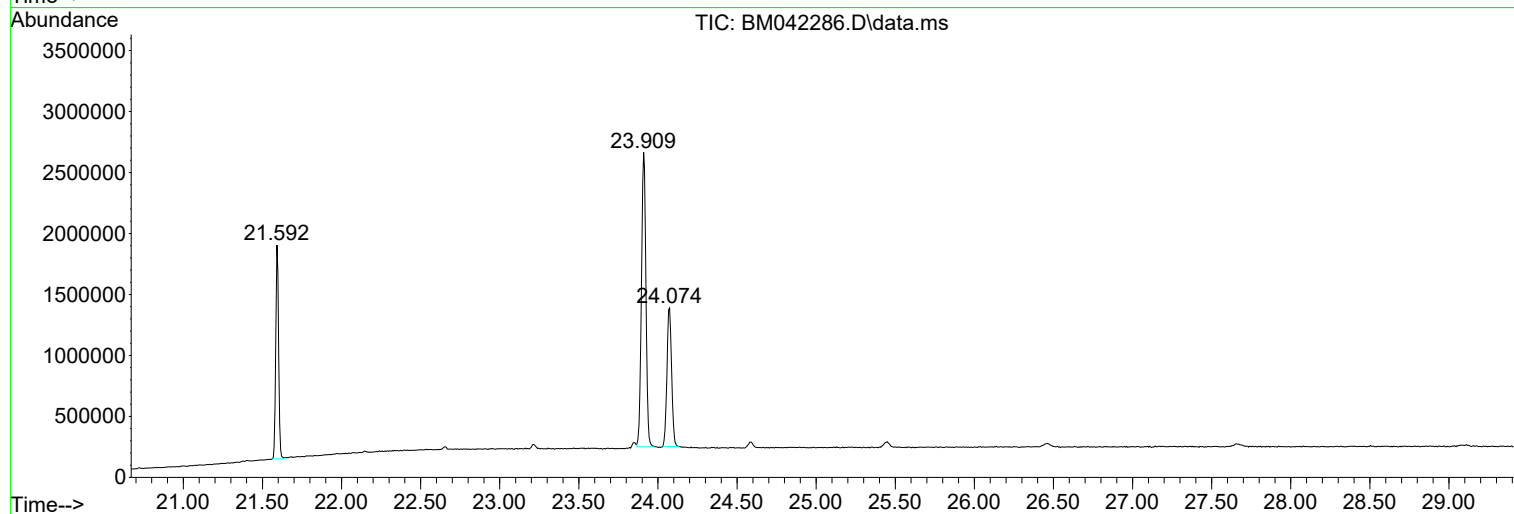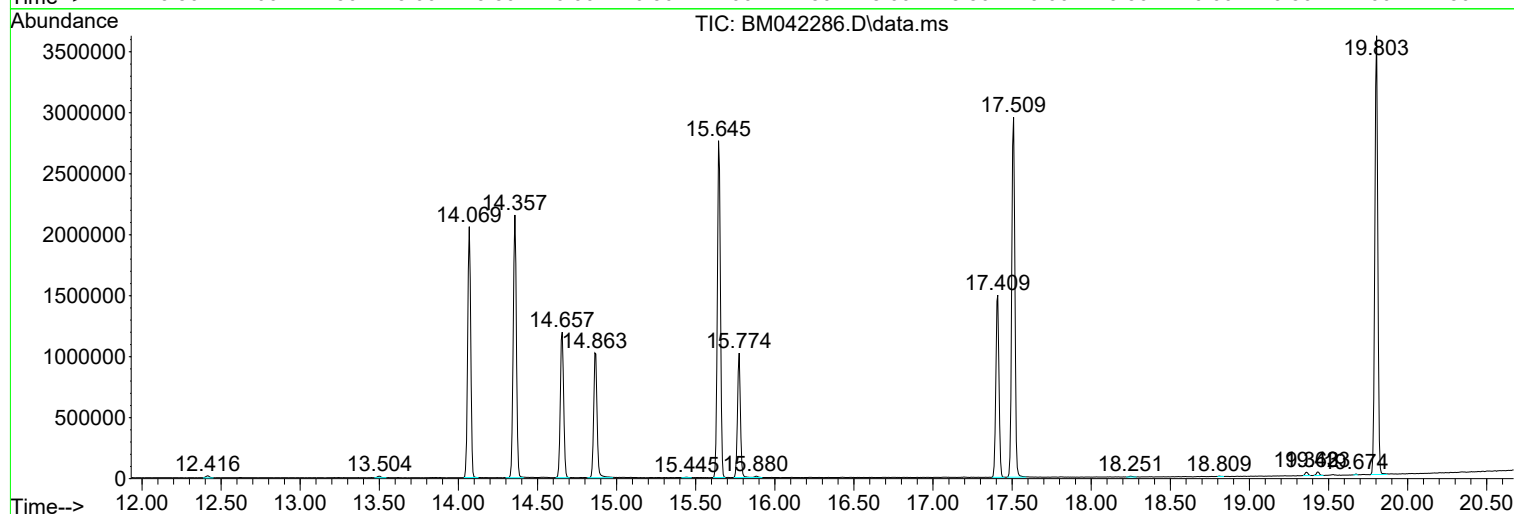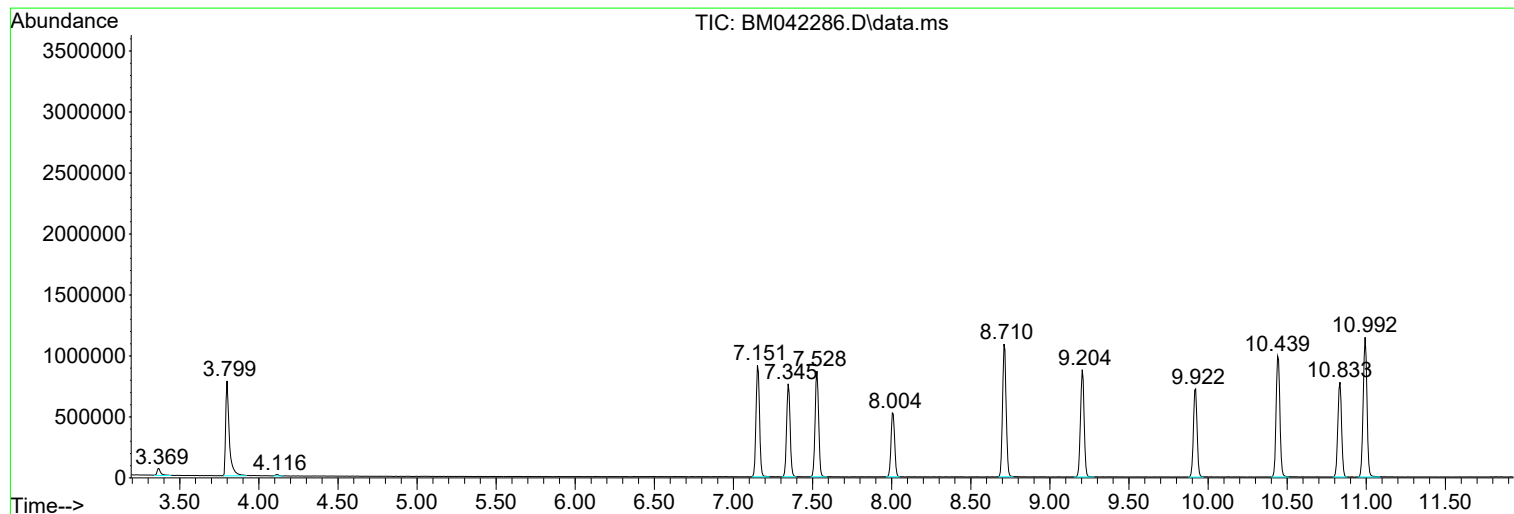

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042286.D
Acq On : 13 Oct 2023 16:44
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042286.D
Acq On : 13 Oct 2023 16:44
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc