

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
 Data File : BM042287.D
 Acq On : 13 Oct 2023 17:21
 Operator : MA/JU
 Sample : PB156223BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	40	rVB	56883	78530	1.73%	0.168%
2	3.804	101	105	127	rBV	754577	1185306	26.10%	2.529%
3	4.122	155	159	165	rVB	9673	13222	0.29%	0.028%
4	6.992	644	647	652	rBV6	2697	5526	0.12%	0.012%
5	7.163	669	676	689	rBV	903807	1382209	30.44%	2.950%
6	7.357	702	709	719	rBV	729594	1146647	25.25%	2.447%
7	7.534	732	739	749	rBV	840734	1311081	28.87%	2.798%
8	8.016	813	821	830	rBV	498691	771335	16.99%	1.646%
9	8.722	934	941	954	rBV	1049479	1650929	36.36%	3.523%
10	9.210	1016	1024	1034	rBV	845951	1367452	30.11%	2.918%
11	9.927	1139	1146	1155	rBV	708760	1122965	24.73%	2.396%
12	10.451	1226	1235	1250	rBV	967054	1592870	35.08%	3.399%
13	10.839	1292	1301	1308	rBV	715344	1170114	25.77%	2.497%
14	10.998	1319	1328	1343	rBV	1086365	1811124	39.88%	3.865%
15	12.421	1564	1570	1577	rBV2	14497	23065	0.51%	0.049%
16	13.504	1749	1754	1763	rVB2	10704	16646	0.37%	0.036%
17	14.074	1844	1851	1859	rBV	1937293	2616985	57.63%	5.585%
18	14.357	1892	1899	1907	rBV	1982908	2885552	63.54%	6.158%
19	14.657	1944	1950	1959	rBV	1110633	1563168	34.42%	3.336%
20	14.868	1979	1986	1999	rBV	1011245	1405704	30.96%	3.000%
21	15.651	2112	2119	2129	rBV	2574911	3634310	80.03%	7.755%
22	15.774	2133	2140	2150	rBV	982777	1271227	27.99%	2.713%
23	15.886	2155	2159	2165	rVB2	9986	14108	0.31%	0.030%
24	17.198	2379	2382	2386	rVB5	3341	4859	0.11%	0.010%
25	17.409	2412	2418	2425	rBV	1380971	1858102	40.92%	3.965%
26	17.509	2428	2435	2455	rBV	2907846	3928610	86.51%	8.384%
27	19.362	2746	2750	2754	rBV2	27376	33744	0.74%	0.072%
28	19.433	2757	2762	2766	rBV	29190	39357	0.87%	0.084%
29	19.668	2800	2802	2810	rBV6	6513	8929	0.20%	0.019%
30	19.797	2819	2824	2832	rBV	3371984	4454554	98.10%	9.506%
31	21.591	3124	3129	3136	rBV	1522113	1931009	42.52%	4.121%
32	23.903	3515	3522	3535	rVB2	2358717	4540987	100.00%	9.690%
33	24.068	3543	3550	3562	rVB	1015016	2020869	44.50%	4.312%




Sum of corrected areas: 46861095

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042287.D
Acq On : 13 Oct 2023 17:21
Operator : MA/JU
Sample : PB156223BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

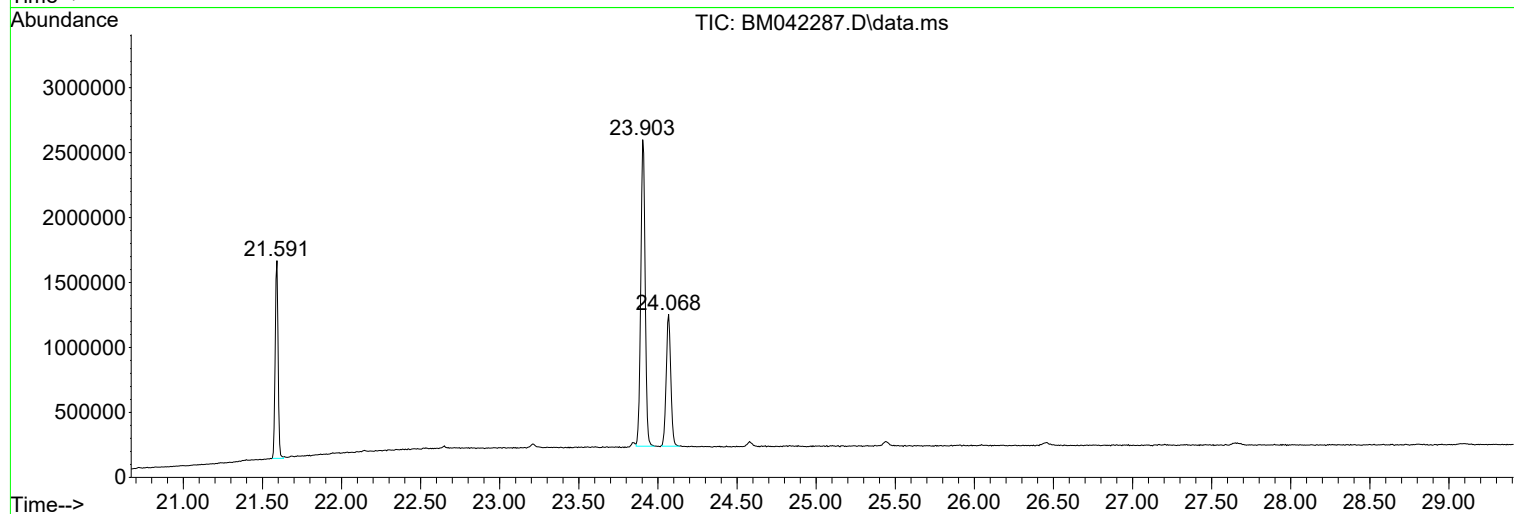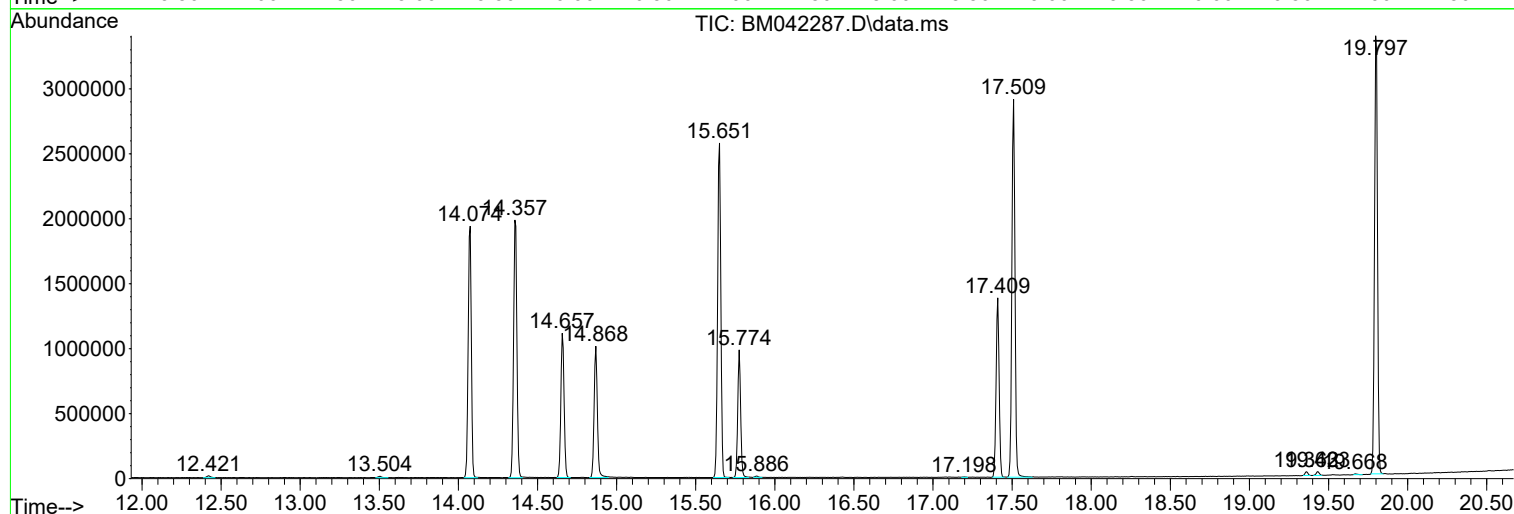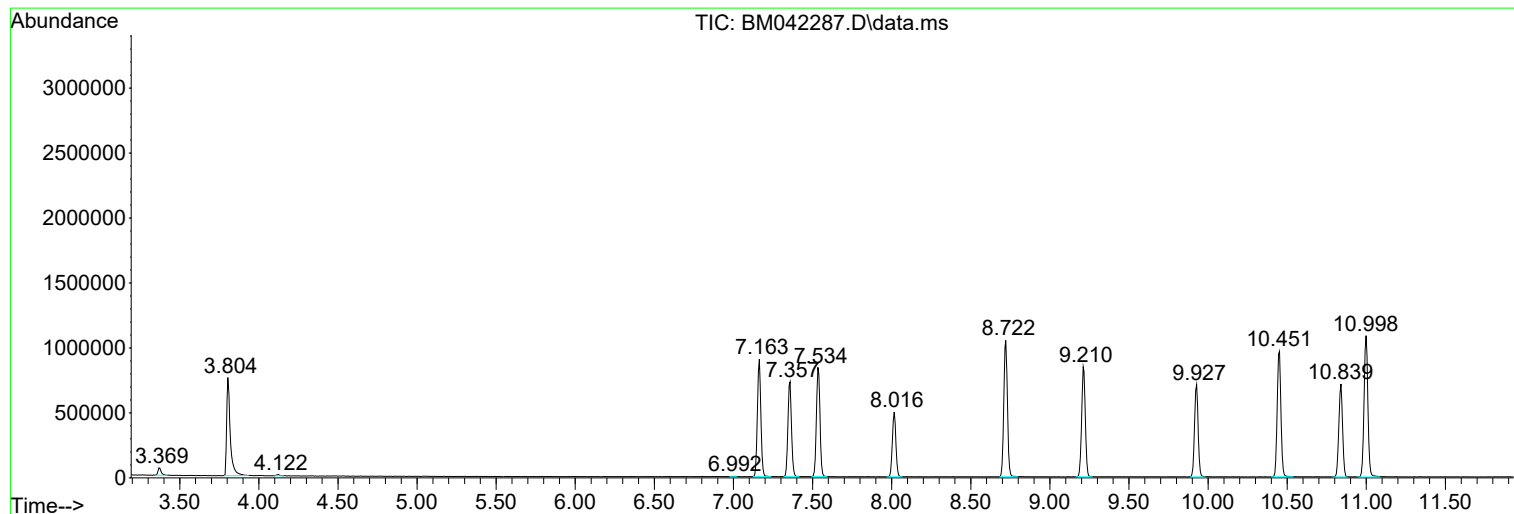

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042287.D
Acq On : 13 Oct 2023 17:21
Operator : MA/JU
Sample : PB156223BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101323\
Data File : BM042287.D
Acq On : 13 Oct 2023 17:21
Operator : MA/JU
Sample : PB156223BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------