

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101417\
 Data File : BM012181.D
 Acq On : 14 Oct 2017 21:40
 Operator : SJ/JU
 Sample : I5840-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Quant Time: Oct 15 05:28:19 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 15 05:22:07 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	121824	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	549042	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	391028	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	1026209	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	1188288	20.00	ng/ul	0.00
83) Perylene-d12	23.70	264	1310668	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	14327	5.59	ng/uL	0.00
5) Phenol-d5	6.98	99	100872	10.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	186835	31.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	243516	29.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	193905	22.78	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	142996	34.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	168508	34.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	296531	31.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.80	131	131	0.01	ng/ul	0.04
43) Dimethylphthalate-d6	13.87	166	1220134	35.30	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1381671	33.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	34729	6.68	ng/ul	0.01
57) Fluorene-d10	15.46	176	1074219	37.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	209098	29.69	ng/ul	0.00
70) Anthracene-d10	17.31	188	1858407	36.62	ng/ul	0.00
76) Pyrene-d10	19.60	212	2297514	38.09	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.55	264	2382646	37.71	ng/ul	0.00


Target Compounds					Ovalue
45) 2,6-Dinitrotoluene	13.87	165	6875	1.00 ng/ul#	26




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101417\
Data File : BM012181.D
Acq On : 14 Oct 2017 21:40
Operator : SJ/JU
Sample : I5840-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Time: Oct 15 05:28:19 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 15 05:22:07 2017
Response via : Initial Calibration

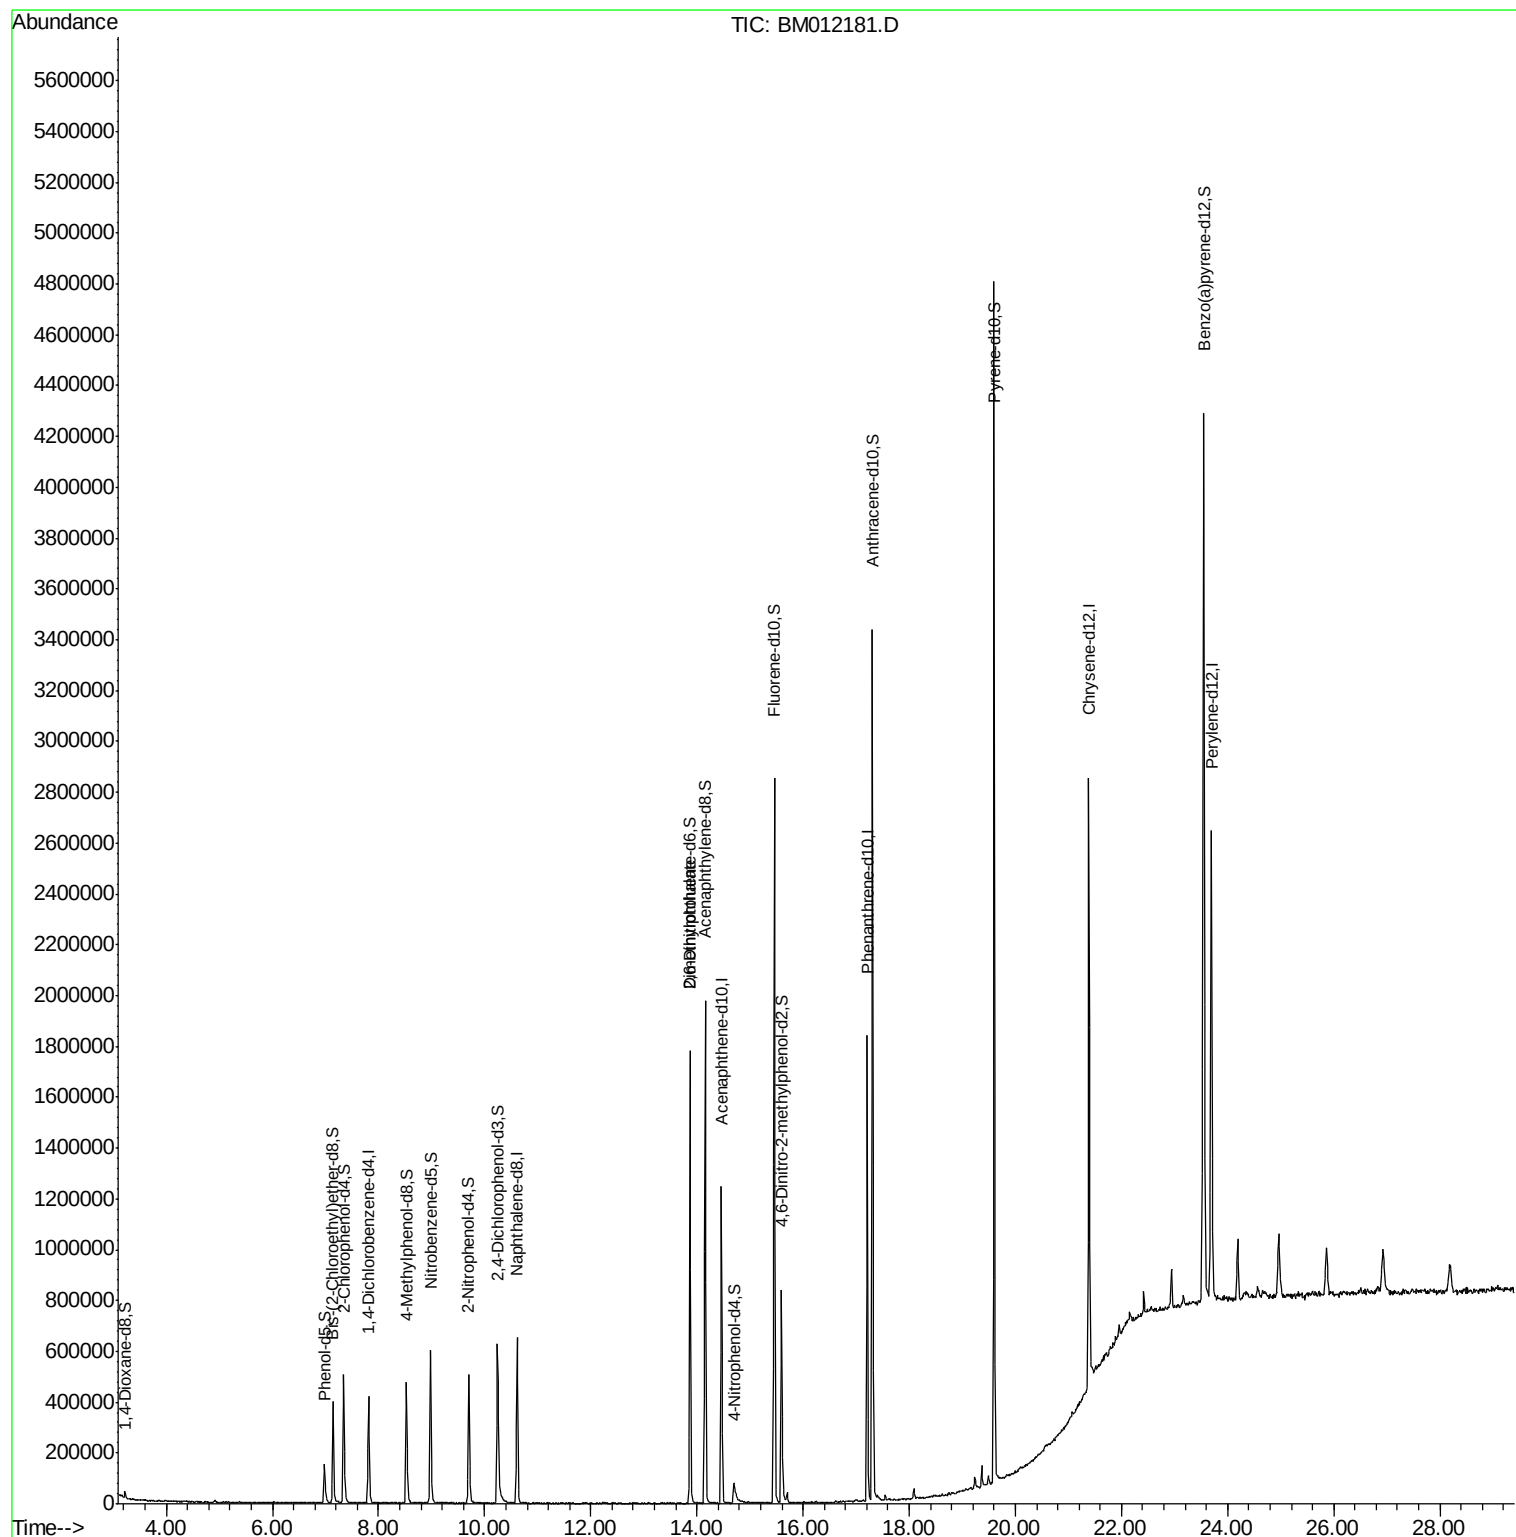

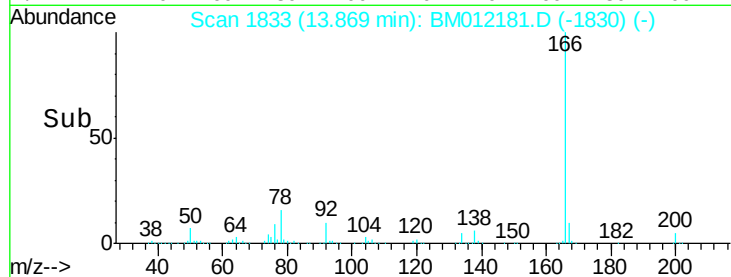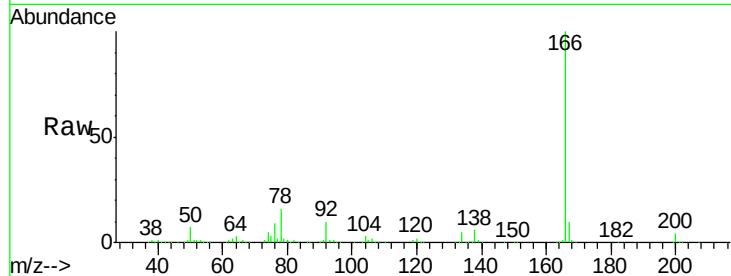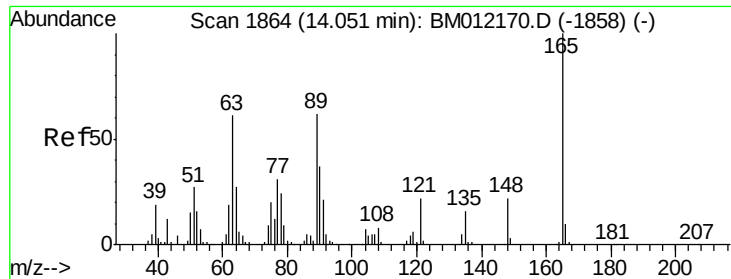

#45

2,6-Dinitrotoluene

Concen: 1.00 ng/ul

RT: 13.87 min Scan# 1833

Delta R.T. -0.18 min

Lab File: BM012181.D

Acq: 14 Oct 2017 21:40

Instrument :

BNA_M

ClientSampleId :

C0AF4

Tot Ion:165 Resp: 6875

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 37.2 14.6 22.0#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

