

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM101617\  
 Data File : BM012246.D  
 Acq On : 17 Oct 2017 09:31  
 Operator : SJ/JU  
 Sample : I5697-03  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 H0AA2

Quant Time: Oct 17 11:29:51 2017  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM101217.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Oct 17 02:52:50 2017  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.79  | 152  | 188025   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.60 | 136  | 689161   | 20.00 | ng/ul | 0.00     |
| 35) Acenaphthene-d10      | 14.45 | 164  | 450954   | 20.00 | ng/ul | 0.00     |
| 61) Phenanthrene-d10      | 17.20 | 188  | 1084089  | 20.00 | ng/ul | 0.00     |
| 75) Chrysene-d12          | 21.38 | 240  | 1097744  | 20.00 | ng/ul | 0.00     |
| 83) Perylene-d12          | 23.68 | 264  | 1053724  | 20.00 | ng/ul | 0.00     |

| System Monitoring Compounds    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 3) 1,4-Dioxane-d8              | 3.21  | 96   | 16441    | 4.16  | ng/uL | 0.00     |
| 5) Phenol-d5                   | 6.96  | 99   | 511940   | 33.56 | ng/ul | 0.00     |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.12  | 67   | 295887   | 32.34 | ng/ul | 0.00     |
| 9) 2-Chlorophenol-d4           | 7.33  | 132  | 451074   | 34.86 | ng/ul | 0.00     |
| 13) 4-Methylphenol-d8          | 8.51  | 113  | 461221   | 35.11 | ng/ul | 0.00     |
| 19) Nitrobenzene-d5            | 8.96  | 128  | 224795   | 42.74 | ng/ul | 0.00     |
| 22) 2-Nitrophenol-d4           | 9.69  | 143  | 246319   | 40.08 | ng/ul | 0.00     |
| 26) 2,4-Dichlorophenol-d3      | 10.23 | 165  | 426171   | 36.32 | ng/ul | 0.00     |
| 29) 4-Chloroaniline-d4         | 10.74 | 131  | 521224   | 47.47 | ng/ul | 0.00     |
| 43) Dimethylphthalate-d6       | 13.86 | 166  | 1416748  | 35.55 | ng/ul | 0.00     |
| 46) Acenaphthylene-d8          | 14.15 | 160  | 1781490  | 36.93 | ng/ul | 0.00     |
| 51) 4-Nitrophenol-d4           | 14.68 | 143  | 129956   | 21.69 | ng/ul | 0.00     |
| 57) Fluorene-d10               | 15.44 | 176  | 1242873  | 37.99 | ng/ul | 0.00     |
| 62) 4,6-Dinitro-2-methylphenol | 15.59 | 200  | 94626    | 12.72 | ng/ul | 0.00     |
| 70) Anthracene-d10             | 17.30 | 188  | 1969074  | 36.73 | ng/ul | 0.00     |
| 76) Pyrene-d10                 | 19.59 | 212  | 2042818  | 36.66 | ng/ul | 0.00     |
| 87) Benzo(a)pyrene-d12         | 23.53 | 264  | 1913248  | 37.66 | ng/ul | 0.00     |


| Target Compounds      | R.T.  | QIon | Response | Conc   | Units | Qvalue |
|-----------------------|-------|------|----------|--------|-------|--------|
| 6) Phenol             | 6.99  | 94   | 114013   | 7.229  | ng/ul | 99     |
| 44) Dimethylphthalate | 13.90 | 163  | 556138   | 13.927 | ng/ul | 99     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM101617\  
Data File : BM012246.D  
Acq On : 17 Oct 2017 09:31  
Operator : SJ/JU  
Sample : I5697-03  
Misc :  
ALS Vial : 31 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
H0AA2

Quant Time: Oct 17 11:29:51 2017  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM101217.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Oct 17 02:52:50 2017  
Response via : Initial Calibration

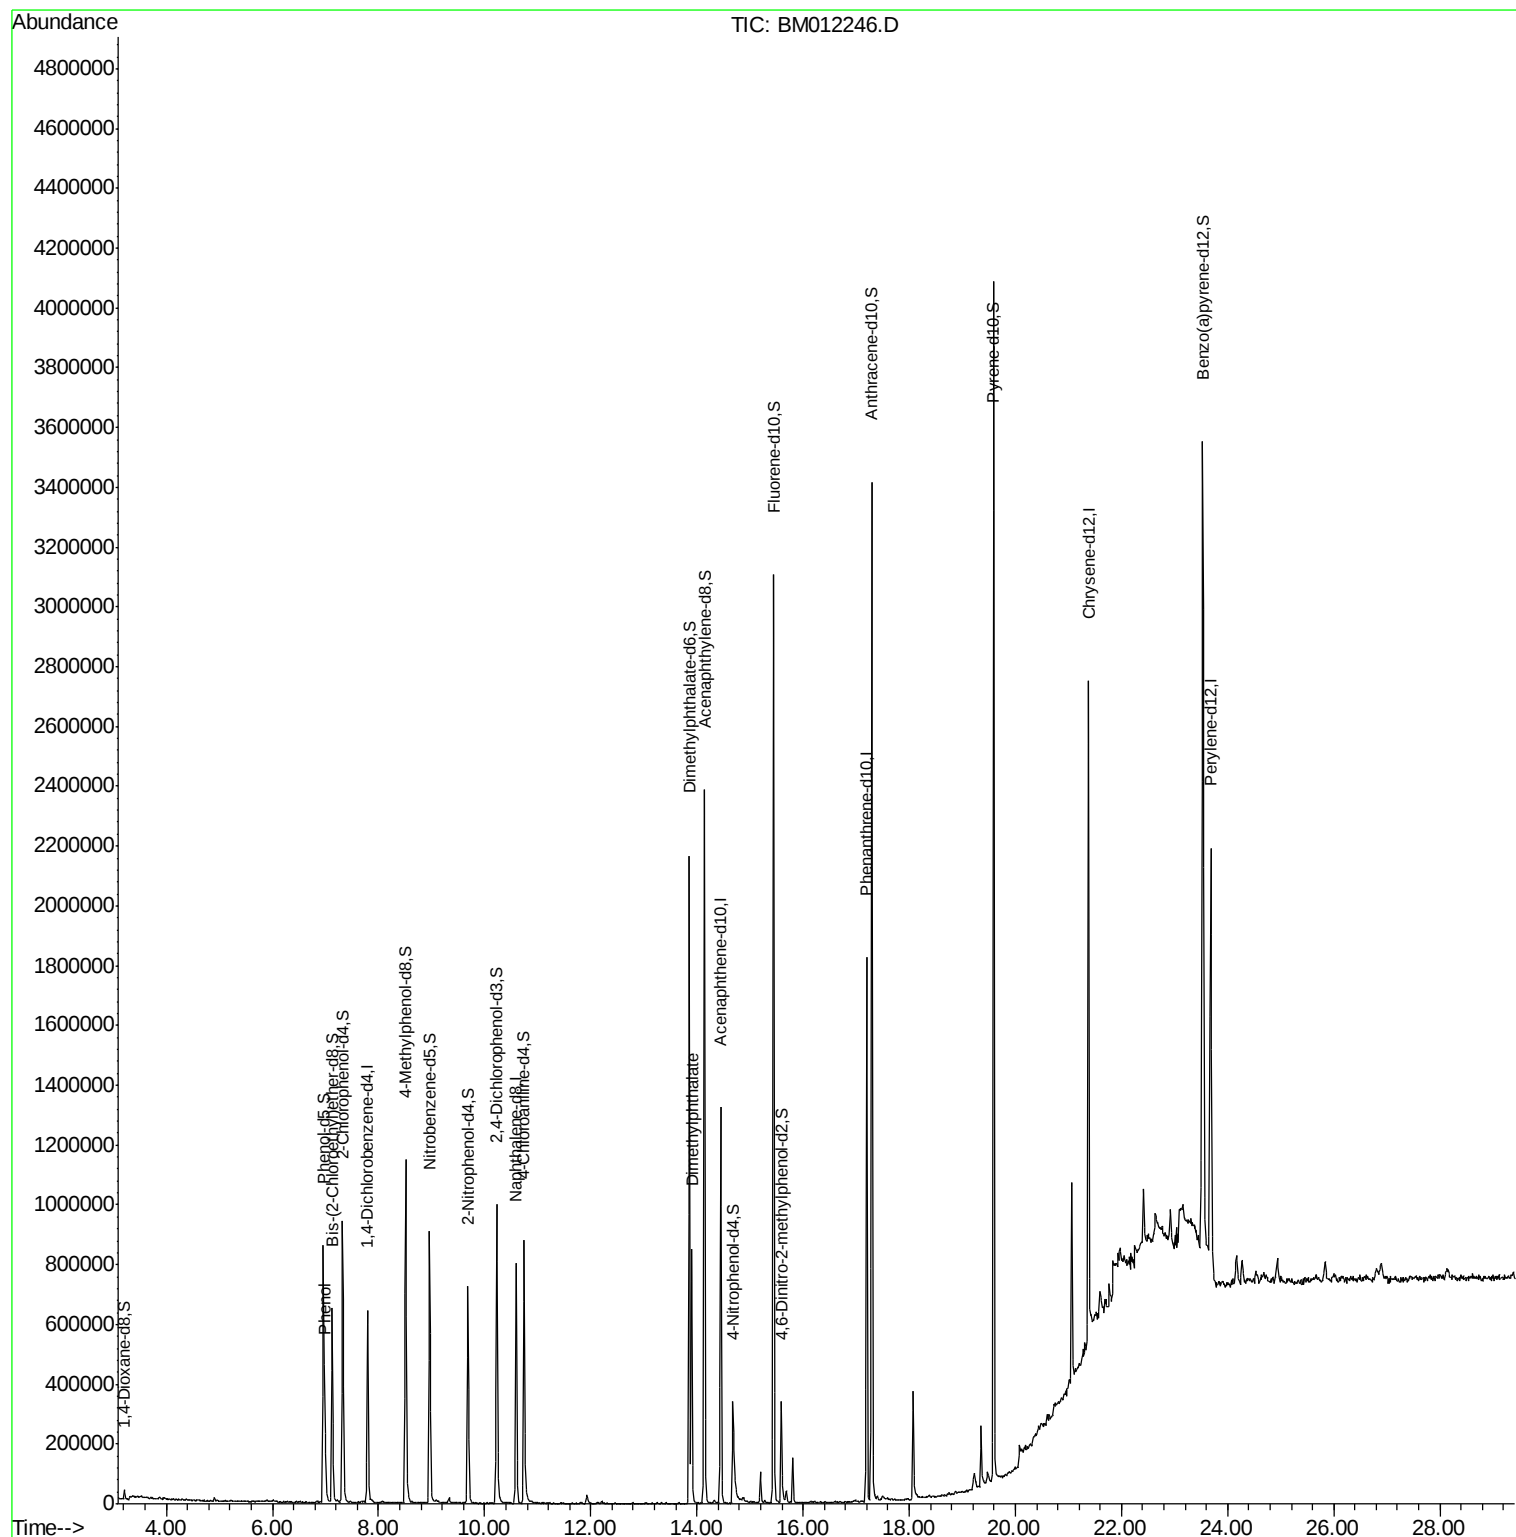

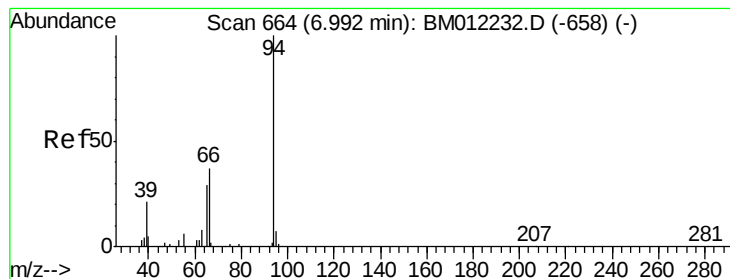

#6

Phenol

Concen: 7.229 ng/ul

RT: 6.99 min Scan# 664

Delta R.T. 0.00 min

Lab File: BM012246.D

Acq: 17 Oct 2017 09:31

Instrument :

BNA\_M

ClientSampleId :

H0AA2





Tgt Ion: 94 Resp: 114013

Ion Ratio Lower Upper

94 100

65 31.5 24.4 36.6

66 43.1 35.0 52.4

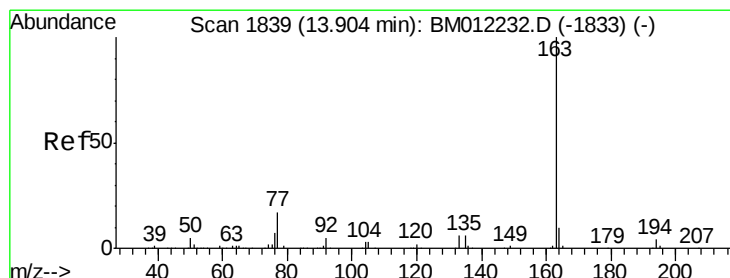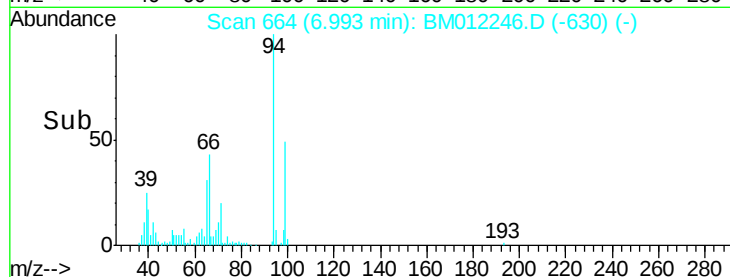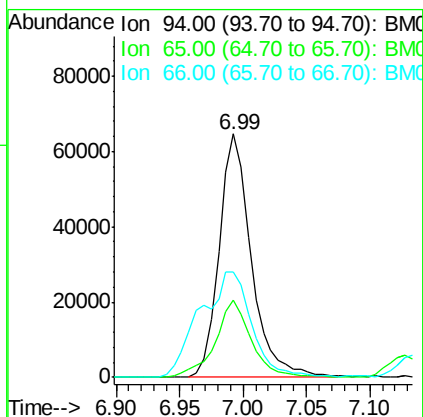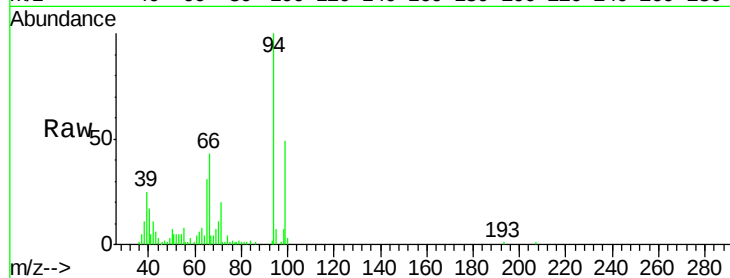

#44

Dimethylphthalate

Concen: 13.927 ng/ul

RT: 13.90 min Scan# 1839

Delta R.T. 0.00 min

Lab File: BM012246.D

Acq: 17 Oct 2017 09:31

Tgt Ion: 163 Resp: 556138

Ion Ratio Lower Upper

163 100

194 4.6 3.7 5.5

164 10.4 8.1 12.1

