

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
 Data File : BM012220.D
 Acq On : 16 Oct 2017 17:53
 Operator : SJ/JU
 Sample : I5840-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.969	654	660	671	rBV	85975	177035	3.70%	0.430%
2	7.128	679	687	699	rBV	354553	580411	12.13%	1.411%
3	7.328	713	721	734	rBV	398472	714660	14.93%	1.738%
4	7.798	794	801	812	rBV	472657	819443	17.12%	1.992%
5	8.510	916	922	935	rBV	313008	593219	12.40%	1.442%
6	8.969	990	1000	1011	rBV	505000	903949	18.89%	2.198%
7	9.686	1113	1122	1135	rBV	471242	864131	18.06%	2.101%
8	10.228	1206	1214	1235	rBV	585550	1250480	26.13%	3.041%
9	10.598	1269	1277	1286	rBV	756011	1292842	27.01%	3.144%
10	13.857	1825	1831	1843	rBV	1614071	2334287	48.78%	5.676%
11	14.145	1873	1880	1890	rBV	1808295	2681343	56.03%	6.520%
12	14.310	1901	1908	1921	rBV3	38801	109762	2.29%	0.267%
13	14.451	1925	1932	1939	rVV2	1311576	2044191	42.71%	4.970%
14	14.698	1968	1974	1986	rBV2	53570	154987	3.24%	0.377%
15	15.445	2095	2101	2107	rBV	2317311	3379521	70.62%	8.217%
16	15.498	2107	2110	2117	rVB3	58058	92386	1.93%	0.225%
17	15.592	2120	2126	2138	rBV	633819	1018309	21.28%	2.476%
18	16.509	2274	2282	2286	rBV2	37845	57726	1.21%	0.140%
19	17.198	2393	2399	2405	rBV2	1840898	2708231	56.59%	6.585%
20	17.298	2410	2416	2431	rVB	2492827	3781835	79.02%	9.196%
21	18.074	2544	2548	2554	rBV5	50704	85745	1.79%	0.208%
22	18.151	2557	2561	2569	rVB	46179	72492	1.51%	0.176%
23	19.233	2740	2745	2747	rBV	37498	62910	1.31%	0.153%
24	19.262	2747	2750	2754	rVB	65960	87525	1.83%	0.213%
25	19.356	2762	2766	2777	rBV	82473	141912	2.97%	0.345%
26	19.598	2800	2807	2817	rBV	3203474	4785718	100.00%	11.637%
27	19.821	2840	2845	2849	rBV	159370	219411	4.58%	0.534%
28	20.509	2958	2962	2966	rBV2	57786	81793	1.71%	0.199%
29	20.568	2969	2972	2976	rVB2	74224	87883	1.84%	0.214%
30	21.268	3089	3091	3095	rBV	71958	80980	1.69%	0.197%
31	21.380	3105	3110	3115	rBV	2432642	3188624	66.63%	7.753%
32	23.538	3470	3477	3491	rVB2	1950755	4006589	83.72%	9.742%
33	23.686	3496	3502	3512	rVB	1384312	2666180	55.71%	6.483%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012220.D
Acq On : 16 Oct 2017 17:53
Operator : SJ/JU
Sample : I5840-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Title : SVOA CALIBRATION


Sum of corrected areas: 41126510

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012220.D
Acq On : 16 Oct 2017 17:53
Operator : SJ/JU
Sample : I5840-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

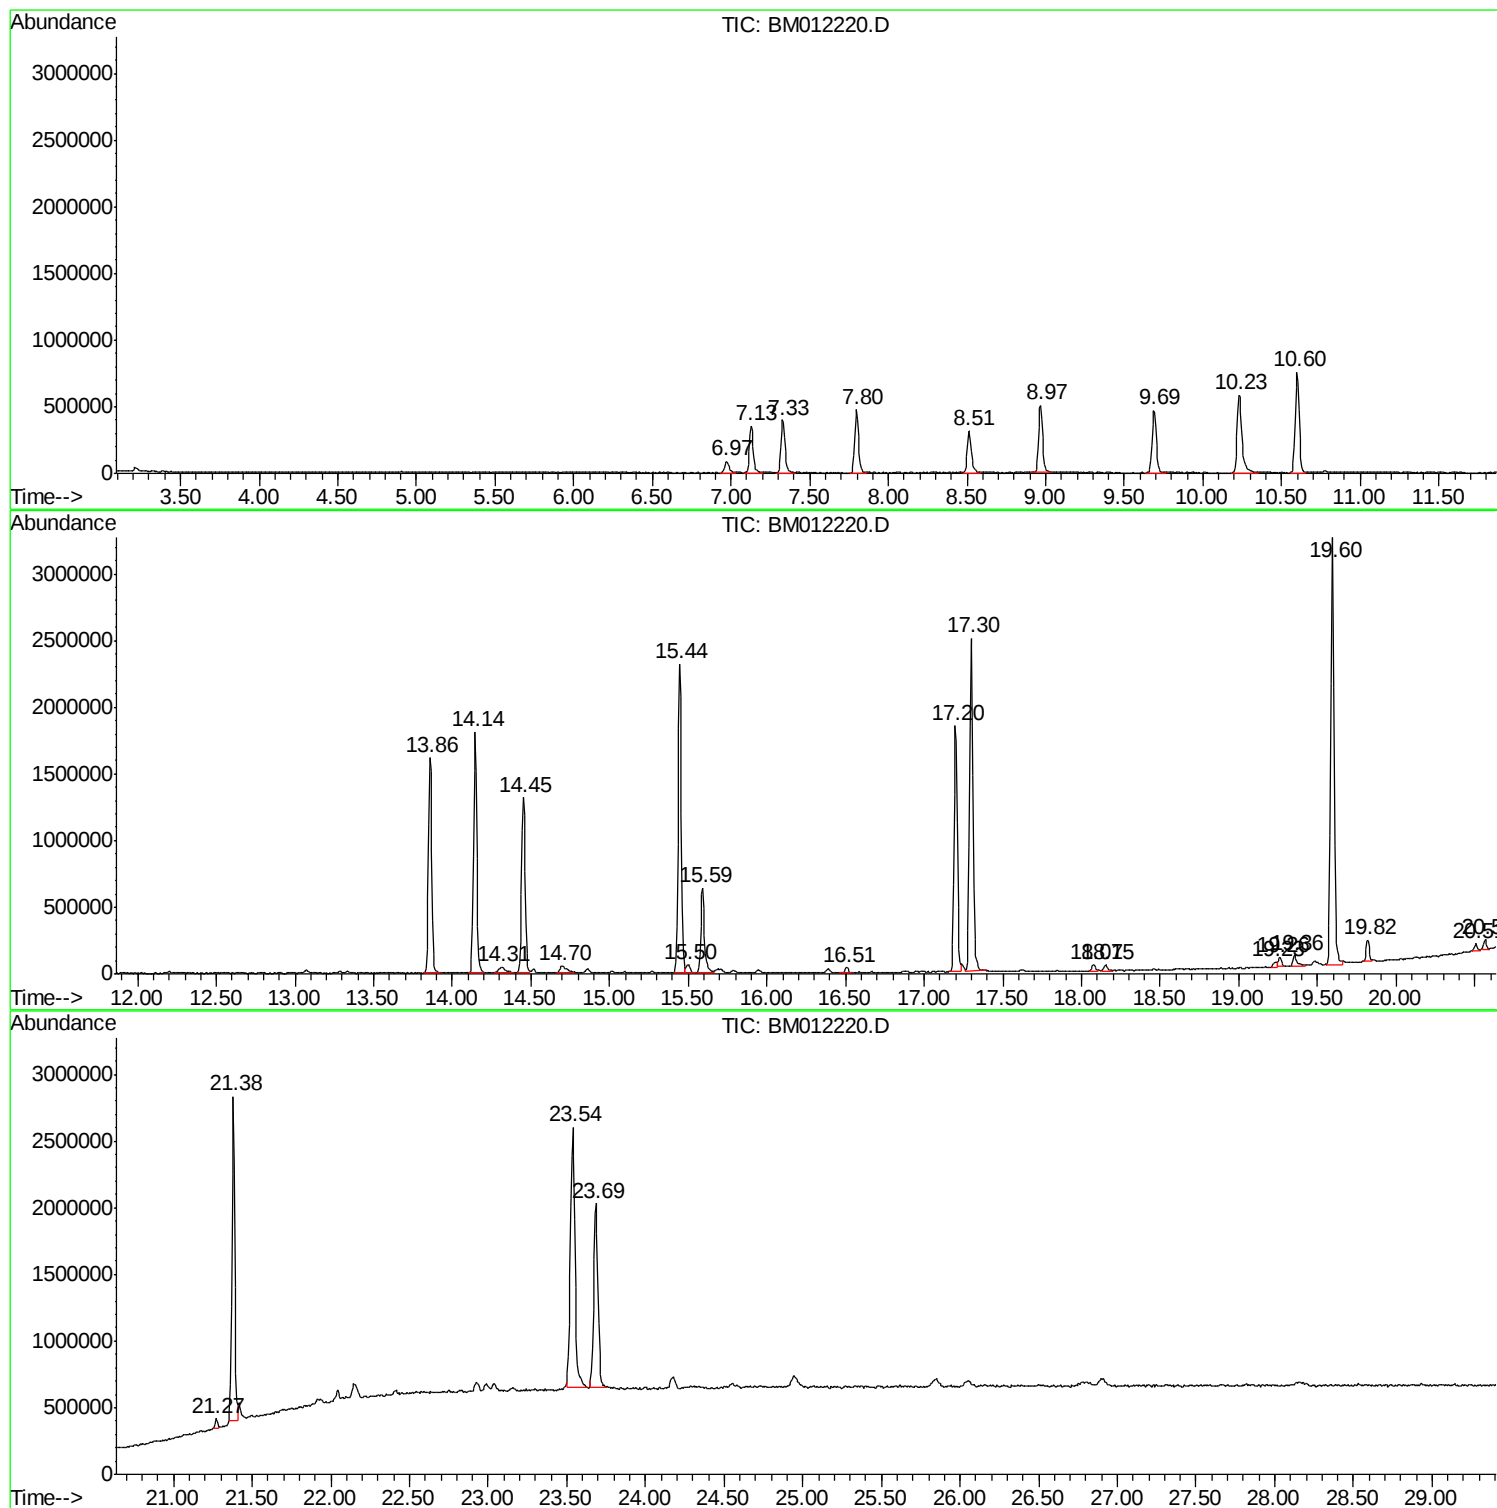

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012220.D
Acq On : 16 Oct 2017 17:53
Operator : SJ/JU
Sample : I5840-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012220.D
Acq On : 16 Oct 2017 17:53
Operator : SJ/JU
Sample : I5840-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc