

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
 Data File : BM012233.D
 Acq On : 17 Oct 2017 01:47
 Operator : SJ/JU
 Sample : PB103191BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	30	rVB	33610	55813	1.20%	0.132%
2	6.969	654	660	677	rBV	499973	940346	20.28%	2.222%
3	7.128	681	687	697	rVV	431903	690215	14.89%	1.631%
4	7.328	714	721	735	rBV	615971	1035538	22.33%	2.447%
5	7.798	793	801	812	rBV	444550	804534	17.35%	1.901%
6	8.510	915	922	935	rBV	730912	1323774	28.55%	3.128%
7	8.963	992	999	1013	rBV	579953	1039112	22.41%	2.455%
8	9.686	1115	1122	1140	rBV	531349	965939	20.83%	2.282%
9	10.227	1207	1214	1232	rBV	774609	1477315	31.86%	3.490%
10	10.598	1269	1277	1288	rBV	703668	1182925	25.51%	2.795%
11	10.745	1294	1302	1320	rBV	687336	1413826	30.49%	3.340%
12	13.857	1825	1831	1846	rBV	1769583	2526540	54.49%	5.969%
13	14.145	1870	1880	1899	rBV	1948540	2944456	63.51%	6.957%
14	14.310	1899	1908	1916	rBV2	51889	131181	2.83%	0.310%
15	14.451	1925	1932	1950	rVB2	1193090	1844066	39.77%	4.357%
16	14.680	1965	1971	1990	rBV	337693	847499	18.28%	2.002%
17	15.445	2094	2101	2116	rBV	2524619	3656477	78.86%	8.639%
18	15.592	2120	2126	2138	rVV	520269	912934	19.69%	2.157%
19	15.686	2138	2142	2148	rVB	30856	47418	1.02%	0.112%
20	17.198	2393	2399	2409	rBV2	1636922	2316231	49.96%	5.472%
21	17.298	2409	2416	2427	rBV	2707552	3992029	86.10%	9.432%
22	19.592	2800	2806	2814	rBV	3402082	4636468	100.00%	10.954%
23	21.380	3105	3110	3122	rBV	1671774	2457188	53.00%	5.805%
24	23.532	3470	3476	3489	rVB2	1601503	3243303	69.95%	7.663%
25	23.680	3496	3501	3513	rVB2	900197	1840475	39.70%	4.348%


Sum of corrected areas: 42325602

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012233.D
Acq On : 17 Oct 2017 01:47
Operator : SJ/JU
Sample : PB103191BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

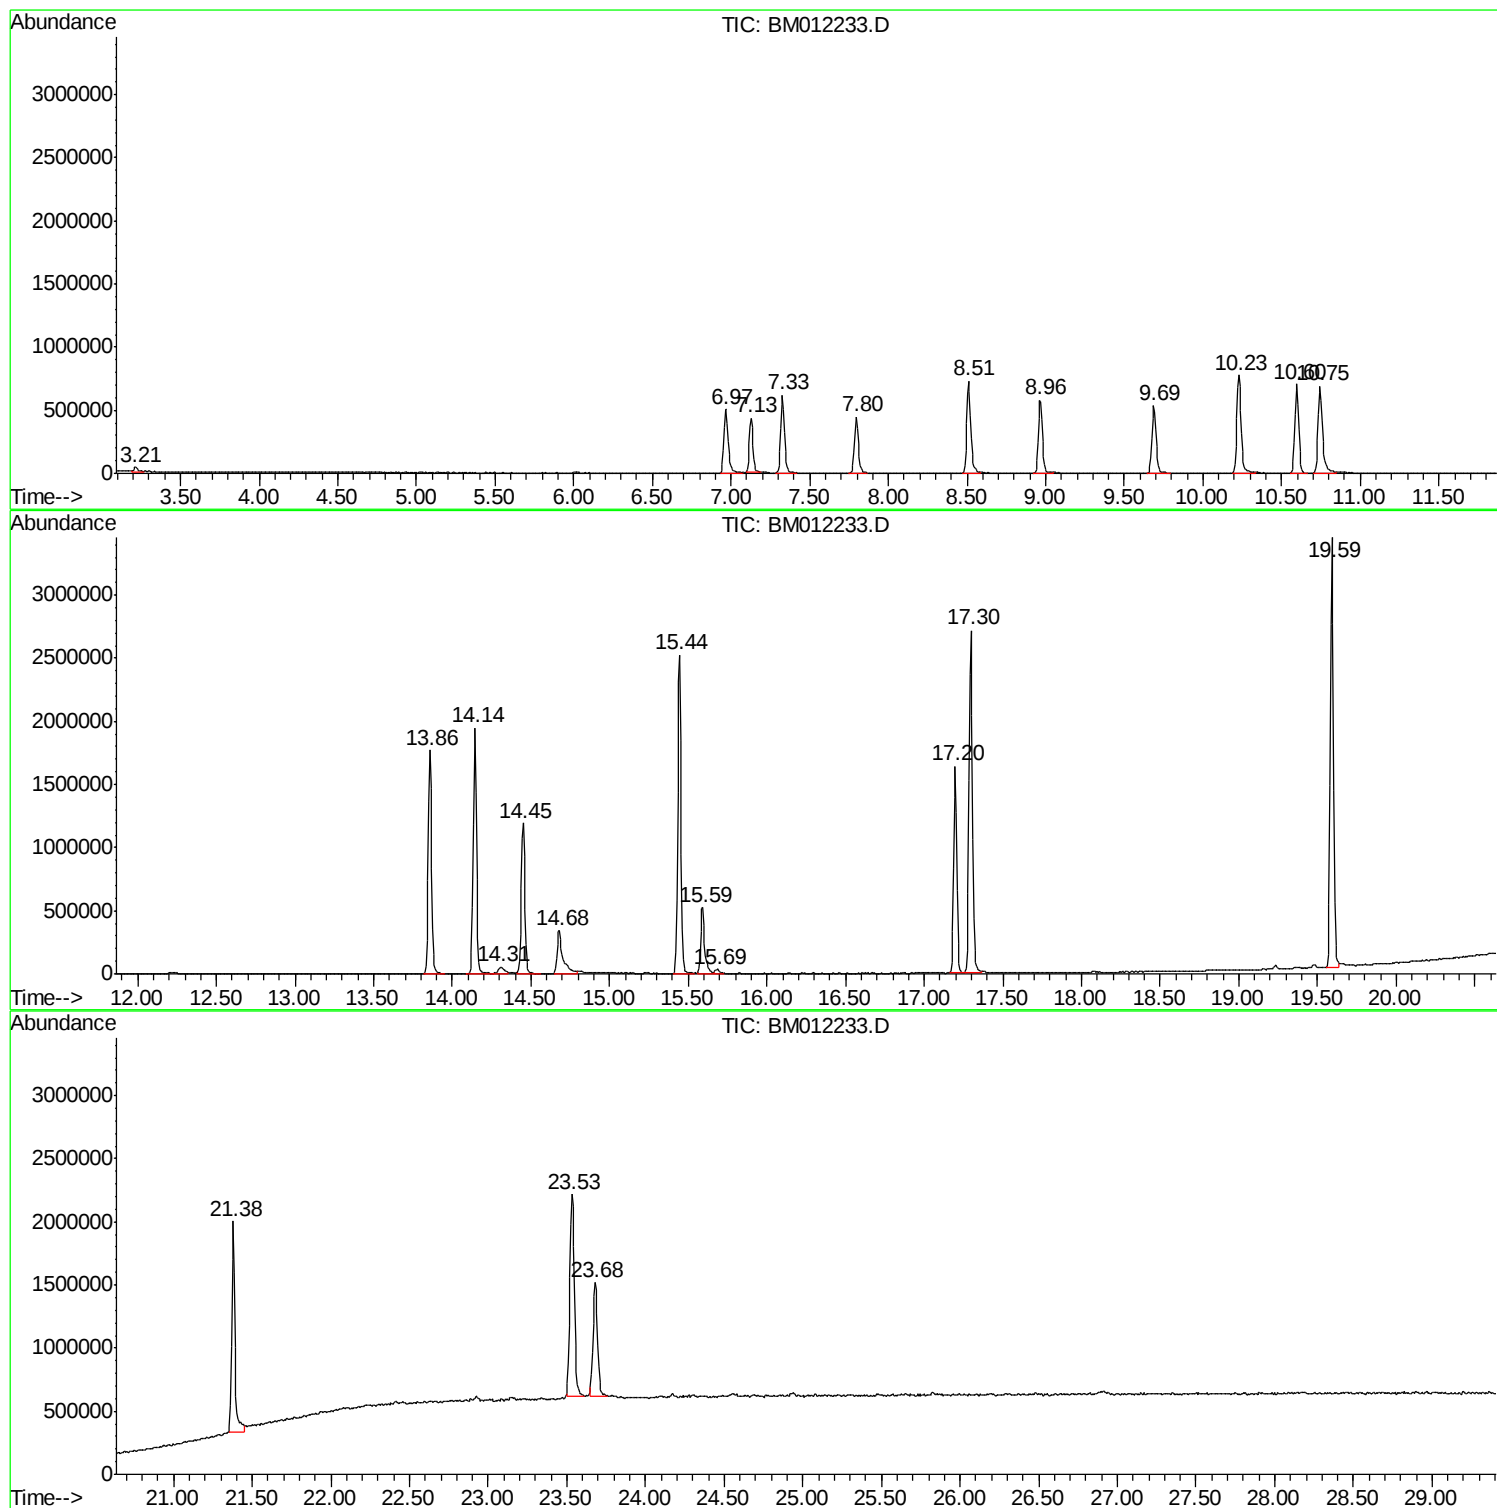

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012233.D
Acq On : 17 Oct 2017 01:47
Operator : SJ/JU
Sample : PB103191BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101617\
Data File : BM012233.D
Acq On : 17 Oct 2017 01:47
Operator : SJ/JU
Sample : PB103191BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc