

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042291.D
 Acq On : 16 Oct 2023 10:11
 Operator : MA/JU
 Sample : PB156260BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	44	rVB	52274	76507	1.66%	0.162%
2	3.805	101	105	127	rBV	676568	1092660	23.70%	2.314%
3	4.116	155	158	164	rVB	9732	14207	0.31%	0.030%
4	7.163	667	676	685	rBV	808798	1276337	27.69%	2.703%
5	7.351	702	708	717	rBV	686387	1085012	23.54%	2.298%
6	7.534	732	739	754	rVB	818534	1256062	27.25%	2.660%
7	8.016	813	821	829	rBV	573260	900245	19.53%	1.907%
8	8.722	934	941	950	rBV	978991	1573591	34.13%	3.333%
9	9.210	1015	1024	1031	rBV	823255	1320518	28.64%	2.797%
10	9.922	1138	1145	1155	rBV	644593	1065092	23.10%	2.256%
11	10.445	1226	1234	1246	rBV	918433	1499046	32.52%	3.175%
12	10.840	1294	1301	1310	rVB	826450	1373705	29.80%	2.909%
13	10.998	1320	1328	1345	rBV	1009382	1715902	37.22%	3.634%
14	12.422	1565	1570	1577	rBV	13171	22224	0.48%	0.047%
15	13.504	1749	1754	1760	rVB	9862	16239	0.35%	0.034%
16	14.069	1844	1850	1861	rBV	1867998	2459792	53.36%	5.210%
17	14.357	1892	1899	1908	rBV	1918368	2736832	59.37%	5.796%
18	14.657	1943	1950	1958	rBV	1306607	1825784	39.61%	3.867%
19	14.786	1968	1972	1977	rVB5	4628	5511	0.12%	0.012%
20	14.869	1979	1986	2006	rVV	955364	1394505	30.25%	2.953%
21	15.651	2112	2119	2127	rVB	2383969	3411567	74.00%	7.226%
22	15.774	2134	2140	2155	rBV	965498	1249627	27.11%	2.647%
23	15.880	2155	2158	2164	rVB2	10804	12987	0.28%	0.028%
24	17.198	2377	2382	2386	rBV6	3032	5881	0.13%	0.012%
25	17.410	2411	2418	2425	rBV	1596903	2171868	47.11%	4.600%
26	17.510	2428	2435	2447	rBV	2722808	3751979	81.39%	7.947%
27	18.257	2559	2562	2569	rBV7	3829	5747	0.12%	0.012%
28	19.362	2746	2750	2754	rBV	26281	34497	0.75%	0.073%
29	19.433	2758	2762	2766	rVB	28334	35403	0.77%	0.075%
30	19.668	2800	2802	2806	rVB3	9334	10365	0.22%	0.022%
31	19.798	2818	2824	2837	rBV	3435368	4492177	97.44%	9.514%
32	21.592	3124	3129	3138	rBV	1793119	2256298	48.94%	4.779%
33	23.845	3509	3512	3515	rBV	83987	118731	2.58%	0.251%
34	23.909	3515	3523	3535	rVB2	2328152	4609969	100.00%	9.764%
35	24.068	3543	3550	3561	rVB	1148962	2338566	50.73%	4.953%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042291.D
Acq On : 16 Oct 2023 10:11
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK260

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47215433

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042291.D
Acq On : 16 Oct 2023 10:11
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

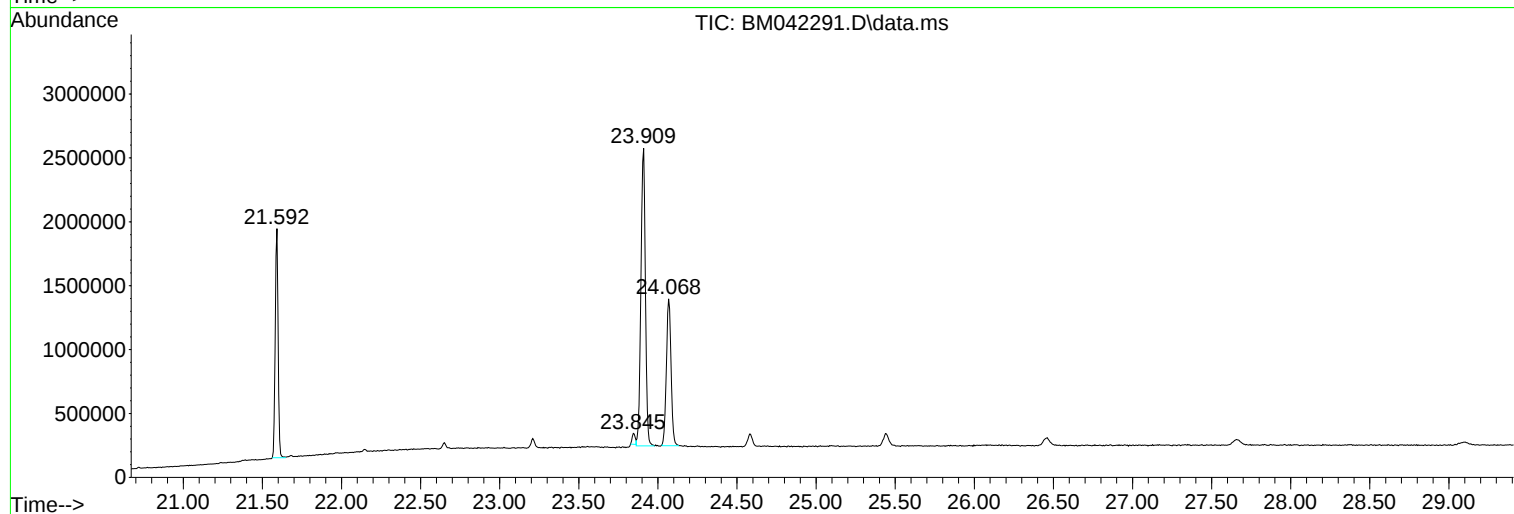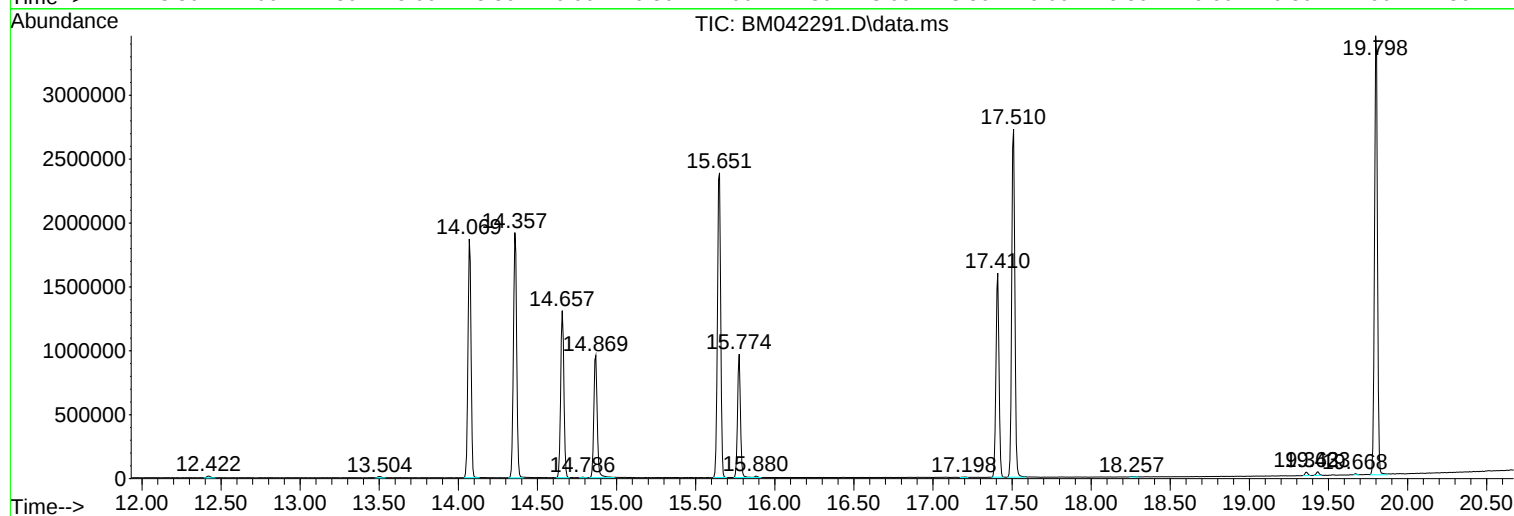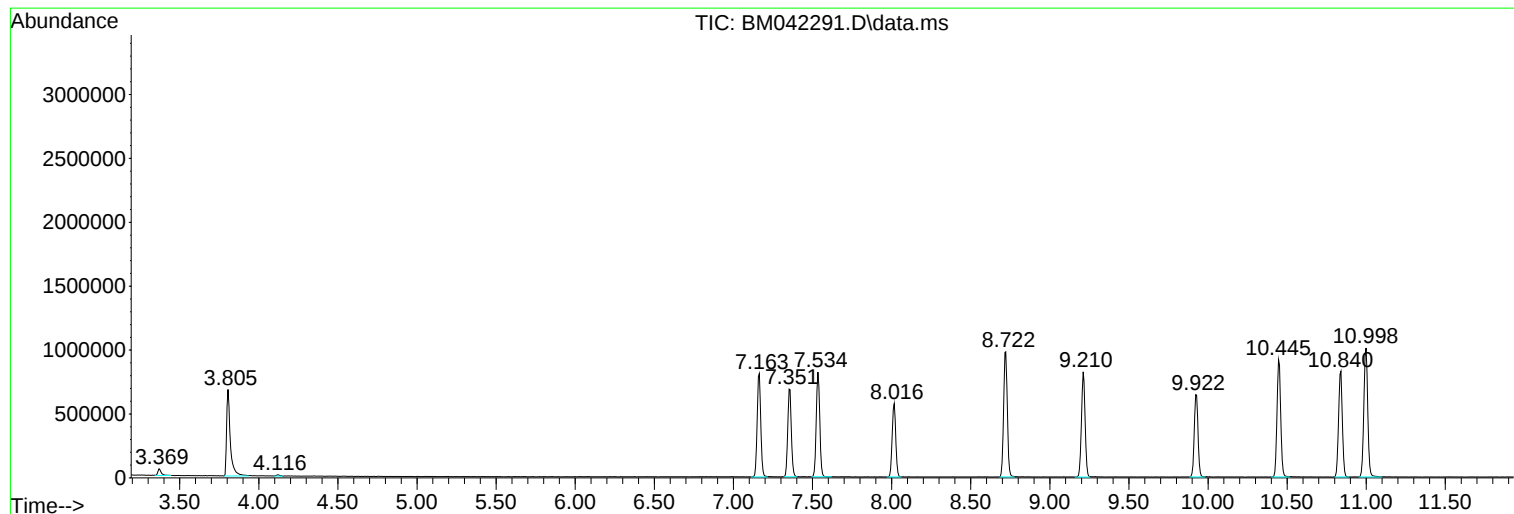

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042291.D
Acq On : 16 Oct 2023 10:11
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042291.D
Acq On : 16 Oct 2023 10:11
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc