

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042295.D
 Acq On : 16 Oct 2023 12:50
 Operator : MA/JU
 Sample : PB156264BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	41	rVB	63348	84451	1.98%	0.174%
2	3.804	101	105	123	rBV	756095	1217638	28.58%	2.503%
3	4.116	154	158	166	rVB	12580	21733	0.51%	0.045%
4	7.157	667	675	688	rBV	912209	1418071	33.29%	2.916%
5	7.351	698	708	718	rBV	766370	1159950	27.23%	2.385%
6	7.534	731	739	755	rBV	867224	1334892	31.33%	2.745%
7	8.010	813	820	831	rVB	637469	1024128	24.04%	2.106%
8	8.716	933	940	951	rBV	1068656	1677313	39.37%	3.449%
9	9.210	1016	1024	1039	rBV	877366	1394378	32.73%	2.867%
10	9.922	1138	1145	1155	rBV	698323	1136150	26.67%	2.336%
11	10.445	1227	1234	1248	rBV	994570	1597256	37.49%	3.284%
12	10.839	1293	1301	1309	rVB	930809	1562029	36.66%	3.212%
13	10.998	1320	1328	1343	rBV	1075530	1816396	42.63%	3.734%
14	12.416	1563	1569	1577	rVB	13251	24833	0.58%	0.051%
15	13.504	1749	1754	1761	rVB2	12095	18240	0.43%	0.038%
16	14.074	1844	1851	1861	rBV	1821957	2498805	58.65%	5.138%
17	14.357	1892	1899	1911	rBV	1991655	2829228	66.41%	5.817%
18	14.657	1943	1950	1962	rVB	1432820	2054867	48.23%	4.225%
19	14.868	1979	1986	2005	rBV	966155	1364190	32.02%	2.805%
20	15.651	2112	2119	2126	rBV	2528877	3524615	82.73%	7.247%
21	15.774	2134	2140	2152	rBV	941425	1193902	28.02%	2.455%
22	15.886	2154	2159	2164	rVB2	11975	15615	0.37%	0.032%
23	17.409	2411	2418	2425	rBV	1781998	2399278	56.32%	4.933%
24	17.509	2428	2435	2451	rBV	2734579	3769147	88.47%	7.749%
25	18.251	2558	2561	2565	rBV4	3739	5159	0.12%	0.011%
26	19.362	2746	2750	2754	rBV3	25667	34347	0.81%	0.071%
27	19.433	2758	2762	2766	rVB	30192	38670	0.91%	0.080%
28	19.533	2775	2779	2782	rBV6	4797	7423	0.17%	0.015%
29	19.674	2800	2803	2808	rBV3	11023	12443	0.29%	0.026%
30	19.803	2819	2825	2833	rBV	3247145	4260361	100.00%	8.759%
31	21.591	3124	3129	3137	rBV	1986908	2476275	58.12%	5.091%
32	23.909	3516	3523	3538	rVB2	2177723	4152983	97.48%	8.538%
33	24.068	3544	3550	3563	rVB	1276678	2513618	59.00%	5.168%




Sum of corrected areas: 48638384

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042295.D
Acq On : 16 Oct 2023 12:50
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

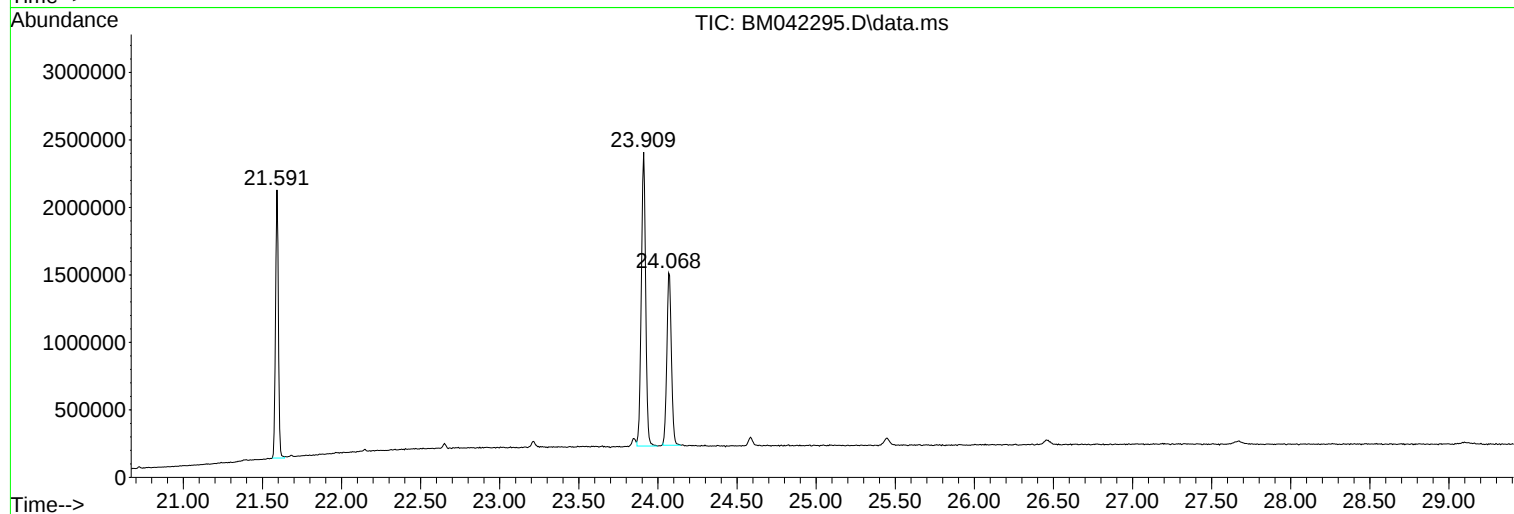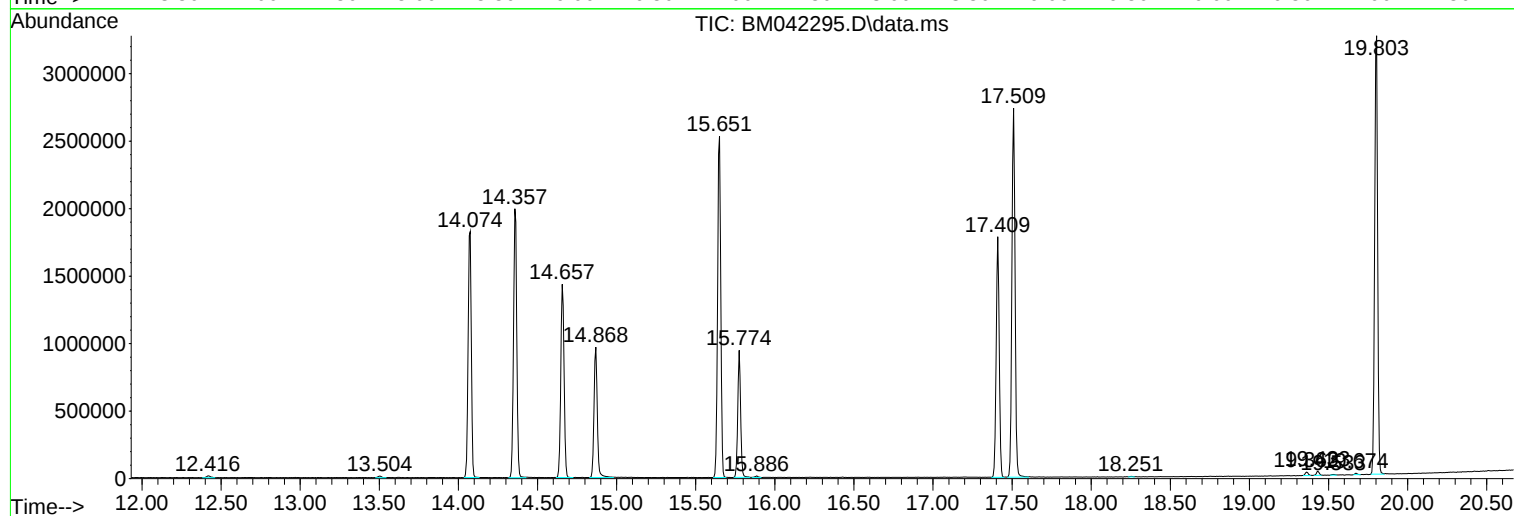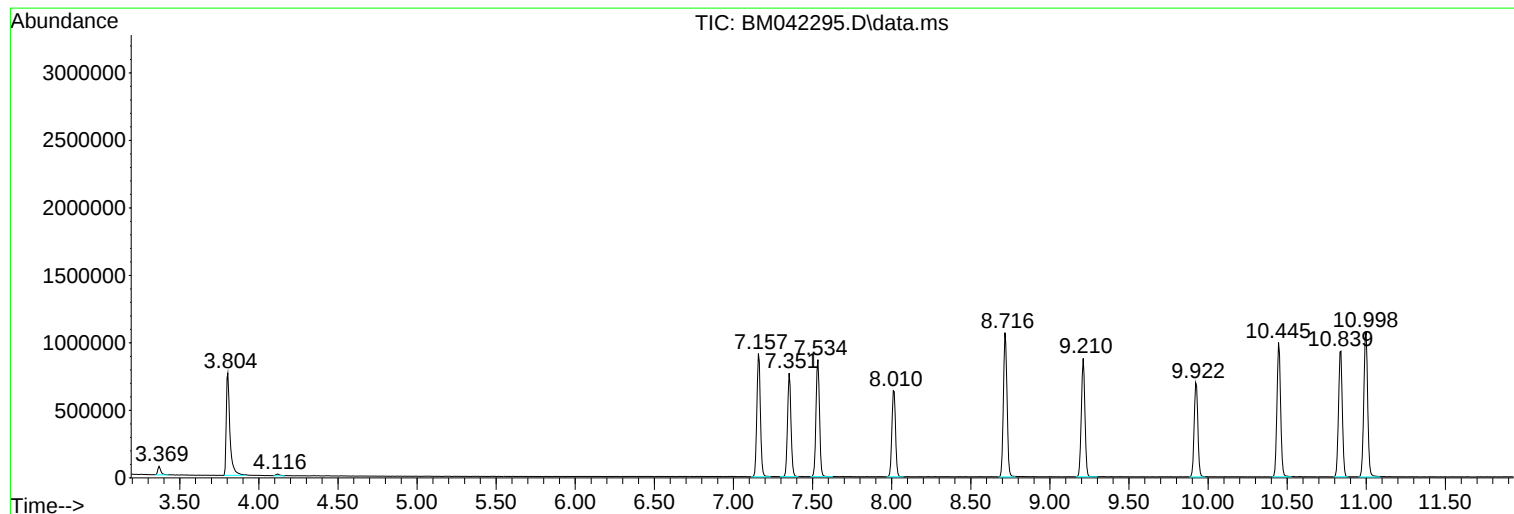

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042295.D
Acq On : 16 Oct 2023 12:50
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042295.D
Acq On : 16 Oct 2023 12:50
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------