

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042300.D
 Acq On : 16 Oct 2023 15:54
 Operator : MA/JU
 Sample : PB156296BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	40	rVB	55378	82798	1.95%	0.177%
2	3.804	101	105	122	rBV	743103	1183177	27.81%	2.531%
3	4.122	155	159	165	rBV2	8884	11853	0.28%	0.025%
4	7.163	669	676	693	rVB	835221	1288192	30.28%	2.756%
5	7.357	701	709	719	rBV	699153	1091057	25.64%	2.334%
6	7.534	732	739	754	rBV	813830	1273169	29.92%	2.724%
7	8.016	814	821	831	rBV	622069	950550	22.34%	2.034%
8	8.722	932	941	950	rBV	996485	1568843	36.87%	3.357%
9	9.210	1017	1024	1035	rBV	803880	1309098	30.77%	2.801%
10	9.928	1139	1146	1155	rBV	659907	1051667	24.72%	2.250%
11	10.451	1228	1235	1250	rVB	887669	1482049	34.83%	3.171%
12	10.839	1293	1301	1309	rBV	894951	1456674	34.24%	3.117%
13	10.998	1320	1328	1346	rBV	1049166	1756959	41.29%	3.759%
14	12.422	1566	1570	1581	rVB2	13565	25971	0.61%	0.056%
15	13.504	1747	1754	1758	rVB2	10065	14004	0.33%	0.030%
16	14.074	1844	1851	1858	rBV	1725917	2374153	55.80%	5.080%
17	14.357	1893	1899	1909	rBV	1871417	2711028	63.72%	5.800%
18	14.657	1943	1950	1958	rBV	1363141	1932534	45.42%	4.135%
19	14.786	1968	1972	1976	rVB5	3872	5180	0.12%	0.011%
20	14.868	1976	1986	1997	rBV	936087	1351153	31.76%	2.891%
21	15.651	2112	2119	2127	rVB	2316868	3333744	78.35%	7.133%
22	15.774	2133	2140	2153	rBV	930514	1183212	27.81%	2.532%
23	15.886	2155	2159	2163	rVB2	9739	13768	0.32%	0.029%
24	17.198	2377	2382	2386	rBV5	3458	6064	0.14%	0.013%
25	17.409	2411	2418	2425	rBV	1686502	2271504	53.39%	4.860%
26	17.509	2428	2435	2450	rVB	2616333	3603717	84.70%	7.710%
27	18.256	2558	2562	2564	rBV4	5354	6381	0.15%	0.014%
28	19.362	2745	2750	2755	rBV3	26079	38424	0.90%	0.082%
29	19.433	2757	2762	2766	rBV	27964	38670	0.91%	0.083%
30	19.527	2775	2778	2782	rBV6	5738	6668	0.16%	0.014%
31	19.674	2800	2803	2806	rBV3	9777	10274	0.24%	0.022%
32	19.798	2818	2824	2836	rBV	3267962	4223189	99.26%	9.036%
33	21.592	3124	3129	3136	rBV	1928379	2355051	55.35%	5.039%
34	23.909	3516	3523	3542	rVB	2249667	4254854	100.00%	9.104%
35	24.068	3543	3550	3563	rVB	1203837	2472761	58.12%	5.291%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042300.D
Acq On : 16 Oct 2023 15:54
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46738390

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042300.D
Acq On : 16 Oct 2023 15:54
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

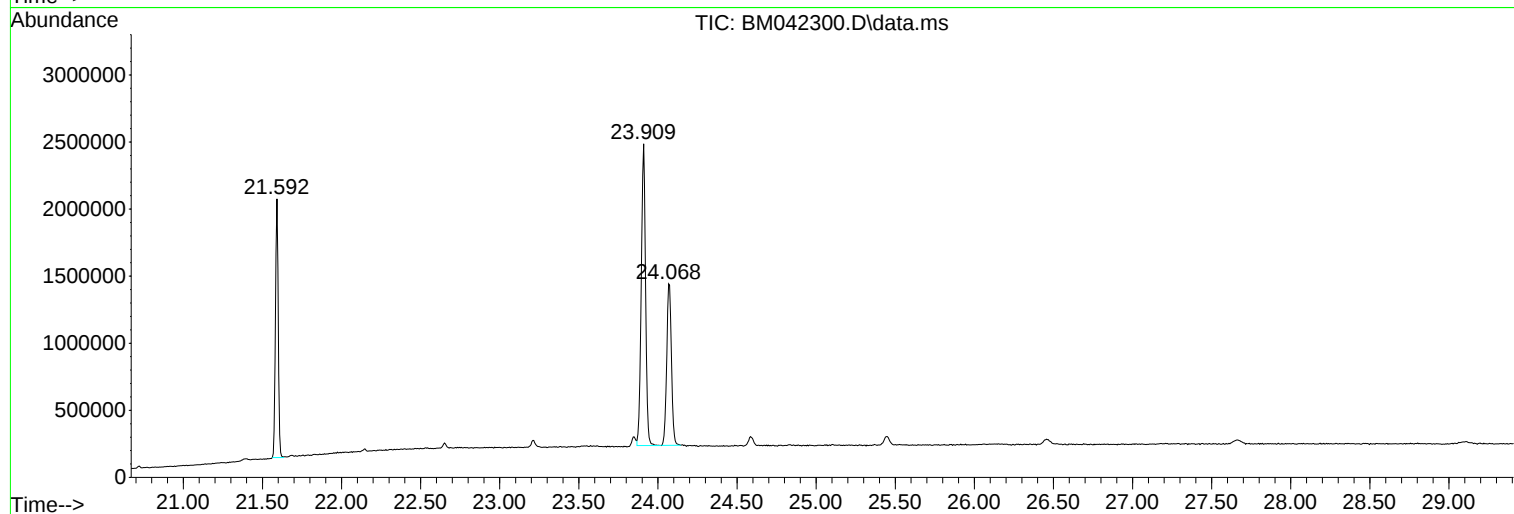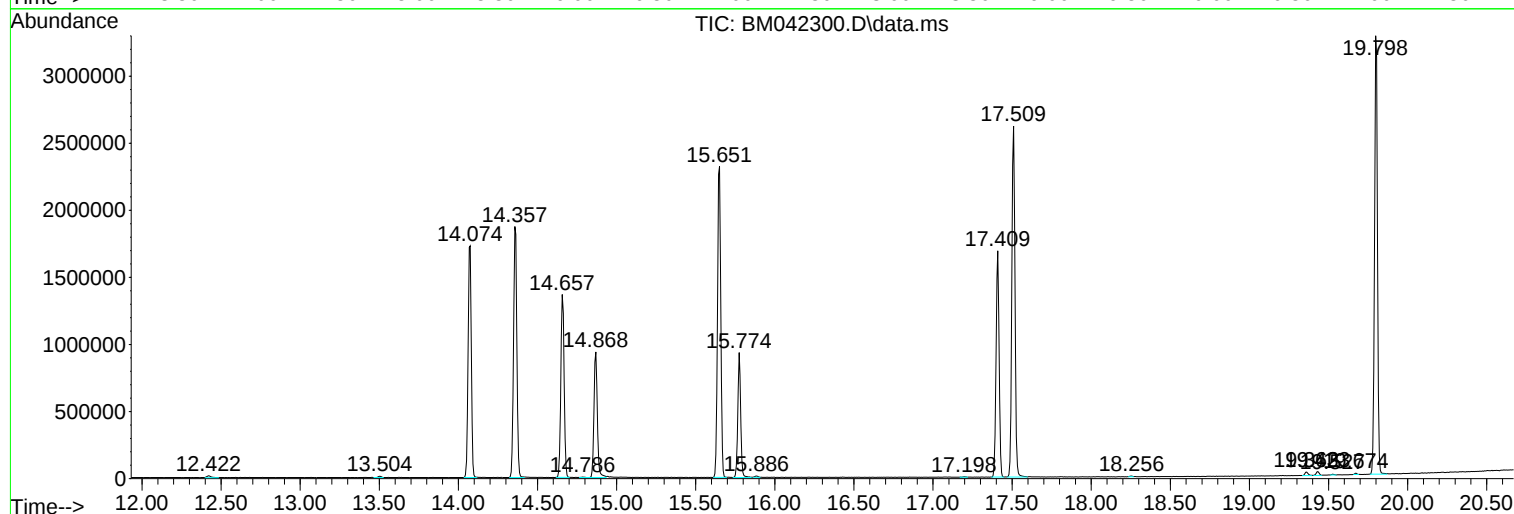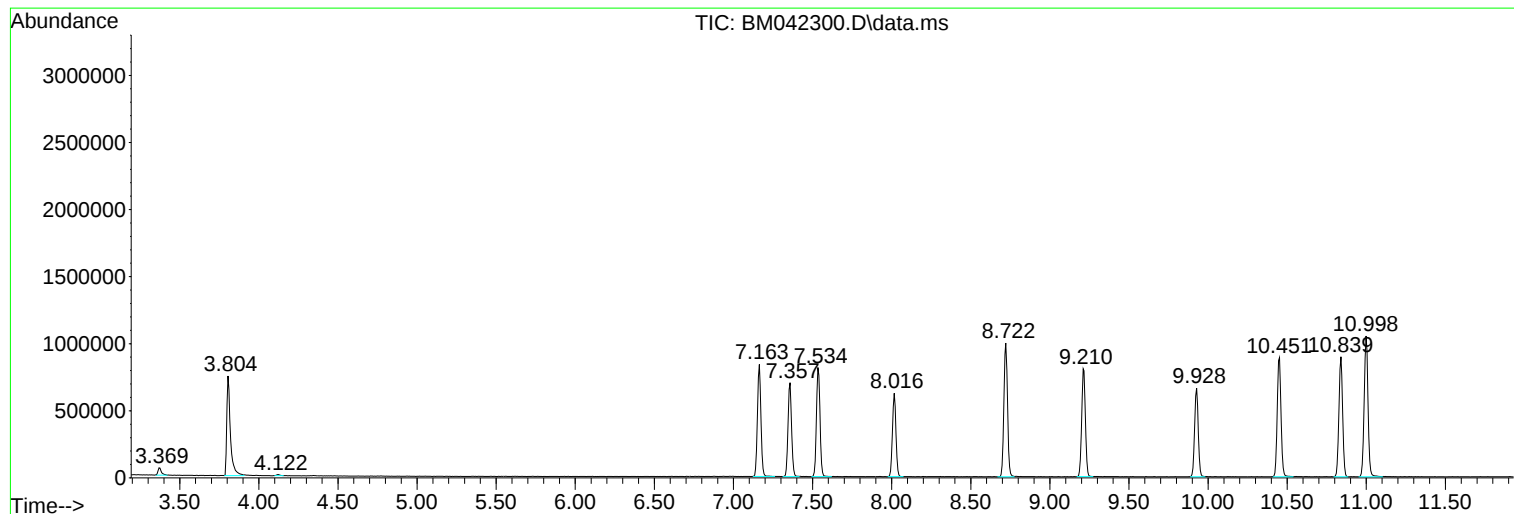

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042300.D
Acq On : 16 Oct 2023 15:54
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042300.D
Acq On : 16 Oct 2023 15:54
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc