

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042301.D
 Acq On : 16 Oct 2023 16:31
 Operator : MA/JU
 Sample : PB156298BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK298

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	44	rVB	63299	91234	1.98%	0.188%
2	3.805	101	105	127	rBV	827661	1326094	28.84%	2.725%
3	4.122	155	159	163	rVB	9152	12017	0.26%	0.025%
4	4.763	265	268	273	rVB7	2665	5070	0.11%	0.010%
5	7.163	669	676	686	rBV	928868	1422207	30.93%	2.923%
6	7.357	702	709	718	rBV	793032	1199846	26.10%	2.466%
7	7.534	732	739	749	rBV	886483	1390668	30.25%	2.858%
8	8.016	814	821	829	rBV	568322	862905	18.77%	1.773%
9	8.722	933	941	949	rBV	1113564	1727438	37.57%	3.550%
10	9.216	1015	1025	1037	rBV	872978	1453064	31.60%	2.986%
11	9.928	1138	1146	1155	rBV	707567	1160460	25.24%	2.385%
12	10.451	1227	1235	1246	rBV	977118	1615978	35.15%	3.321%
13	10.839	1294	1301	1310	rVB	798390	1319634	28.70%	2.712%
14	10.998	1320	1328	1347	rBV	1140253	1909885	41.54%	3.925%
15	12.422	1565	1570	1579	rVB2	14847	26277	0.57%	0.054%
16	13.498	1749	1753	1758	rBV3	7791	10857	0.24%	0.022%
17	14.075	1844	1851	1859	rBV	1927978	2582467	56.17%	5.307%
18	14.357	1893	1899	1908	rBV	2043950	2967451	64.54%	6.099%
19	14.657	1943	1950	1960	rBV	1206420	1730667	37.64%	3.557%
20	14.786	1969	1972	1976	rVB4	4892	5914	0.13%	0.012%
21	14.869	1979	1986	2000	rBV	1068105	1494013	32.50%	3.070%
22	15.651	2112	2119	2128	rBV	2595424	3619113	78.72%	7.438%
23	15.774	2134	2140	2151	rBV	1027146	1294082	28.15%	2.660%
24	15.886	2155	2159	2163	rVB2	11127	15632	0.34%	0.032%
25	16.421	2242	2250	2252	rBV7	2775	5461	0.12%	0.011%
26	17.410	2411	2418	2424	rBV	1498507	2020511	43.95%	4.153%
27	17.510	2428	2435	2450	rBV2	2800626	3910462	85.05%	8.037%
28	18.251	2558	2561	2567	rBV7	5303	6922	0.15%	0.014%
29	19.362	2745	2750	2754	rBV	31531	44325	0.96%	0.091%
30	19.433	2757	2762	2767	rVV	28116	40507	0.88%	0.083%
31	19.674	2799	2803	2806	rBV2	12519	15059	0.33%	0.031%
32	19.804	2818	2825	2834	rBV	3399074	4534644	98.63%	9.320%
33	20.721	2978	2981	2986	rBV6	16428	21111	0.46%	0.043%
34	21.592	3124	3129	3136	rBV	1655642	2047193	44.53%	4.207%
35	23.909	3516	3523	3539	rVB2	2354052	4597578	100.00%	9.449%
36	24.068	3544	3550	3563	rVB	1084921	2170270	47.20%	4.460%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042301.D
Acq On : 16 Oct 2023 16:31
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 48657016

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042301.D
Acq On : 16 Oct 2023 16:31
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

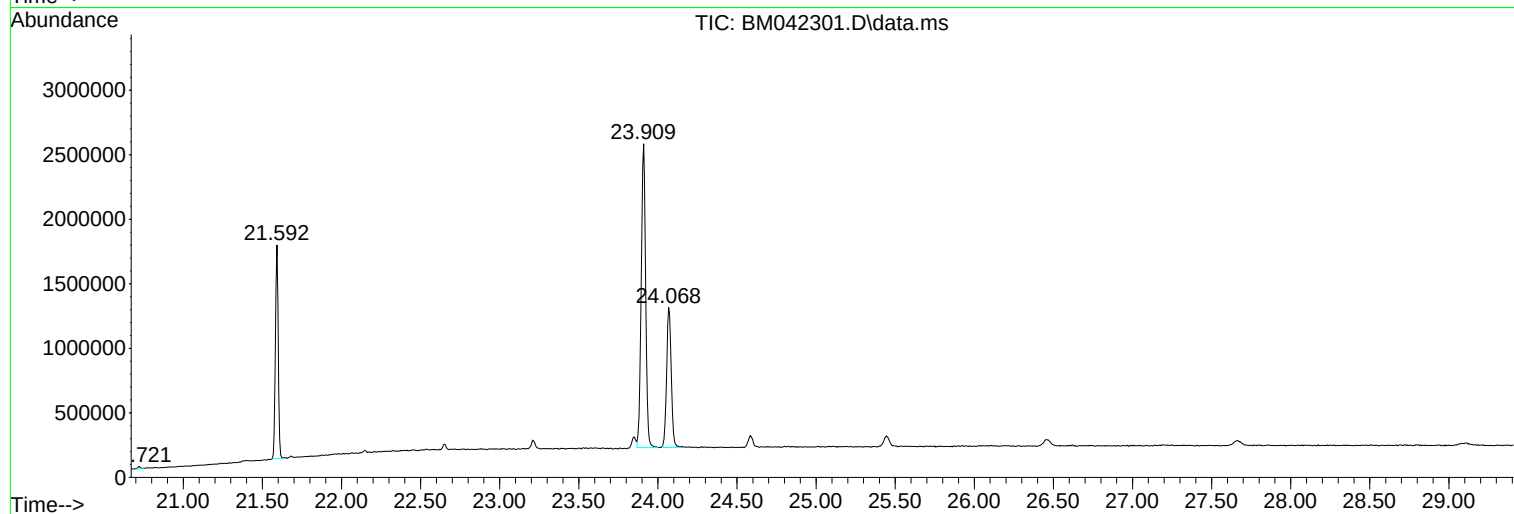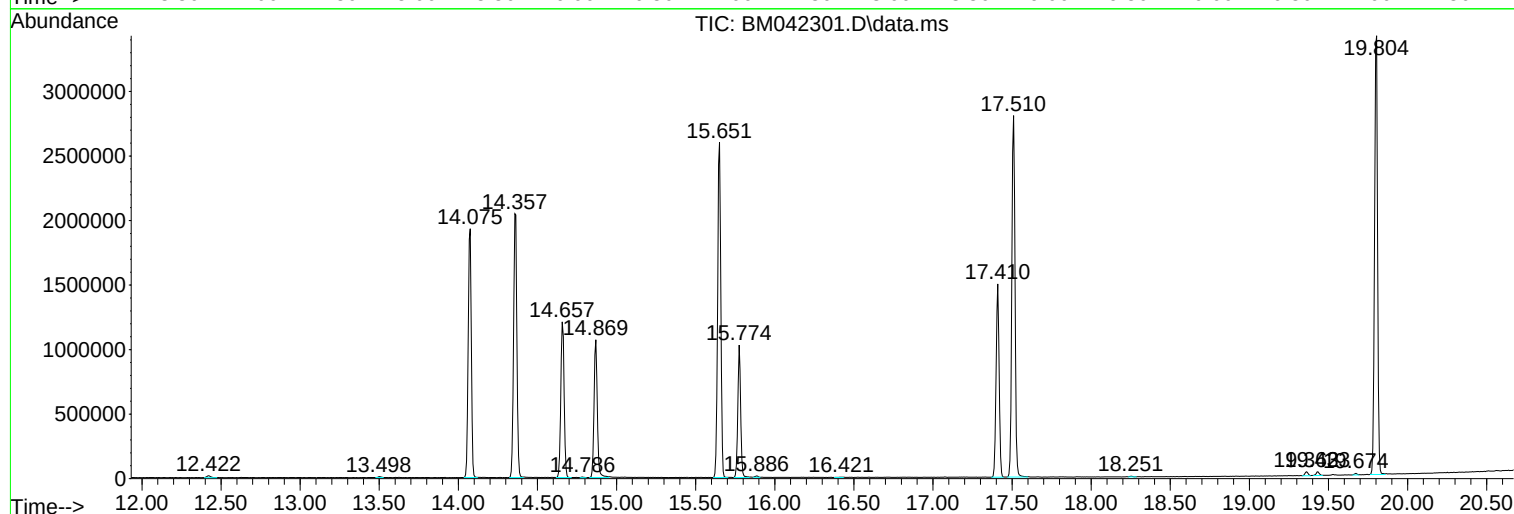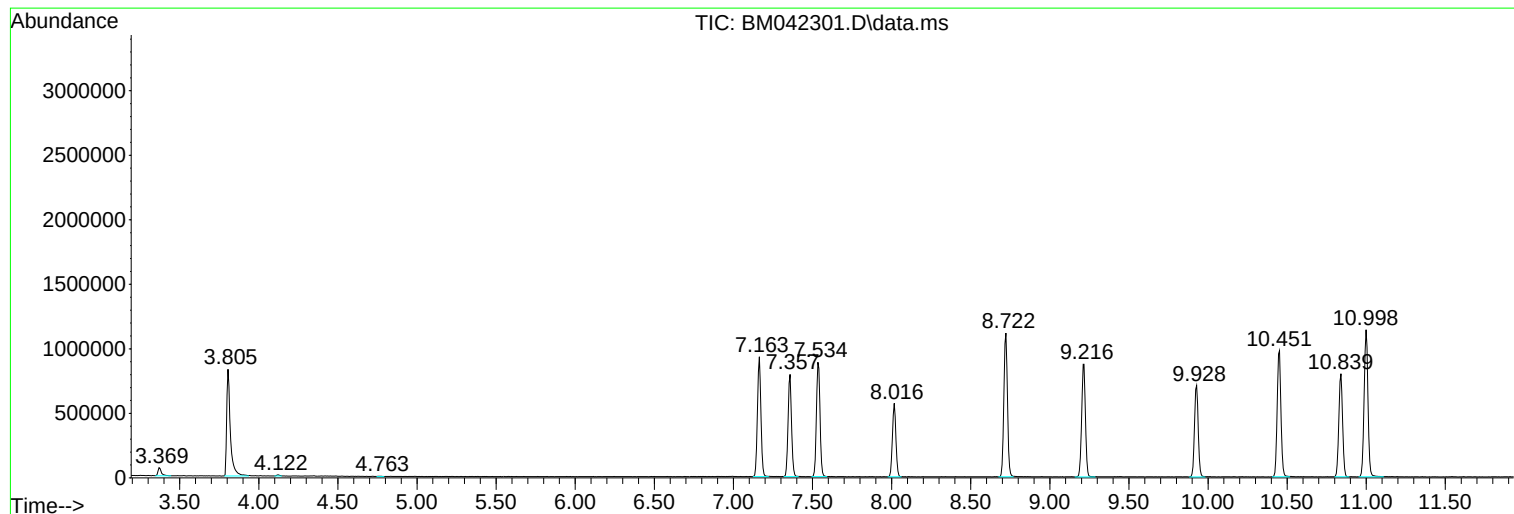

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042301.D
Acq On : 16 Oct 2023 16:31
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042301.D
Acq On : 16 Oct 2023 16:31
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc