

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042304.D
 Acq On : 16 Oct 2023 18:22
 Operator : MA/JU
 Sample : PB156402BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK402

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	39	rVB	53069	70922	1.73%	0.157%
2	3.810	102	106	125	rBV	298155	510828	12.46%	1.132%
3	4.122	155	159	166	rVB	13869	21444	0.52%	0.048%
4	7.163	668	676	690	rBV	809415	1250106	30.49%	2.771%
5	7.357	700	709	719	rBV	675339	1048911	25.58%	2.325%
6	7.534	732	739	750	rBV	772521	1209130	29.49%	2.680%
7	8.016	814	821	830	rBV	680511	1068914	26.07%	2.370%
8	8.722	933	941	956	rBV	960626	1509316	36.81%	3.346%
9	9.210	1015	1024	1035	rBV	776518	1261521	30.77%	2.797%
10	9.928	1138	1146	1159	rBV	630689	1018684	24.85%	2.258%
11	10.451	1227	1235	1249	rBV	860304	1433297	34.96%	3.177%
12	10.839	1293	1301	1309	rVB	1005390	1636401	39.91%	3.628%
13	10.998	1320	1328	1338	rBV	256215	446355	10.89%	0.989%
14	12.422	1565	1570	1581	rVB2	11403	21498	0.52%	0.048%
15	13.498	1749	1753	1757	rBV4	5673	8156	0.20%	0.018%
16	14.074	1844	1851	1860	rBV	1653851	2304056	56.20%	5.108%
17	14.357	1893	1899	1908	rBV	1837309	2607782	63.61%	5.781%
18	14.657	1943	1950	1959	rBV	1480331	2161059	52.71%	4.791%
19	14.780	1970	1971	1978	rVB4	2607	4799	0.12%	0.011%
20	14.868	1978	1986	2000	rBV	929356	1330510	32.45%	2.949%
21	15.651	2112	2119	2126	rBV	2254388	3231931	78.83%	7.165%
22	15.774	2134	2140	2155	rBV	900405	1160433	28.30%	2.572%
23	15.886	2155	2159	2164	rVV5	11450	17047	0.42%	0.038%
24	17.192	2378	2381	2389	rBV5	3637	7562	0.18%	0.017%
25	17.410	2411	2418	2427	rBV	1813010	2540295	61.96%	5.631%
26	17.509	2428	2435	2454	rVV	2605110	3577714	87.26%	7.931%
27	18.251	2558	2561	2567	rVB7	4008	4825	0.12%	0.011%
28	19.356	2746	2749	2755	rVB2	23001	31951	0.78%	0.071%
29	19.433	2758	2762	2766	rVB	27237	34216	0.83%	0.076%
30	19.527	2775	2778	2782	rBV4	5448	8668	0.21%	0.019%
31	19.674	2800	2803	2806	rBV4	10953	12464	0.30%	0.028%
32	19.798	2818	2824	2831	rBV	3225282	4099957	100.00%	9.089%
33	21.592	3123	3129	3136	rBV	2116983	2679093	65.34%	5.939%
34	23.903	3515	3522	3535	rVB2	2058647	4044216	98.64%	8.965%
35	24.068	3543	3550	3561	rVB	1334934	2735842	66.73%	6.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042304.D
Acq On : 16 Oct 2023 18:22
Operator : MA/JU
Sample : PB156402BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK402

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 45109903

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042304.D
Acq On : 16 Oct 2023 18:22
Operator : MA/JU
Sample : PB156402BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

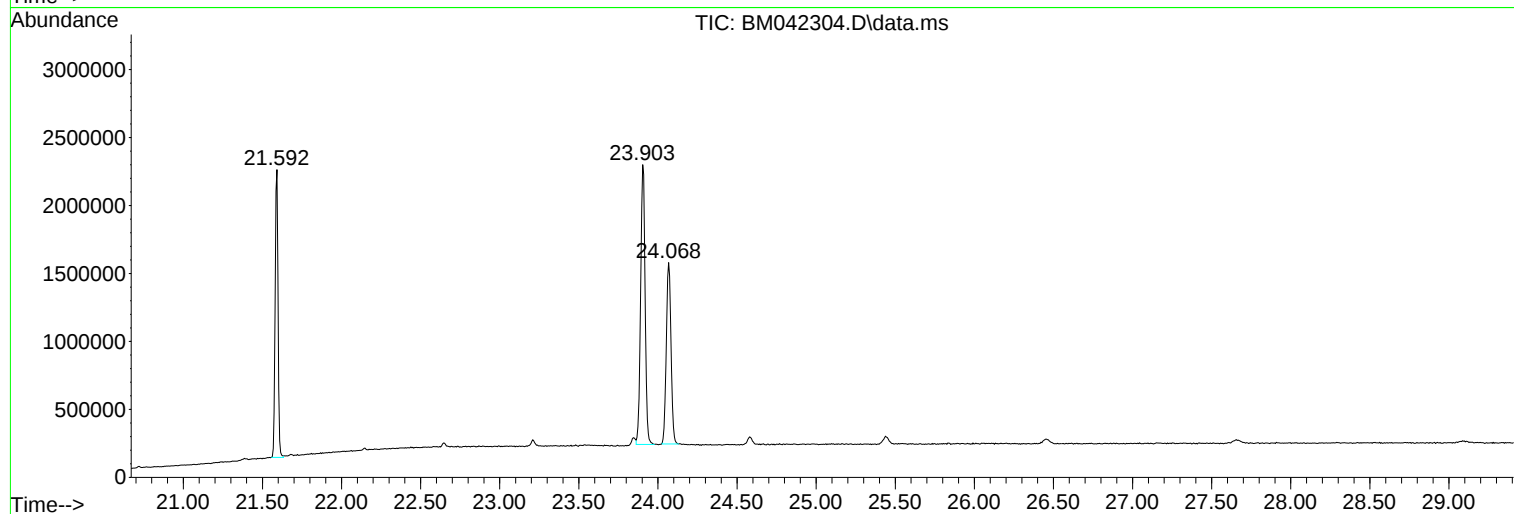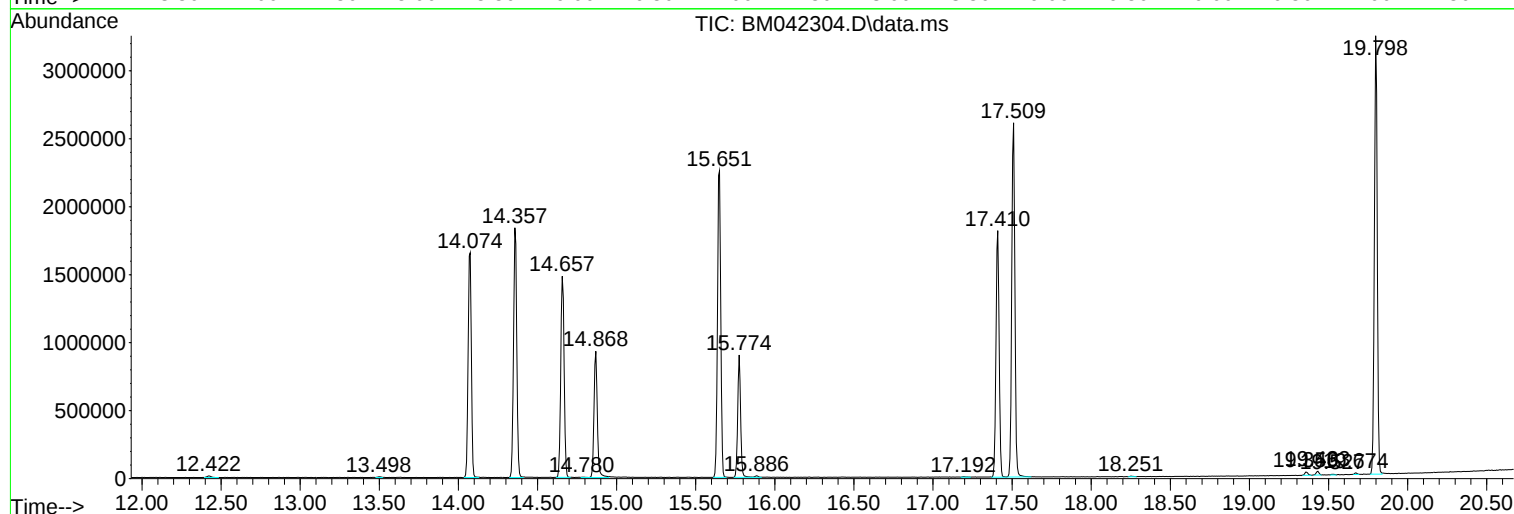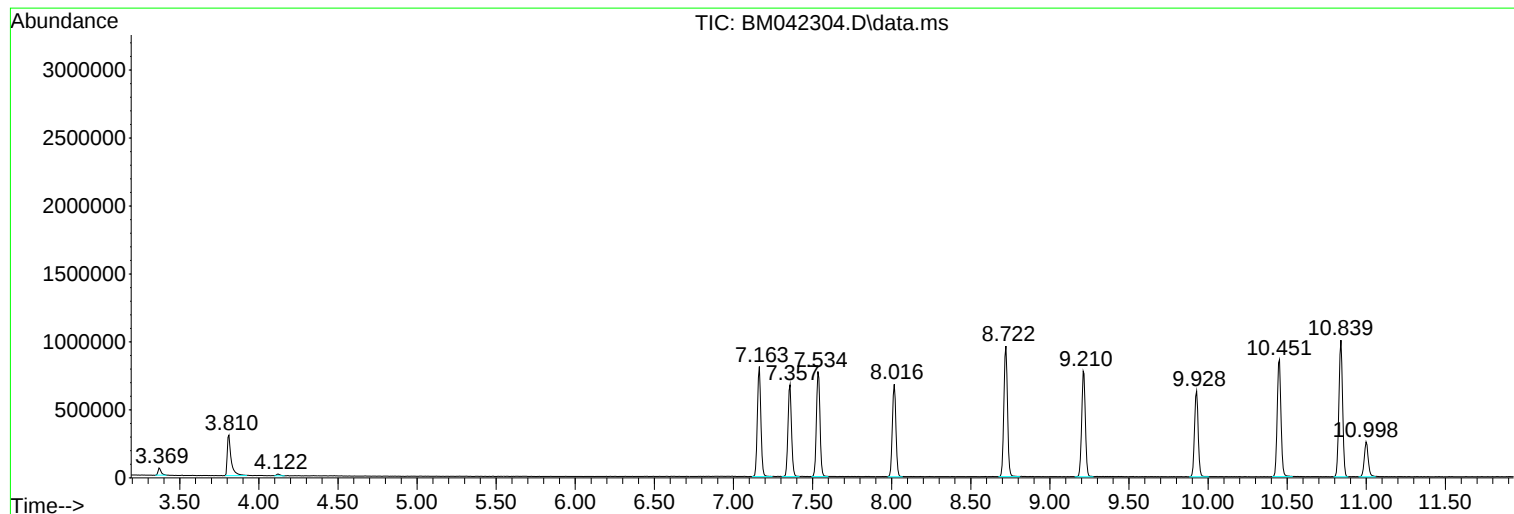

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042304.D
Acq On : 16 Oct 2023 18:22
Operator : MA/JU
Sample : PB156402BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042304.D
Acq On : 16 Oct 2023 18:22
Operator : MA/JU
Sample : PB156402BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------