

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042305.D
 Acq On : 16 Oct 2023 18:59
 Operator : MA/JU
 Sample : PB156404BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	41	rVB	53475	77729	1.89%	0.179%
2	3.810	102	106	124	rBV	305900	517777	12.60%	1.192%
3	4.122	155	159	168	rVB	13662	22660	0.55%	0.052%
4	7.163	669	676	685	rBV	837889	1281146	31.18%	2.948%
5	7.357	702	709	719	rBV	698289	1080021	26.29%	2.486%
6	7.534	732	739	749	rBV	777827	1226652	29.86%	2.823%
7	8.016	814	821	830	rVB	593974	927330	22.57%	2.134%
8	8.722	934	941	951	rBV	973619	1529361	37.23%	3.520%
9	9.210	1017	1024	1036	rBV	789326	1287054	31.33%	2.962%
10	9.928	1138	1146	1160	rBV	641672	1040357	25.32%	2.394%
11	10.451	1228	1235	1249	rBV	874108	1462842	35.61%	3.367%
12	10.839	1293	1301	1308	rBV	860549	1400845	34.10%	3.224%
13	10.998	1319	1328	1339	rBV	266811	473326	11.52%	1.089%
14	12.421	1564	1570	1576	rBV2	13697	22285	0.54%	0.051%
15	13.504	1747	1754	1758	rBV	20351	31993	0.78%	0.074%
16	14.068	1844	1850	1860	rBV	1708369	2332869	56.78%	5.369%
17	14.357	1892	1899	1906	rBV	1842825	2637146	64.19%	6.069%
18	14.657	1944	1950	1958	rVB	1289443	1841579	44.83%	4.238%
19	14.868	1979	1986	2002	rBV	957052	1338411	32.58%	3.080%
20	15.651	2112	2119	2127	rBV	2308220	3280301	79.85%	7.549%
21	15.774	2134	2140	2150	rBV	933776	1166626	28.40%	2.685%
22	15.886	2155	2159	2164	rVB3	9804	13535	0.33%	0.031%
23	17.198	2378	2382	2386	rBV4	3545	5293	0.13%	0.012%
24	17.409	2411	2418	2426	rVB	1585568	2141284	52.12%	4.928%
25	17.509	2428	2435	2448	rBV	2583782	3592733	87.45%	8.268%
26	17.803	2482	2485	2489	rBV6	2932	4715	0.11%	0.011%
27	19.356	2745	2749	2755	rBV2	26609	37912	0.92%	0.087%
28	19.427	2757	2761	2766	rVB	25708	36213	0.88%	0.083%
29	19.527	2775	2778	2782	rBV5	4935	6980	0.17%	0.016%
30	19.674	2799	2803	2807	rBV2	9392	11382	0.28%	0.026%
31	19.797	2818	2824	2832	rBV	3207409	4108282	100.00%	9.455%
32	21.591	3123	3129	3137	rBV	1744966	2207124	53.72%	5.079%
33	23.903	3515	3522	3533	rVB2	2090910	4037531	98.28%	9.292%
34	24.068	3543	3550	3561	rVB	1119290	2270979	55.28%	5.226%

Sum of corrected areas: 43452273

Instrument :

BNA_M

ClientSampleId :




SBLK404

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042305.D
Acq On : 16 Oct 2023 18:59
Operator : MA/JU
Sample : PB156404BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

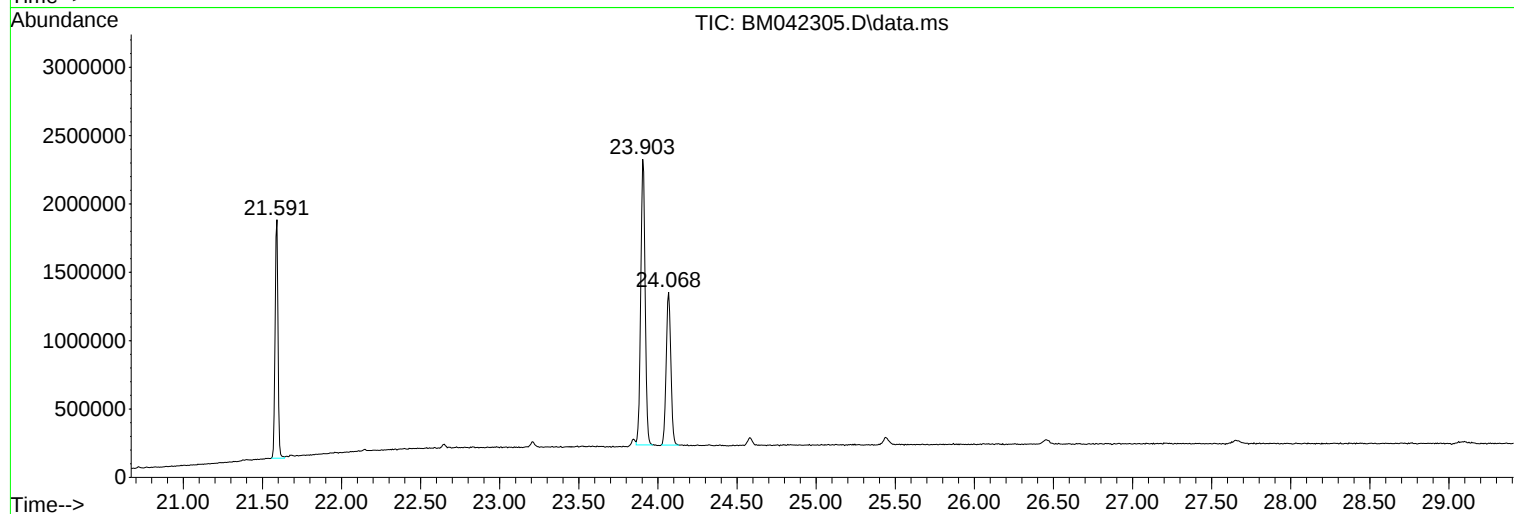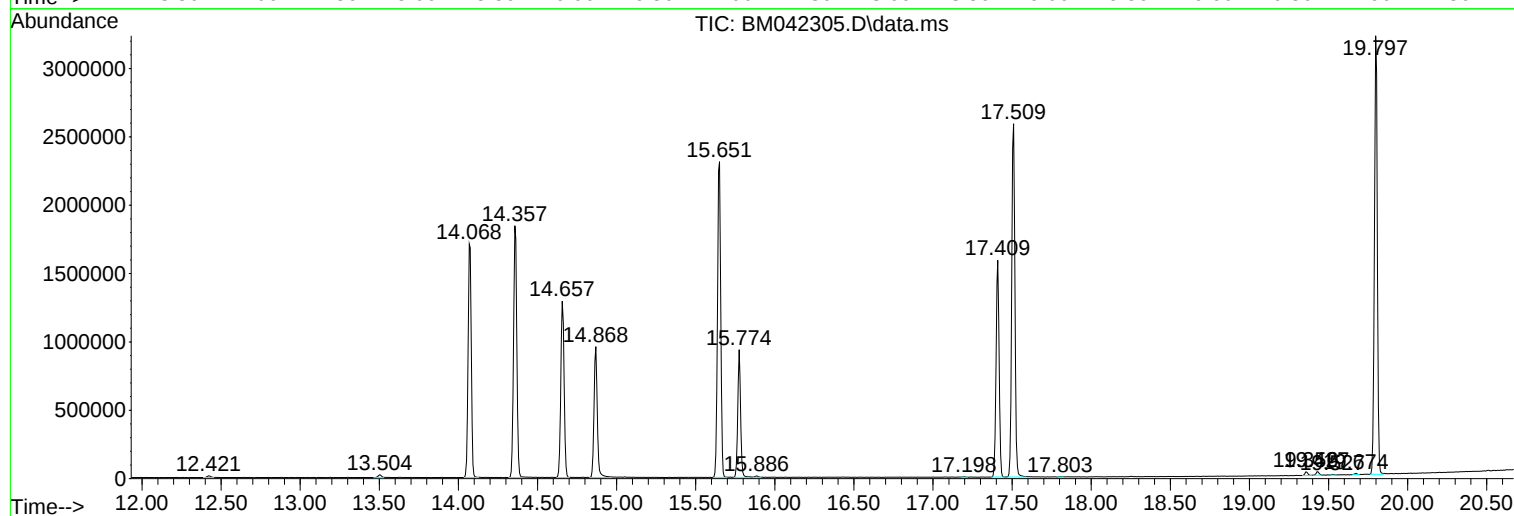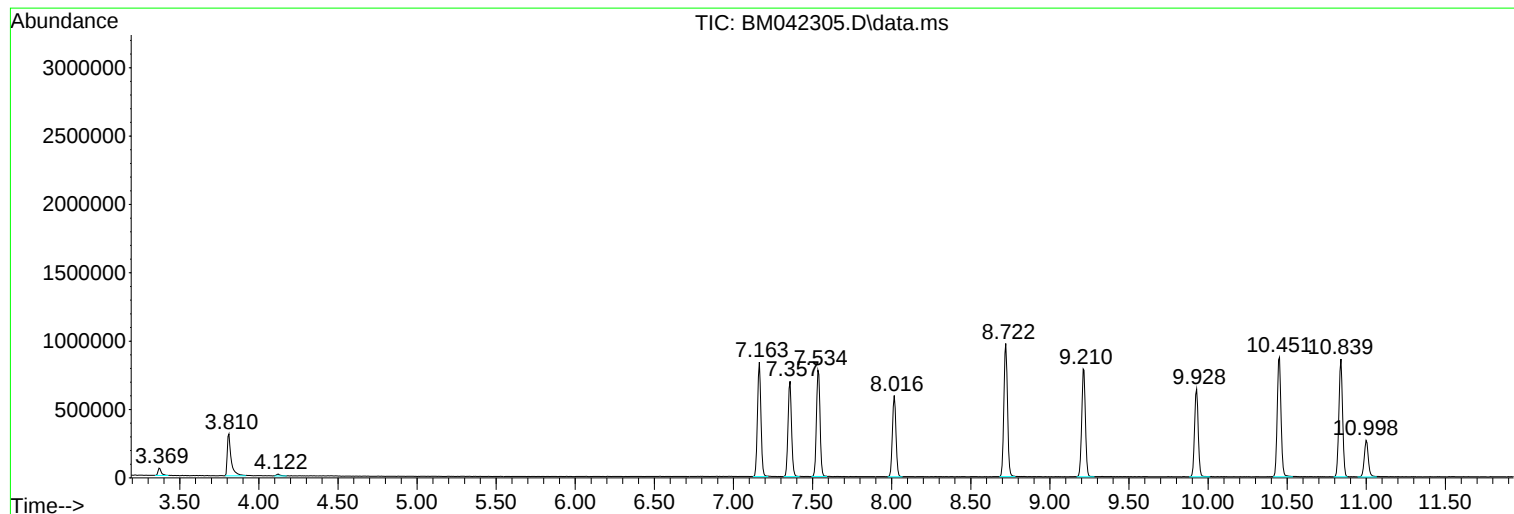

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042305.D
Acq On : 16 Oct 2023 18:59
Operator : MA/JU
Sample : PB156404BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042305.D
Acq On : 16 Oct 2023 18:59
Operator : MA/JU
Sample : PB156404BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc