

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042308.D
 Acq On : 16 Oct 2023 20:50
 Operator : MA/JU
 Sample : 04900-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	27	32	41	rVB	38472	57947	0.93%	0.107%
2	3.810	102	106	122	rBV	202580	339401	5.46%	0.628%
3	4.005	133	139	148	rVB	40024	61836	0.99%	0.114%
4	4.122	156	159	165	rVB	11635	15972	0.26%	0.030%
5	4.510	222	225	229	rVB4	6892	8911	0.14%	0.016%
6	5.057	314	318	324	rBV	12174	18096	0.29%	0.033%
7	5.646	412	418	424	rBV3	4159	7375	0.12%	0.014%
8	7.163	668	676	683	rBV	203421	318106	5.12%	0.589%
9	7.357	701	709	720	rBV	989976	1541509	24.80%	2.852%
10	7.534	733	739	749	rBV	852198	1305040	21.00%	2.414%
11	8.016	814	821	830	rVB	580071	905993	14.58%	1.676%
12	8.722	932	941	952	rBV	589893	949085	15.27%	1.756%
13	9.210	1016	1024	1036	rBV	1151172	1855274	29.85%	3.432%
14	9.422	1054	1060	1067	rVB	18562	27594	0.44%	0.051%
15	9.928	1139	1146	1159	rBV	912301	1454955	23.41%	2.692%
16	10.045	1159	1166	1170	rVB3	7447	16958	0.27%	0.031%
17	10.281	1203	1206	1211	rBV5	3643	6436	0.10%	0.012%
18	10.445	1227	1234	1248	rBV	1150684	1904833	30.65%	3.524%
19	10.839	1293	1301	1308	rBV	842485	1381771	22.23%	2.556%
20	10.998	1321	1328	1343	rBV	1078257	1781908	28.67%	3.297%
21	11.592	1424	1429	1436	rVB6	3483	7235	0.12%	0.013%
22	11.910	1478	1483	1489	rVB	21074	31374	0.50%	0.058%
23	12.416	1564	1569	1575	rVB2	19725	31952	0.51%	0.059%
24	13.233	1704	1708	1715	rVB7	4659	7898	0.13%	0.015%
25	13.504	1750	1754	1762	rBV	18823	26901	0.43%	0.050%
26	13.898	1813	1821	1825	rBV3	5037	7143	0.11%	0.013%
27	14.075	1844	1851	1862	rBV	2368897	3290872	52.95%	6.089%
28	14.357	1892	1899	1910	rBV2	2616611	3745649	60.27%	6.930%
29	14.657	1943	1950	1959	rBV	1271936	1814166	29.19%	3.356%
30	14.869	1980	1986	2001	rBV	175691	283087	4.55%	0.524%
31	15.651	2112	2119	2126	rBV	3321352	4734517	76.18%	8.759%
32	15.774	2134	2140	2150	rBV	1349007	1702613	27.39%	3.150%
33	15.880	2155	2158	2164	rVB	14024	19215	0.31%	0.036%
34	16.968	2337	2343	2348	rBV4	14983	19170	0.31%	0.035%
35	17.410	2411	2418	2426	rBV	1539271	2117029	34.06%	3.917%
36	17.510	2428	2435	2446	rBV	3796145	5359275	86.23%	9.915%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042308.D
 Acq On : 16 Oct 2023 20:50
 Operator : MA/JU
 Sample : 04900-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

37	18.027	2519	2523	2528	rBV7	3742	6504	0.10%	0.012%
38	18.251	2556	2561	2568	rBV	46899	64641	1.04%	0.120%
39	18.345	2574	2577	2582	rBV2	5261	6420	0.10%	0.012%
40	19.357	2745	2749	2755	rBV	39681	58057	0.93%	0.107%
41	19.427	2757	2761	2767	rVB	45923	63777	1.03%	0.118%
42	19.527	2774	2778	2786	rBV	43041	57009	0.92%	0.105%
43	19.668	2800	2802	2806	rVB2	18208	19711	0.32%	0.036%
44	19.798	2818	2824	2831	rBV	4769967	6215102	100.00%	11.499%
45	21.586	3123	3128	3134	rBV2	1680566	2158681	34.73%	3.994%
46	23.844	3508	3512	3515	rBV	88637	144142	2.32%	0.267%
47	23.903	3515	3522	3537	rVB2	3034916	5920014	95.25%	10.953%
48	24.062	3543	3549	3562	rVB	1058942	2179457	35.07%	4.032%




Sum of corrected areas: 54050611

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042308.D
Acq On : 16 Oct 2023 20:50
Operator : MA/JU
Sample : 04900-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

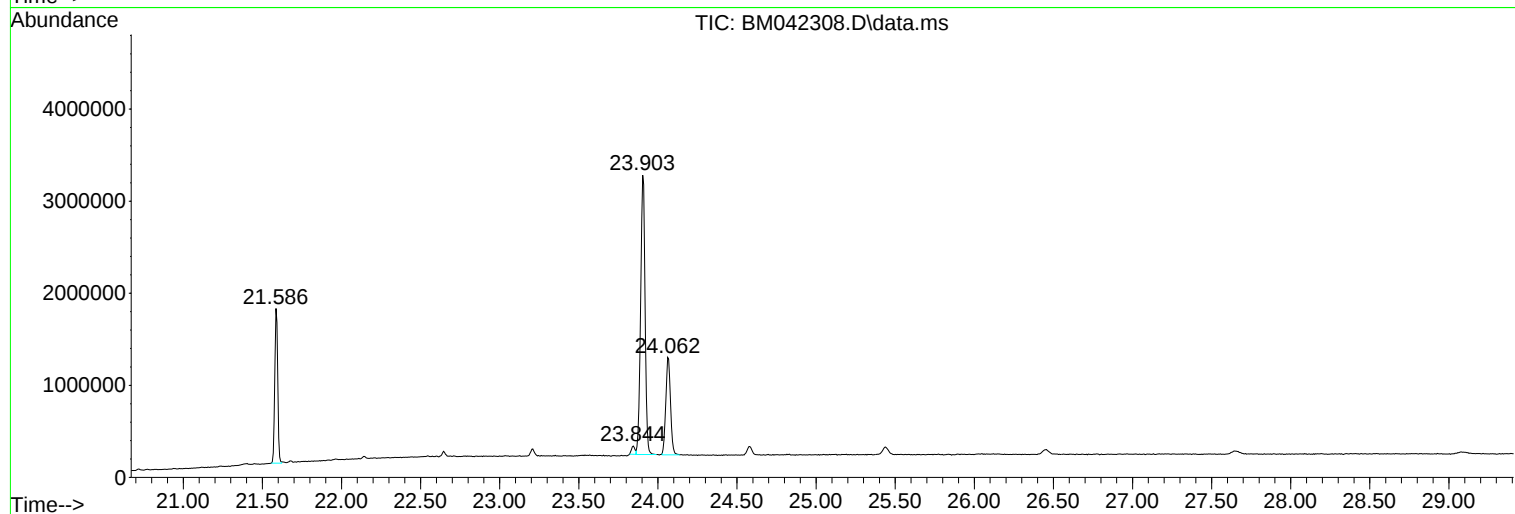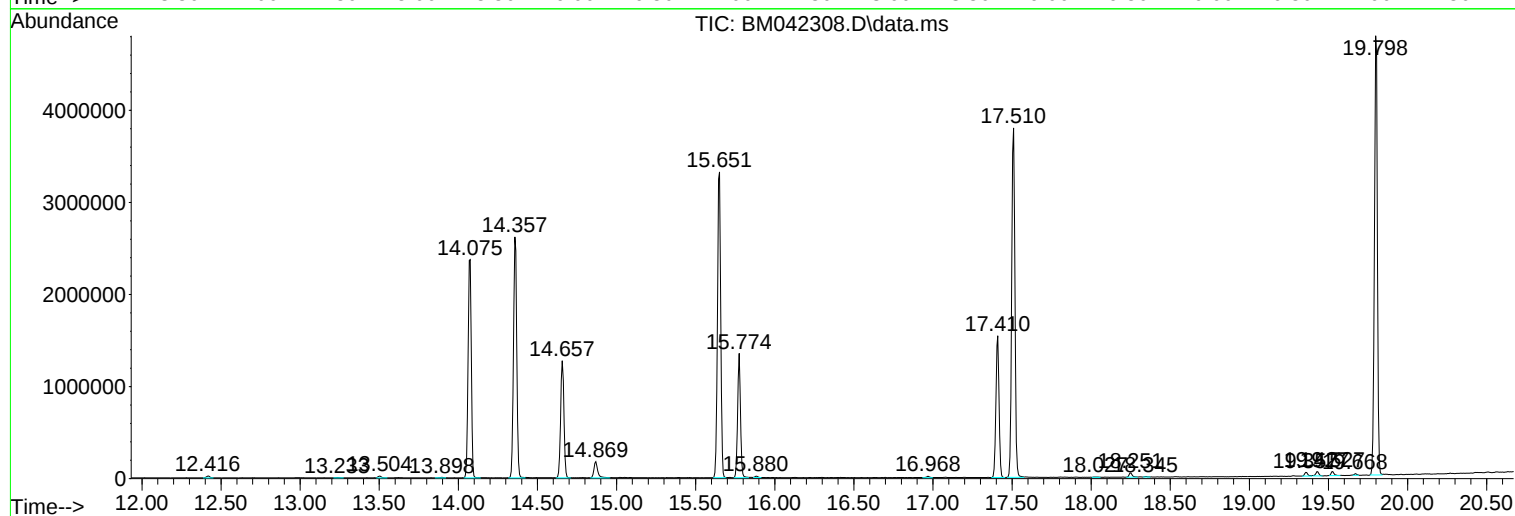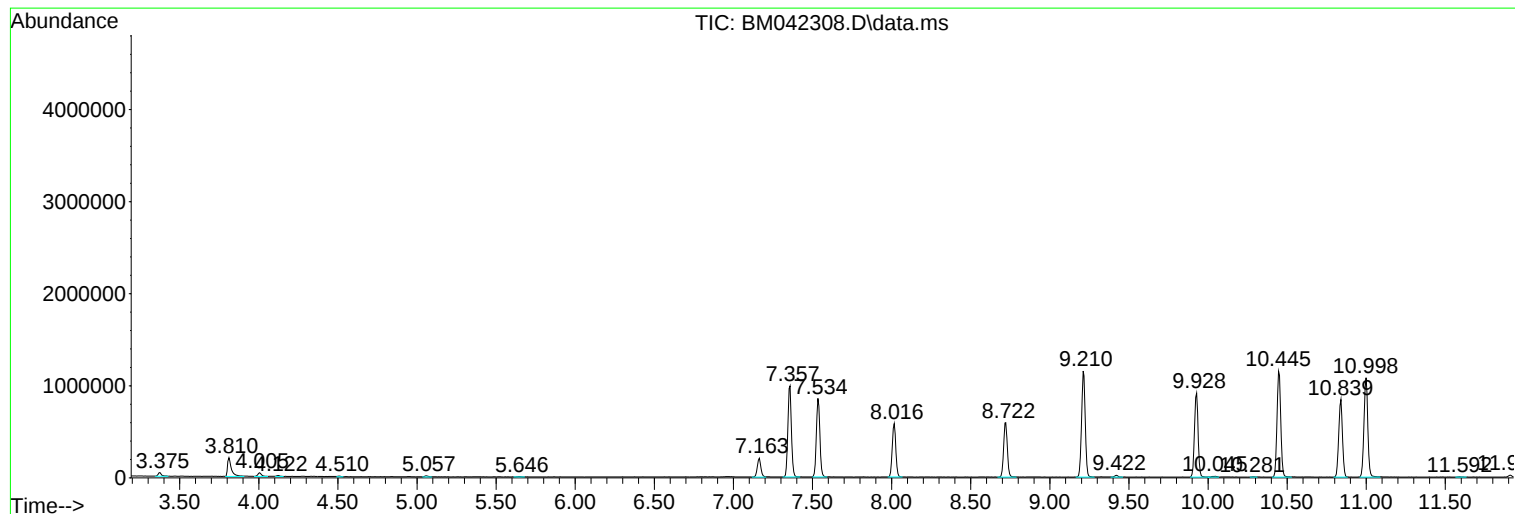

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042308.D
Acq On : 16 Oct 2023 20:50
Operator : MA/JU
Sample : 04900-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042308.D
Acq On : 16 Oct 2023 20:50
Operator : MA/JU
Sample : 04900-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------