

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
 Data File : BM042309.D
 Acq On : 16 Oct 2023 21:26
 Operator : MA/JU
 Sample : 04900-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	40	rBV	40872	61963	1.00%	0.113%
2	3.811	102	106	119	rBV	275725	448676	7.27%	0.815%
3	4.005	134	139	148	rVB	41705	66444	1.08%	0.121%
4	4.122	155	159	166	rVB	12961	20697	0.34%	0.038%
5	4.505	222	224	231	rVB6	7524	11159	0.18%	0.020%
6	5.058	314	318	323	rVB	13341	19591	0.32%	0.036%
7	7.163	669	676	686	rBV	220092	343494	5.57%	0.624%
8	7.357	699	709	721	rBV	1005115	1587041	25.72%	2.884%
9	7.534	732	739	753	rBV	884358	1381062	22.39%	2.510%
10	8.016	814	821	834	rBV	562363	890772	14.44%	1.619%
11	8.716	932	940	950	rBV	636510	1017488	16.49%	1.849%
12	9.210	1017	1024	1037	rBV	1213570	1928137	31.25%	3.504%
13	9.422	1055	1060	1067	rVB	10480	16167	0.26%	0.029%
14	9.928	1138	1146	1155	rBV	940304	1510430	24.48%	2.745%
15	10.045	1160	1166	1172	rVB3	10571	22062	0.36%	0.040%
16	10.287	1201	1207	1212	rVB2	4957	8182	0.13%	0.015%
17	10.445	1227	1234	1245	rBV	1217228	1986529	32.20%	3.610%
18	10.840	1292	1301	1311	rBV	831671	1355481	21.97%	2.464%
19	10.998	1319	1328	1345	rBV	1181222	1980210	32.10%	3.599%
20	11.592	1423	1429	1434	rBV8	4230	9773	0.16%	0.018%
21	11.910	1479	1483	1487	rVB2	11530	17002	0.28%	0.031%
22	12.422	1564	1570	1577	rVB	20578	35929	0.58%	0.065%
23	12.981	1660	1665	1670	rBV7	4495	7463	0.12%	0.014%
24	13.233	1705	1708	1713	rBV6	4095	6933	0.11%	0.013%
25	13.498	1748	1753	1759	rBV	13956	21506	0.35%	0.039%
26	14.075	1844	1851	1860	rBV	2478665	3379404	54.78%	6.142%
27	14.357	1892	1899	1914	rBV	2752238	3902377	63.25%	7.092%
28	14.657	1944	1950	1959	rVB	1238478	1785066	28.93%	3.244%
29	14.869	1977	1986	2002	rBV	189376	306227	4.96%	0.557%
30	15.645	2112	2118	2127	rBV	3417685	4883633	79.16%	8.876%
31	15.775	2133	2140	2152	rBV	1324358	1700467	27.56%	3.091%
32	15.886	2155	2159	2163	rVB2	13987	19530	0.32%	0.035%
33	16.969	2338	2343	2349	rVB	21872	27544	0.45%	0.050%
34	17.410	2411	2418	2425	rBV	1525191	2094439	33.95%	3.807%
35	17.510	2428	2435	2445	rBV	3937245	5323896	86.29%	9.676%
36	18.251	2556	2561	2570	rBV2	48109	73281	1.19%	0.133%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042309.D
Acq On : 16 Oct 2023 21:26
Operator : MA/JU
Sample : 04900-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Title : SVOA CALIBRATION

37	18.345	2574	2577	2583	rVB3	8033	13003	0.21%	0.024%
38	19.363	2745	2750	2756	rVV	39969	61418	1.00%	0.112%
39	19.427	2756	2761	2766	rVB	45051	65080	1.05%	0.118%
40	19.527	2774	2778	2784	rBV2	43338	58310	0.95%	0.106%
41	19.668	2799	2802	2808	rBV2	18449	21038	0.34%	0.038%
42	19.798	2818	2824	2832	rBV	4658494	6169471	100.00%	11.213%
43	21.586	3123	3128	3137	rBV	1705024	2166821	35.12%	3.938%
44	23.845	3508	3512	3515	rBV	81673	132504	2.15%	0.241%
45	23.903	3515	3522	3537	rVB2	2957405	5899519	95.62%	10.722%
46	24.062	3542	3549	3560	rVB	1074898	2184383	35.41%	3.970%




Sum of corrected areas: 55021602

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042309.D
Acq On : 16 Oct 2023 21:26
Operator : MA/JU
Sample : 04900-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

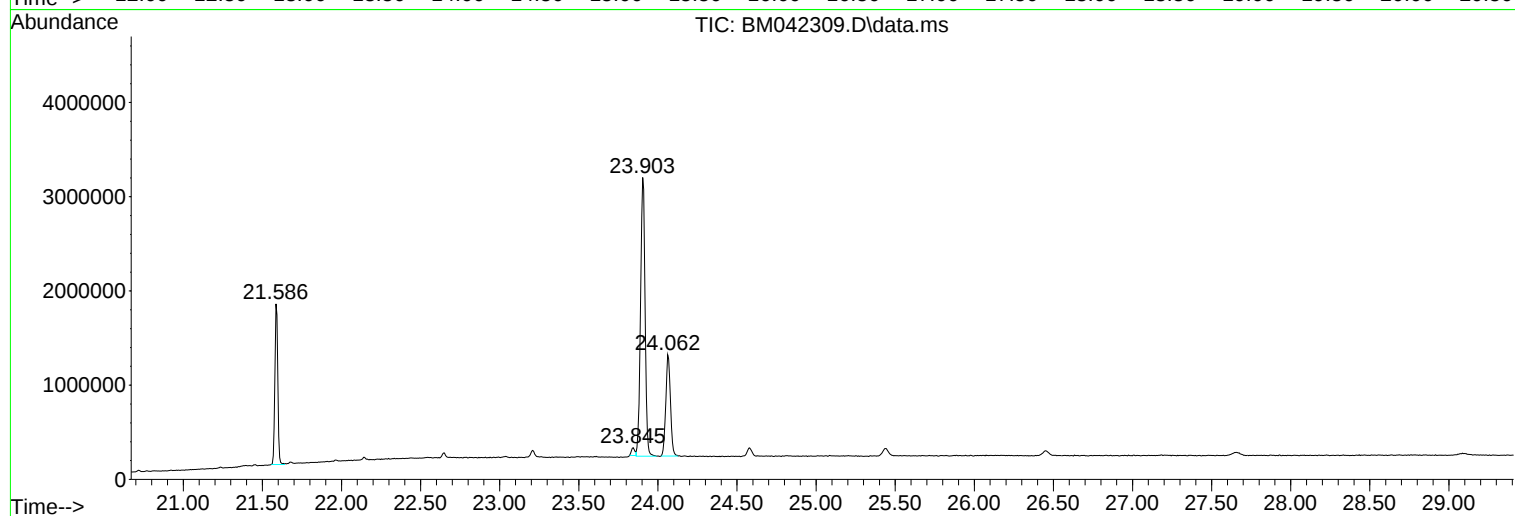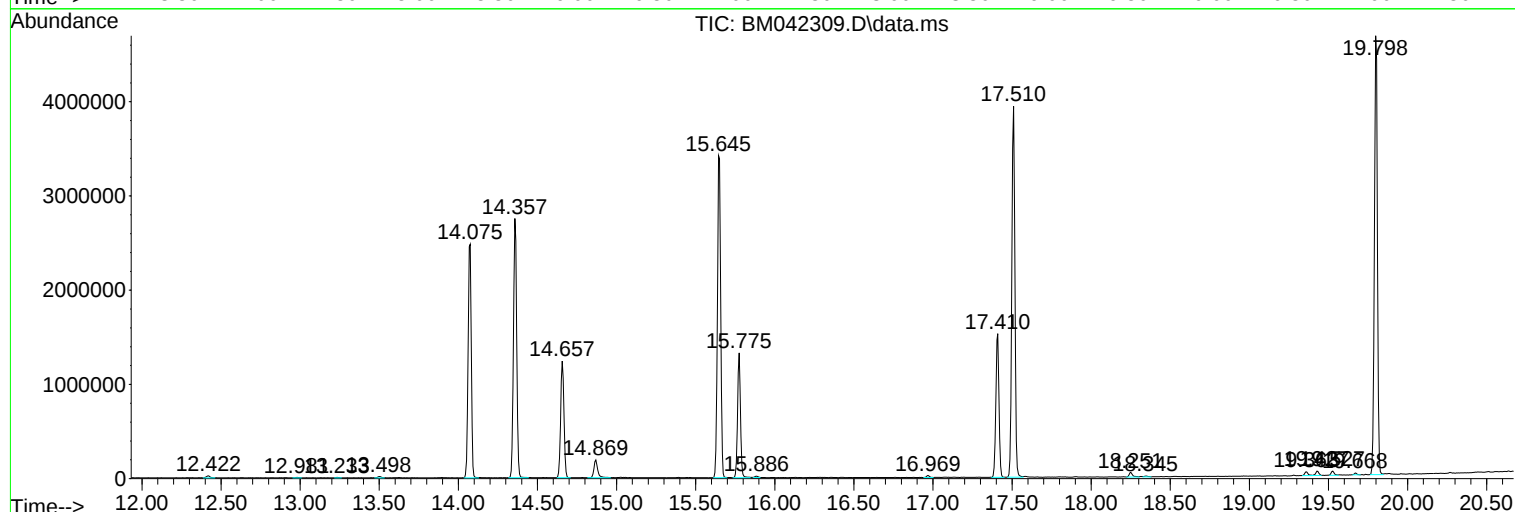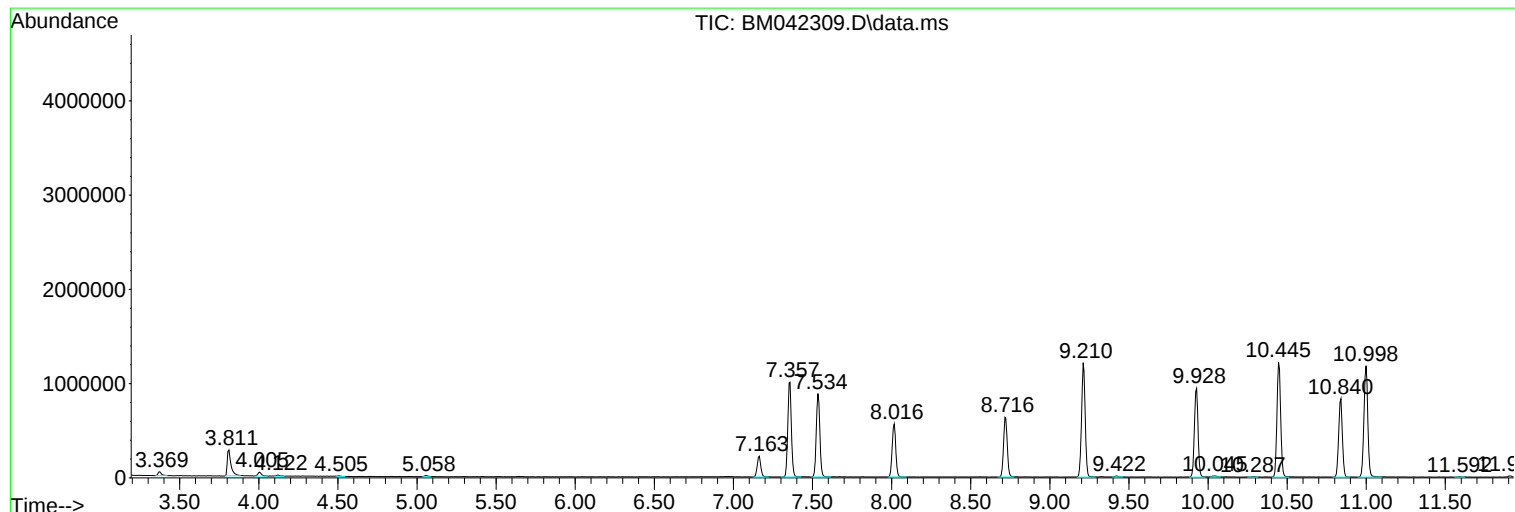

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042309.D
Acq On : 16 Oct 2023 21:26
Operator : MA/JU
Sample : 04900-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101623\
Data File : BM042309.D
Acq On : 16 Oct 2023 21:26
Operator : MA/JU
Sample : 04900-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc