


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM101718\
 Data File : BM017159.D
 Acq On : 17 Oct 2018 09:12
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

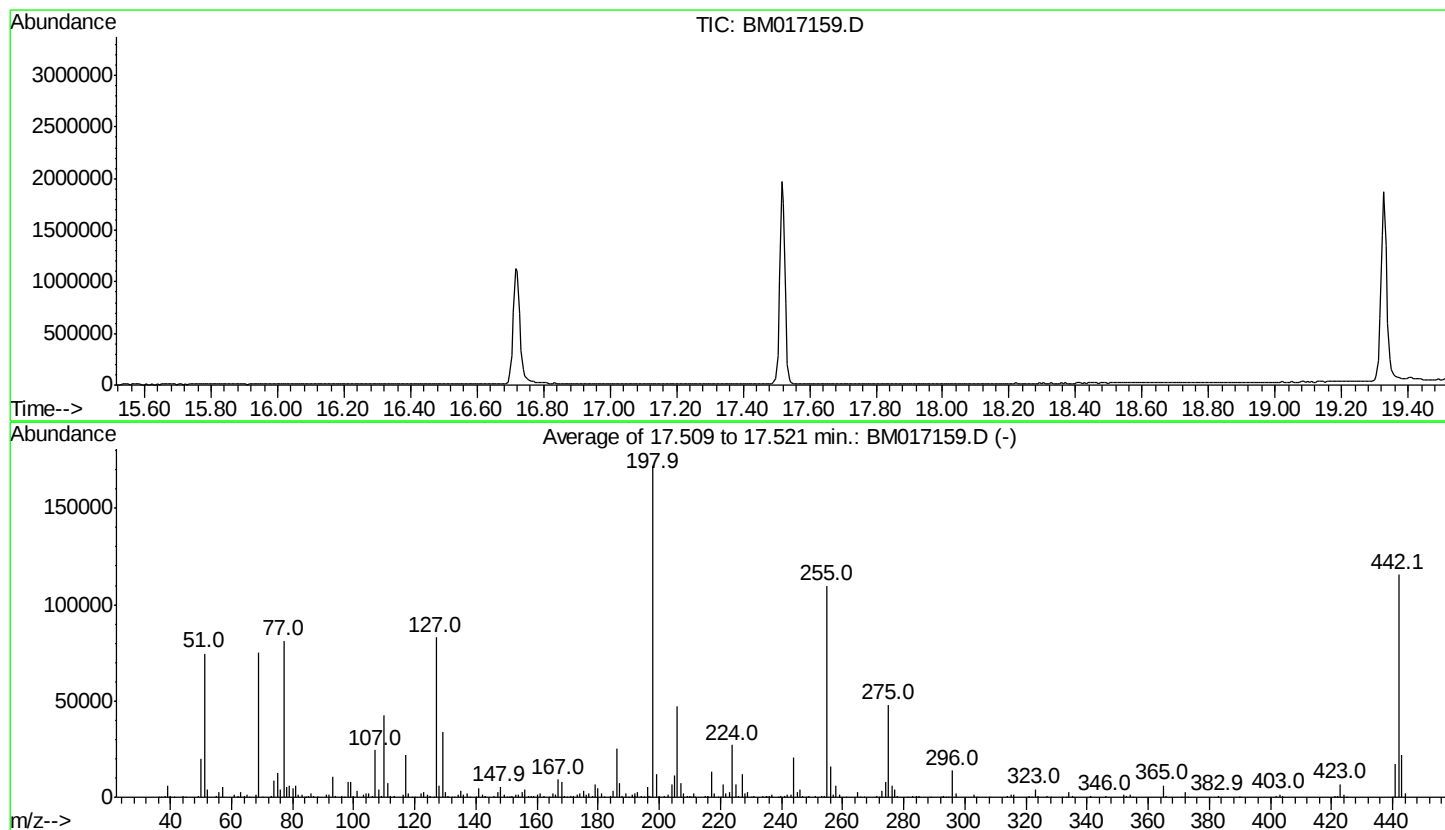

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	74680	PASS
68	69	0.00	2	1.5	1139	PASS
69	198	0.00	100	43.7	75317	PASS
70	69	0.00	2	0.4	298	PASS
127	198	10	80	48.2	82992	PASS
197	198	0.00	2	0.2	396	PASS
198	198	100	100	100.0	172181	PASS
199	198	5	9	6.8	11671	PASS
275	198	10	60	27.8	47898	PASS
365	198	1	100	3.7	6301	PASS
441	198	0.01	100	10.0	17202	PASS
442	198	50	100	67.2	115629	PASS
443	442	15	24	18.7	21672	PASS