


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM101718\
 Data File : BM017168.D
 Acq On : 17 Oct 2018 15:47
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

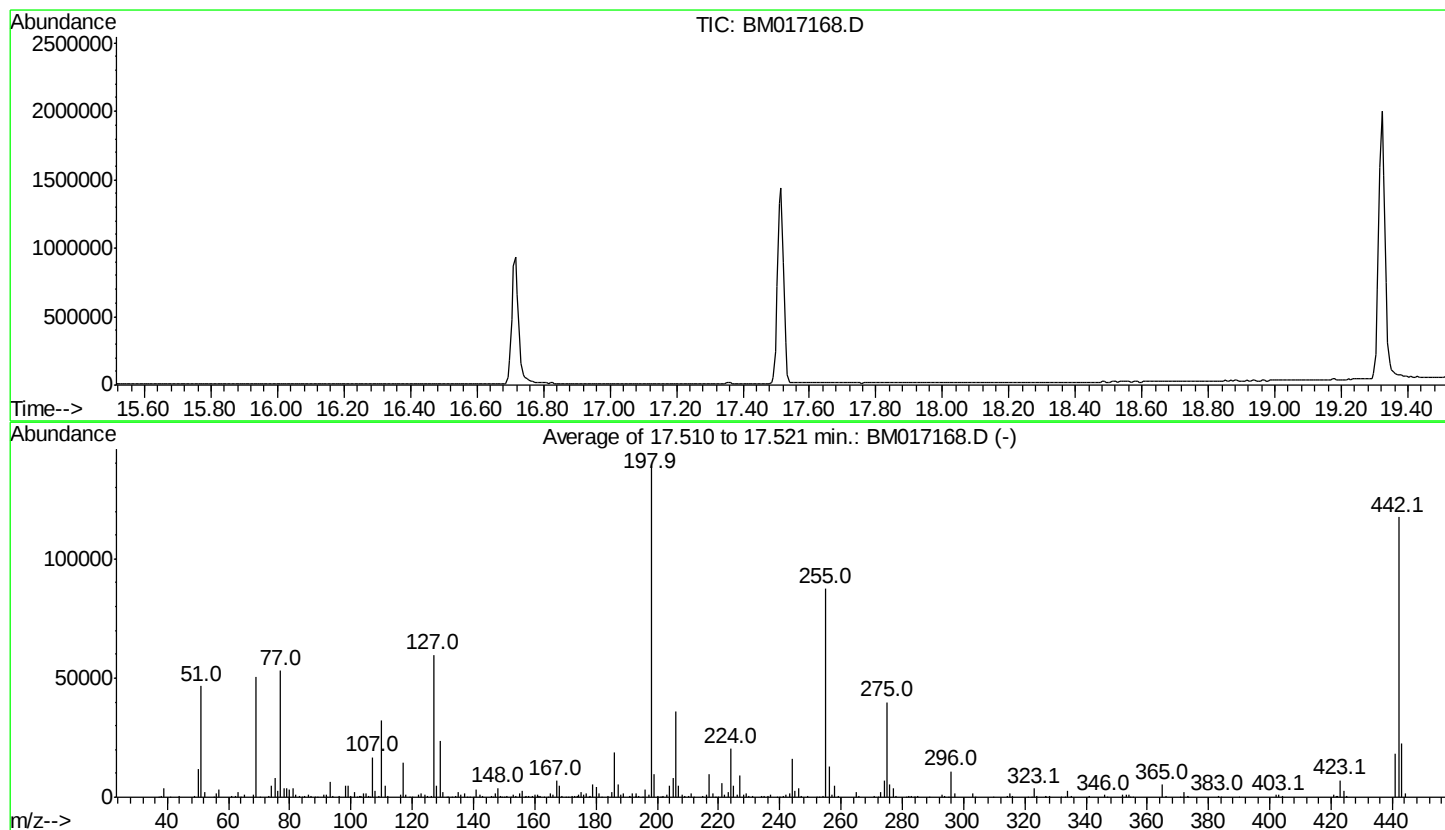

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	46613	PASS
68	69	0.00	2	2.0	998	PASS
69	198	0.00	100	36.1	50253	PASS
70	69	0.00	2	0.2	107	PASS
127	198	10	80	42.9	59653	PASS
197	198	0.00	2	0.7	983	PASS
198	198	100	100	100.0	139080	PASS
199	198	5	9	6.8	9481	PASS
275	198	10	60	28.7	39906	PASS
365	198	1	100	3.9	5371	PASS
441	198	0.01	100	13.2	18408	PASS
442	198	50	100	84.5	117544	PASS
443	442	15	24	19.1	22410	PASS