


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM101718\
 Data File : BM017177.D
 Acq On : 18 Oct 2018 03:46
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

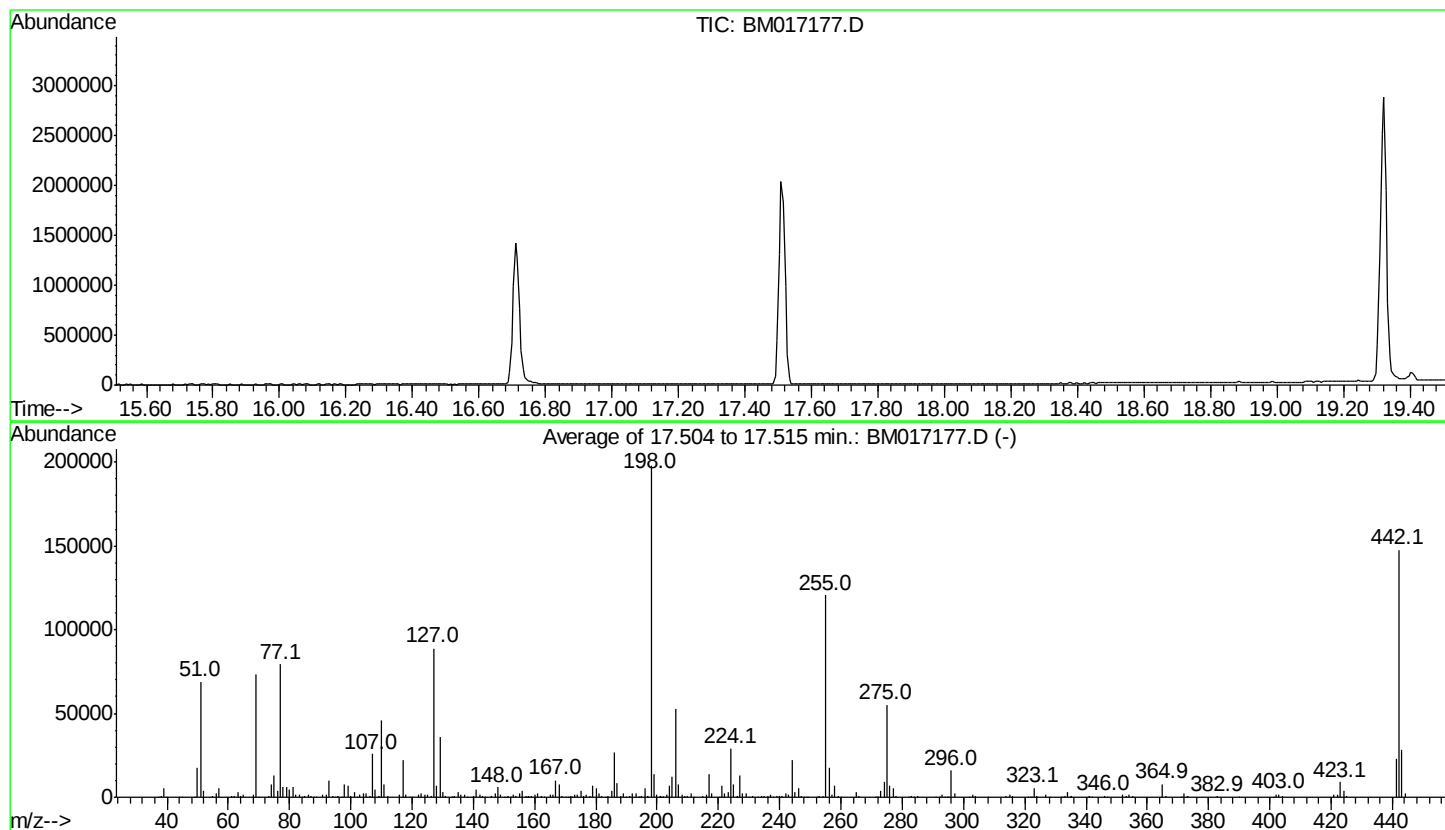

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	68848	PASS
68	69	0.00	2	2.0	1454	PASS
69	198	0.00	100	37.1	73328	PASS
70	69	0.00	2	0.3	248	PASS
127	198	10	80	44.9	88821	PASS
197	198	0.00	2	0.5	919	PASS
198	198	100	100	100.0	197824	PASS
199	198	5	9	6.9	13558	PASS
275	198	10	60	28.0	55344	PASS
365	198	1	100	3.9	7811	PASS
441	198	0.01	100	11.6	22907	PASS
442	198	50	100	74.7	147688	PASS
443	442	15	24	19.0	28086	PASS