

Data File : BM023241.D
Acq On : 18 Oct 2019 04:41
Operator : JU
Sample : K5262-18DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFB79DL

Quant Time: Oct 18 07:51:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 07:48:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	441740	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	1739390	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	1105542	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	2349728	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	2521298	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	3011008	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	3566	0.36	ng/uL	0.00
5) Phenol-d5	6.83	99	50999	1.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	29574	1.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	43241	1.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	40153	1.30	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	20441	1.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	19901	1.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	42948	1.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	31885	0.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	144227	1.70	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	163671	1.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	12418	0.91	ng/ul	0.00
58) Fluorene-d10	15.30	176	130367	1.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	7626	0.82	ng/ul	0.00
71) Anthracene-d10	17.15	188	212336	1.87	ng/ul	0.00
79) Pyrene-d10	19.44	212	241833	1.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	285602	1.87	ng/ul	0.00

Target Compounds


					Qvalue
48) Acenaphthylene	14.02	152	139415	1.372 ng/ul	98
50) Acenaphthene	14.37	153	105716	1.494 ng/ul	98
54) Dibenzofuran	14.70	168	131757	1.312 ng/ul	98
59) Fluorene	15.36	166	140293	1.703 ng/ul	99
70) Phenanthrene	17.09	178	2697046	20.453 ng/ul	100
72) Anthracene	17.18	178	578420	4.245 ng/ul	100
75) Carbazole	17.45	167	266230	2.187 ng/ul	98
77) Fluoranthene	19.12	202	4581837	29.215 ng/ul	98
80) Pyrene	19.47	202	3903644	24.715 ng/ul	100
83) Benzo(a)anthracene	21.23	228	2136121	12.504 ng/ul	98
85) Chrysene	21.27	228	2052768	12.941 ng/ul	97
88) Benzo(b)fluoranthene	22.79	252	3186935	17.457 ng/ul	98
89) Benzo(k)fluoranthene	22.79	252	3186935	18.180 ng/ul	97
91) Benzo(a)pyrene	23.36	252	2252774	12.862 ng/ul	97
92) Indeno(1,2,3-cd)pyrene	25.67	276	1763152	8.462 ng/ul	97
93) Dibenzo(a,h)anthracene	25.67	278	447232	2.567 ng/ul#	91
94) Benzo(g,h,i)perylene	26.34	276	1224340	7.137 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM023241.D
Acq On : 18 Oct 2019 04:41
Operator : JU
Sample : K5262-18DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFB79DL

Quant Time: Oct 18 07:51:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 07:48:41 2019
Response via : Initial Calibration

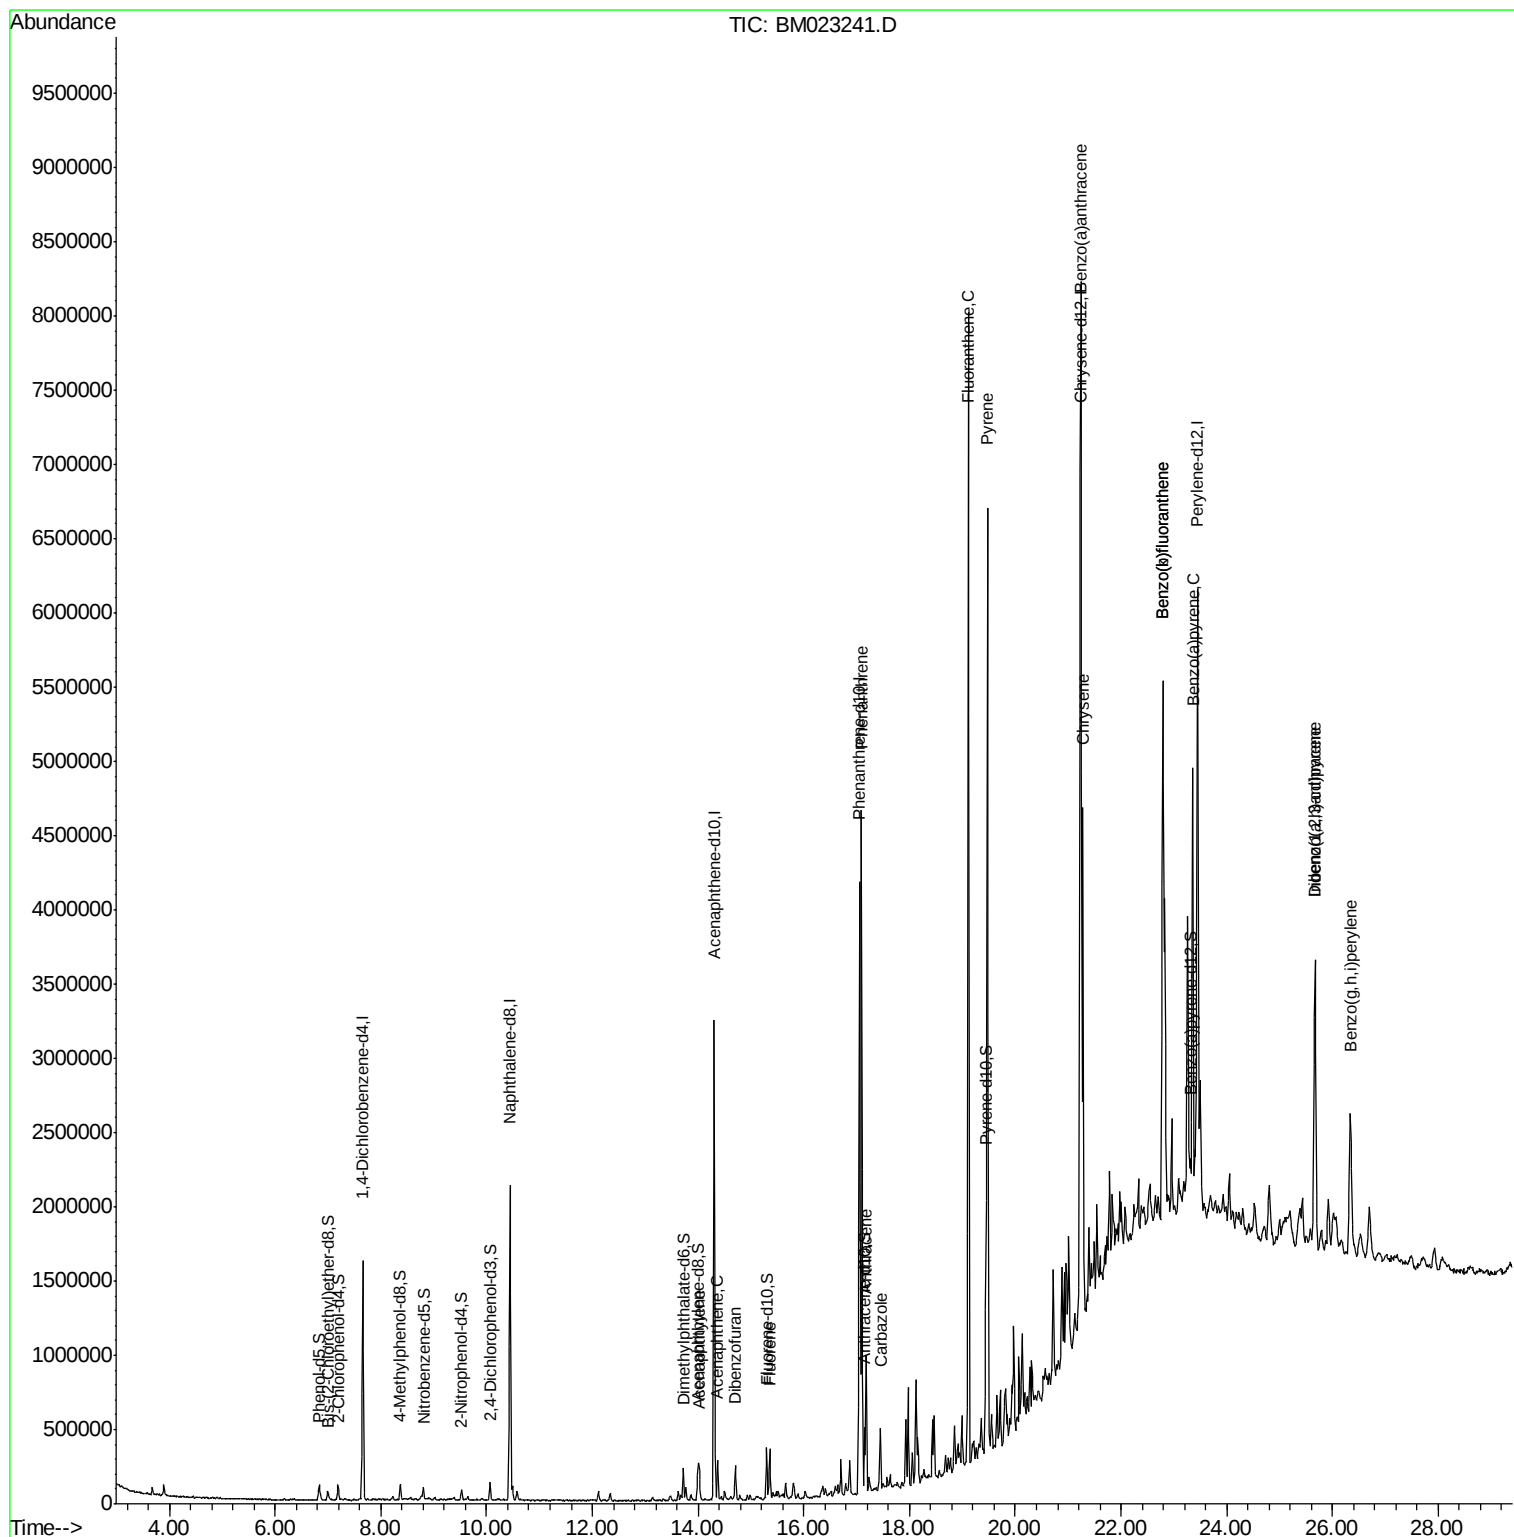

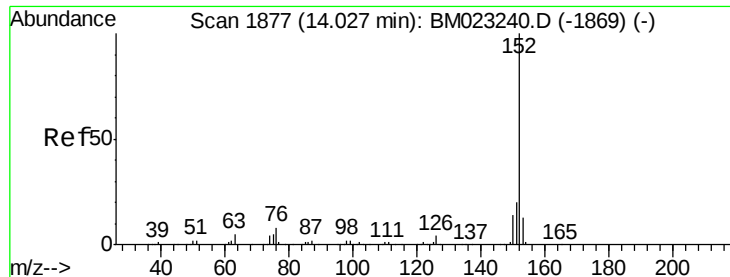

#48

Acenaphthylene

Concen: 1.372 ng/ul

RT: 14.02 min Scan# 1876

Delta R.T. -0.01 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion:152 Resp: 139415

Ion Ratio Lower Upper

152 100

151 20.7 15.8 23.6




153 13.5 10.3 15.5

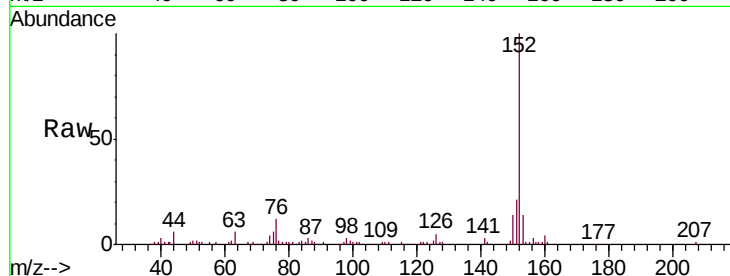

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

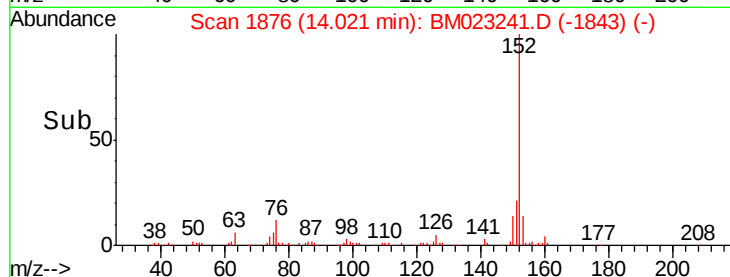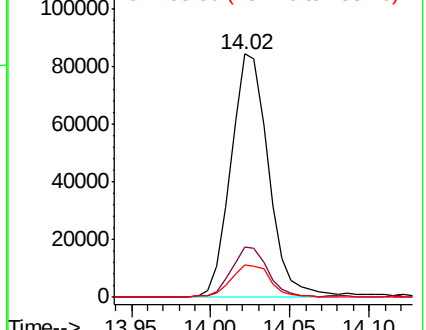

#50

Acenaphthene

Concen: 1.494 ng/ul

RT: 14.37 min Scan# 1935

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:153 Resp: 105716

Ion Ratio Lower Upper

153 100

152 45.0 38.0 57.0



154 89.4 70.4 105.6




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

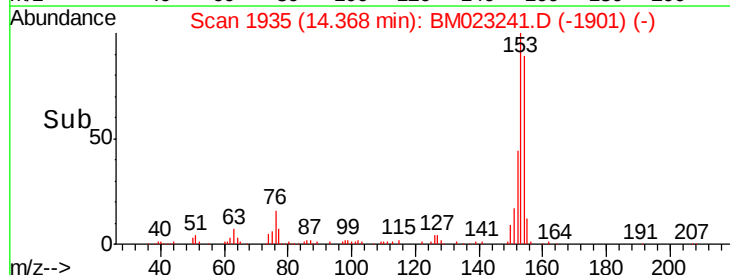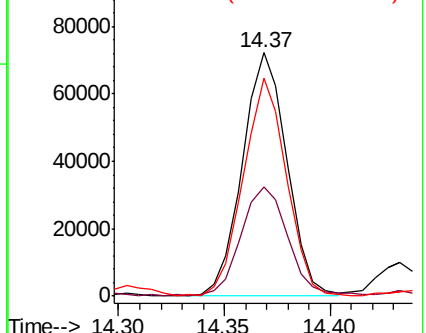

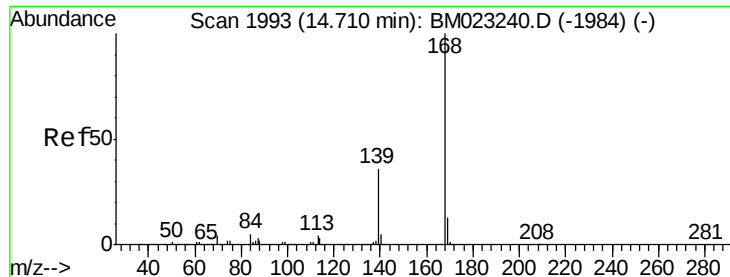

#54

Dibenzenofuran

Concen: 1.312 ng/ul

RT: 14.70 min Scan# 1992

Delta R.T. -0.01 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :


BFB79DL

Tgt Ion:168 Resp: 131757

Ion Ratio Lower Upper




168 100

139 38.8 30.1 45.1



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

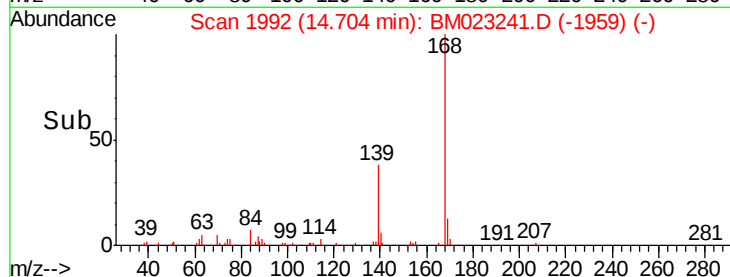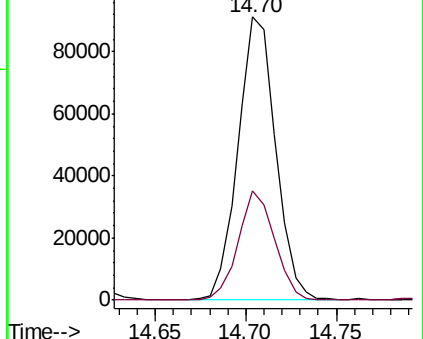

#59

Fluorene

Concen: 1.703 ng/ul

RT: 15.36 min Scan# 2103

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:166 Resp: 140293

Ion Ratio Lower Upper

166 100

165 97.8 77.4 116.0



167 14.5 10.8 16.2




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

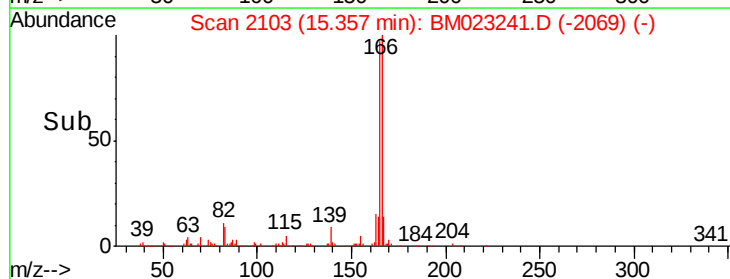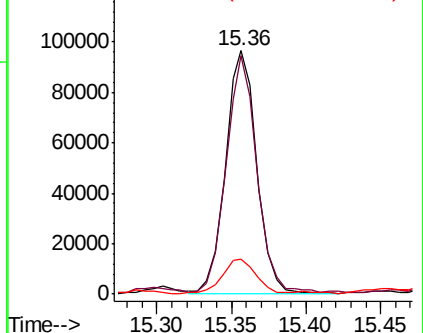

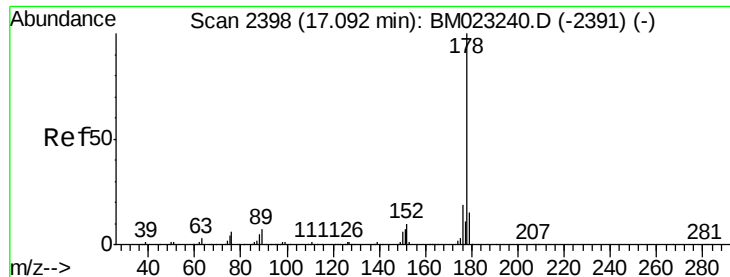

#70

Phenanthrene

Concen: 20.453 ng/ul

RT: 17.09 min Scan# 2398

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion:178 Resp: 2697046

Ion Ratio Lower Upper




178 100

179 15.5 12.3 18.5

176 19.2 15.5 23.3



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

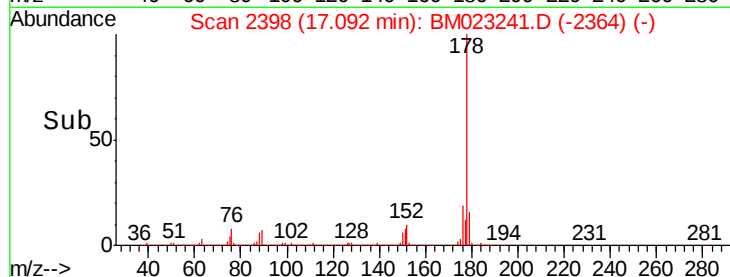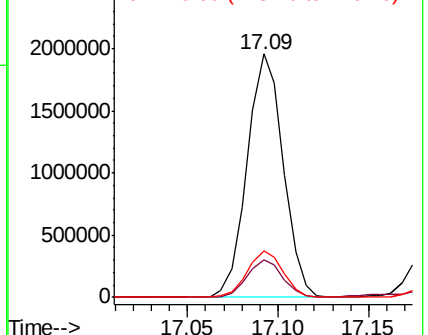

#72

Anthracene

Concen: 4.245 ng/ul

RT: 17.18 min Scan# 2413

Delta R.T. -0.01 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:178 Resp: 578420

Ion Ratio Lower Upper



178 100


179 15.5 12.3 18.5

176 18.7 15.0 22.4



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

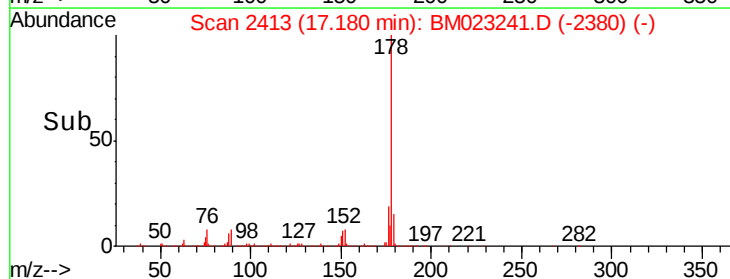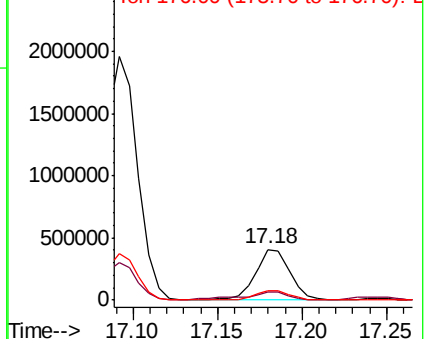

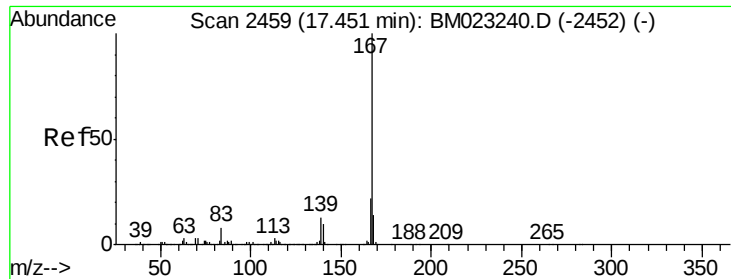

#75

Carbazole

Concen: 2.187 ng/ul

RT: 17.45 min Scan# 2459

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion:167 Resp: 266230

Ion Ratio Lower Upper

167 100

166 21.1 17.4 26.0




139 11.9 10.2 15.2

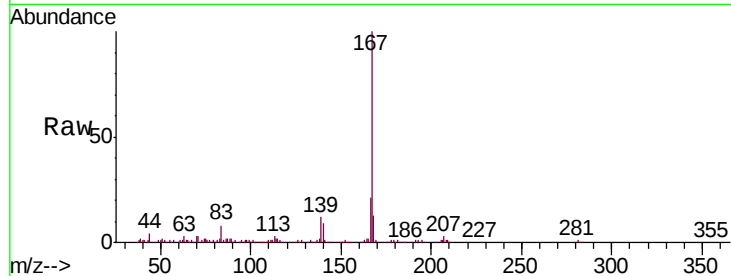

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

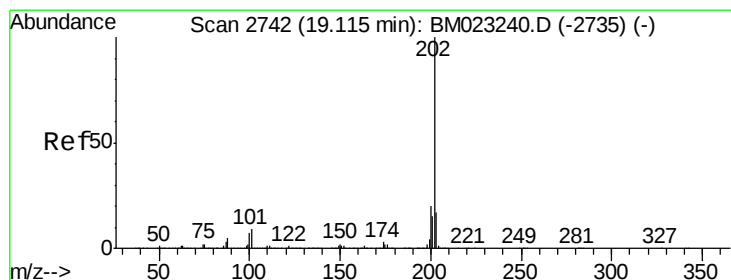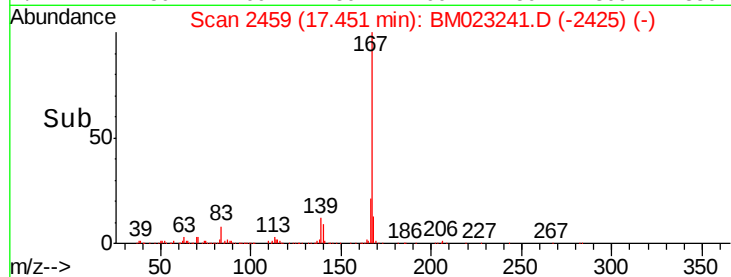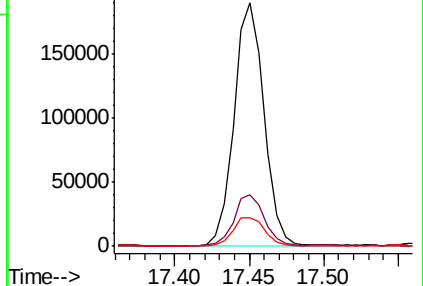

#77

Fluoranthene

Concen: 29.215 ng/ul

RT: 19.12 min Scan# 2742

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:202 Resp: 4581837

Ion Ratio Lower Upper

202 100

101 9.3 7.8 11.8



100 6.8 6.1 9.1

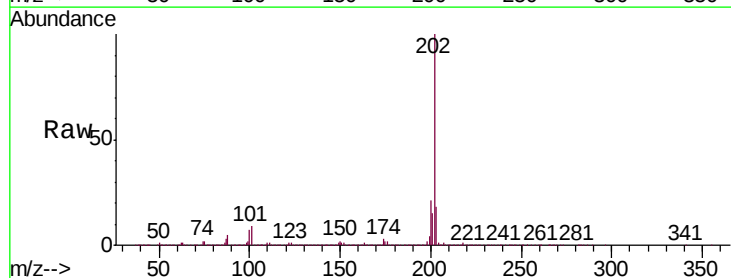


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

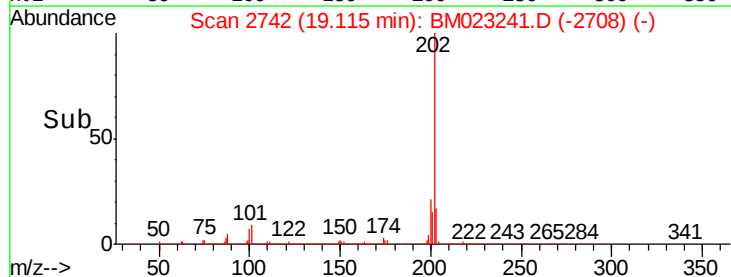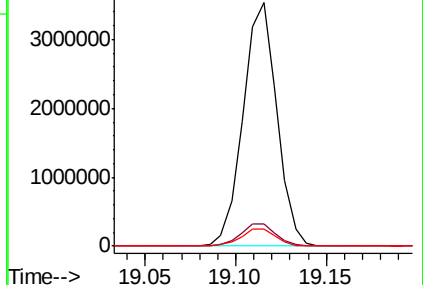

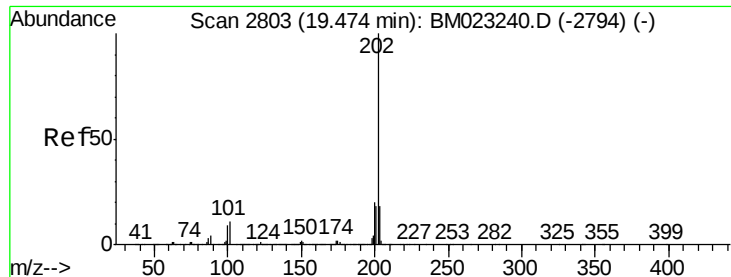

#80

Pyrene

Concen: 24.715 ng/ul

RT: 19.47 min Scan# 2803

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion:202 Resp: 3903644

Ion Ratio Lower Upper

202 100

101 11.1 9.1 13.7




100 9.3 7.5 11.3

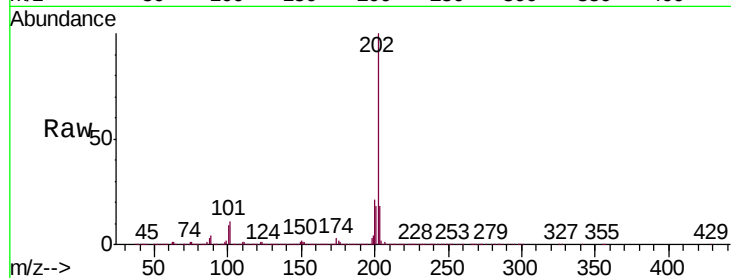

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

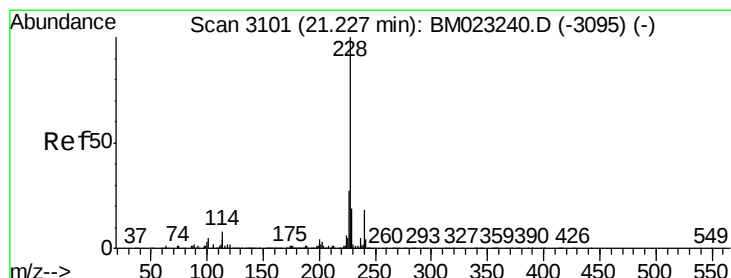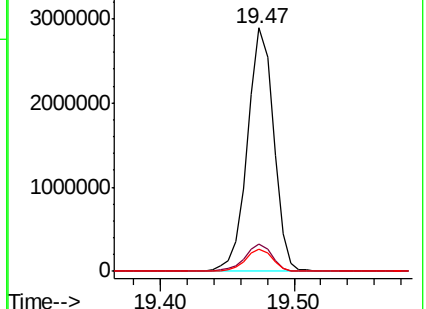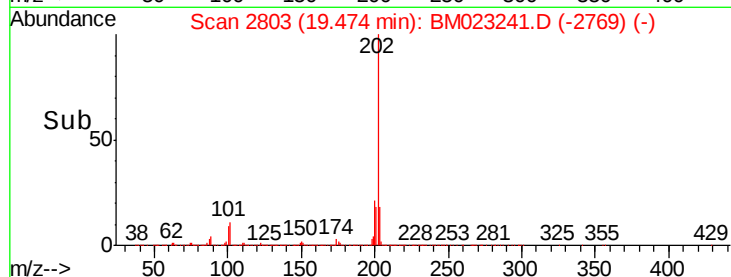

#83

Benzo(a)anthracene

Concen: 12.504 ng/ul

RT: 21.23 min Scan# 3101

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:228 Resp: 2136121

Ion Ratio Lower Upper

228 100

229 20.7 15.7 23.5



226 28.2 21.6 32.4

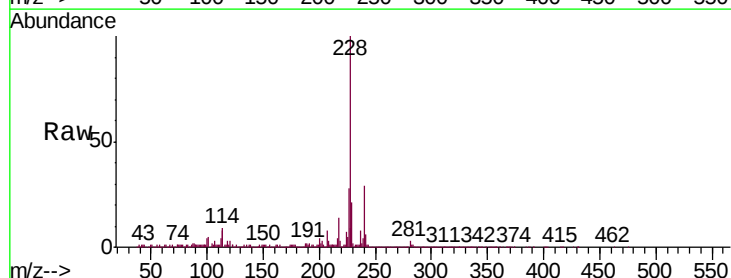


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

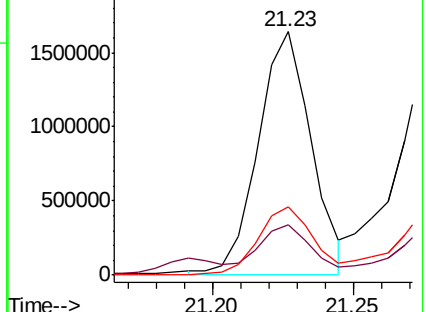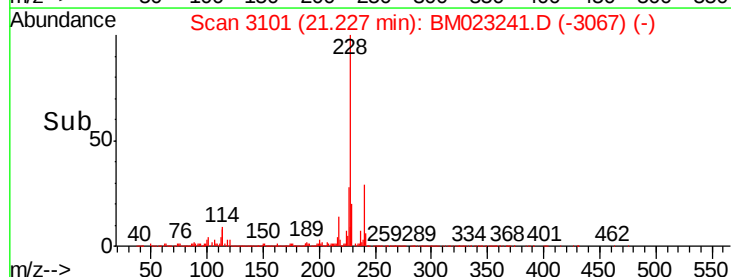

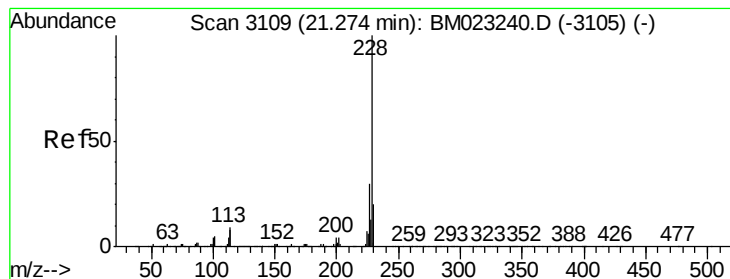

#85

Chrysene

Concen: 12.941 ng/ul

RT: 21.27 min Scan# 3109

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion:228 Resp: 2052768

Ion Ratio Lower Upper

228 100

226 29.1 23.8 35.6

229 22.3 15.5 23.3






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

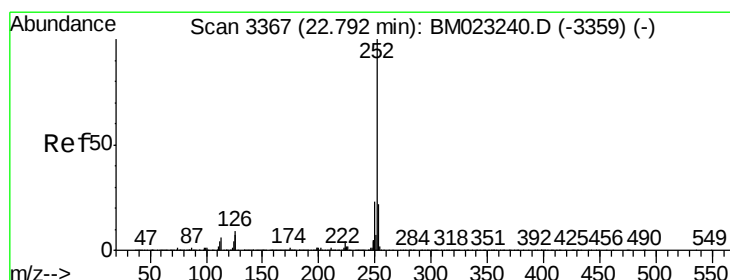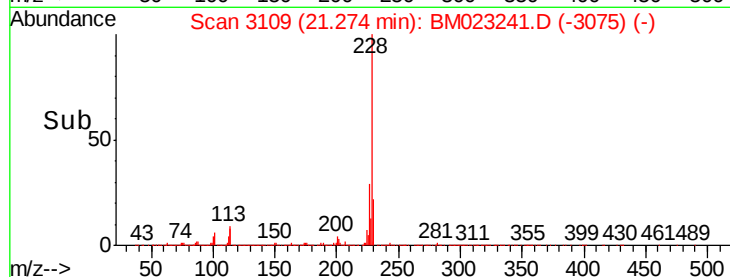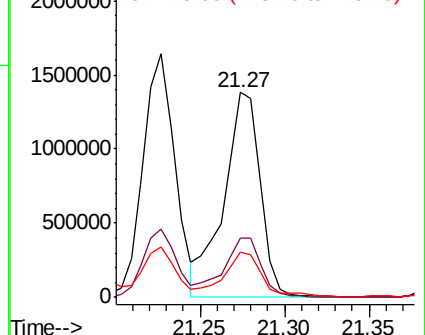

#88

Benzo(b)fluoranthene

Concen: 17.457 ng/ul

RT: 22.79 min Scan# 3367

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:252 Resp: 3186935

Ion Ratio Lower Upper

252 100

253 23.1 17.6 26.4

125 8.7 6.4 9.6






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

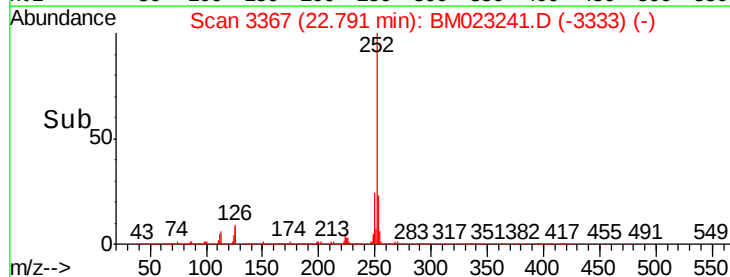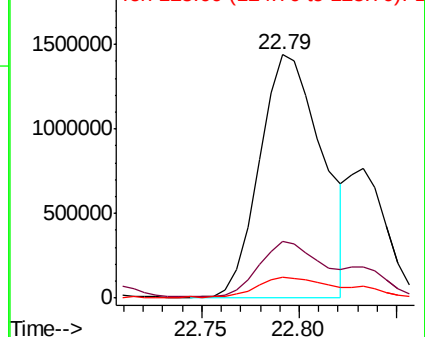

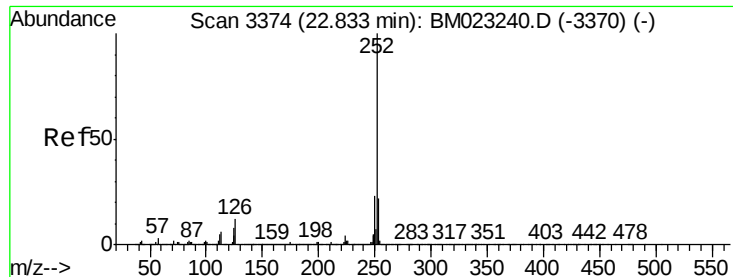

#89

Benzo(k)fluoranthene

Concen: 18.180 ng/ul

RT: 22.79 min Scan# 3367

Delta R.T. -0.04 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion:252 Resp: 3186935

Ion Ratio Lower Upper

252 100

253 23.1 17.4 26.0

125 8.7 6.5 9.7



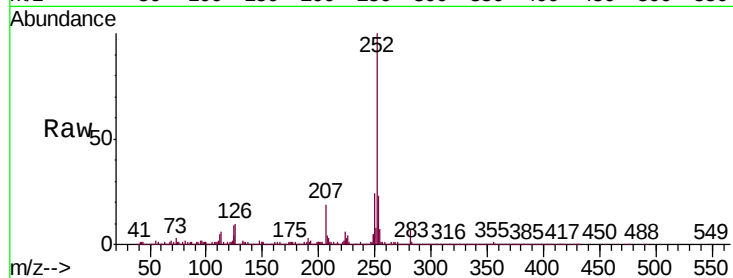


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

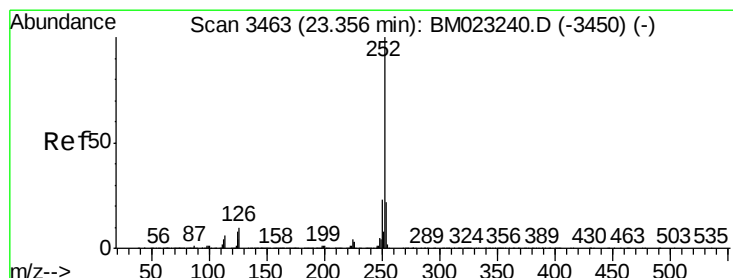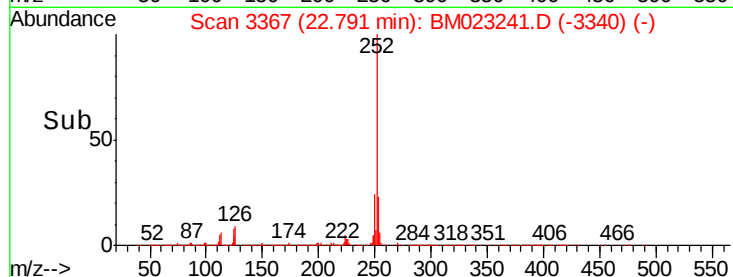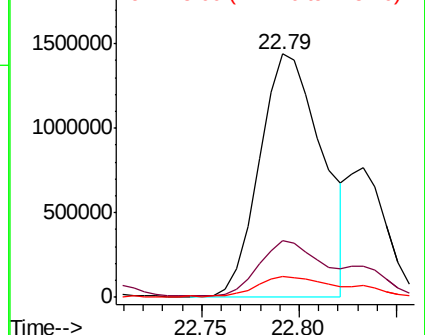

#91

Benzo(a)pyrene

Concen: 12.862 ng/ul

RT: 23.36 min Scan# 3463

Delta R.T. -0.00 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41


Tgt Ion:252 Resp: 2252774

Ion Ratio Lower Upper

252 100

253 22.7 17.2 25.8

125 8.2 7.4 11.0


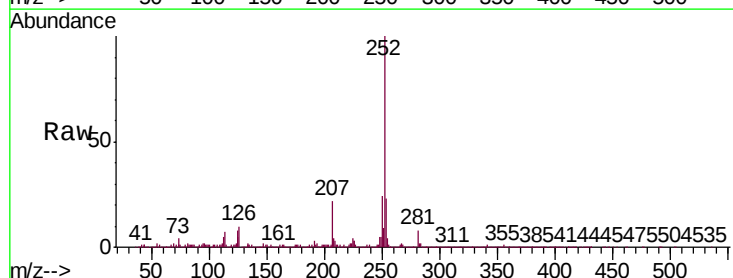



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

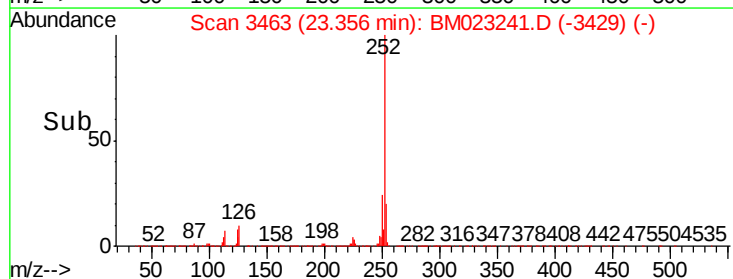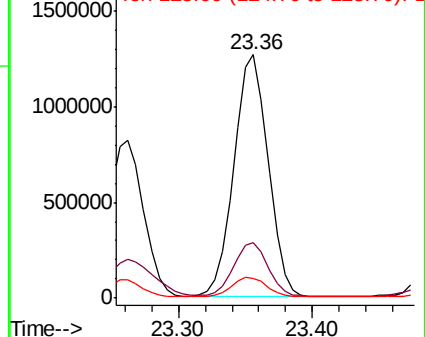




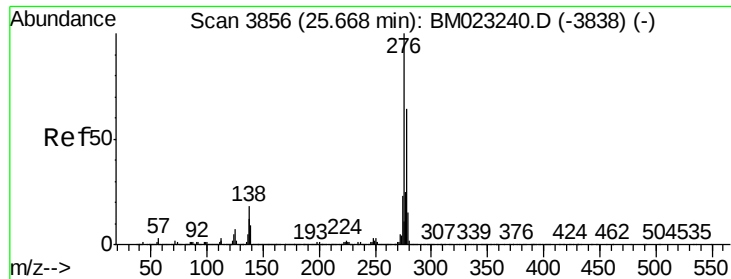


#92

Indeno(1,2,3-cd)pyrene
Concen: 8.462 ng/ul
RT: 25.67 min Scan# 3856
Delta R.T. -0.00 min
Lab File: BM023241.D
Acq: 18 Oct 2019 04:41

Instrument :
BNA_M
ClientSampleId :
BFB79DL




Tgt Ion:276 Resp: 1763152
Ion Ratio Lower Upper
276 100
138 15.6 14.9 22.3
277 25.0 19.8 29.8

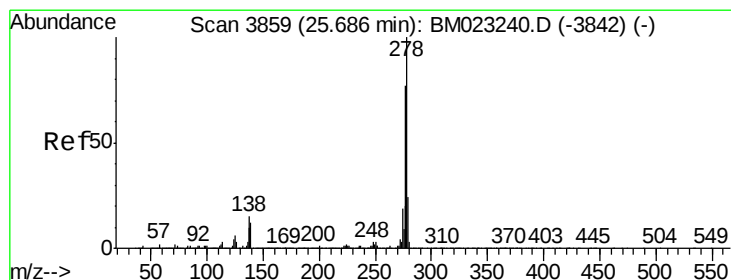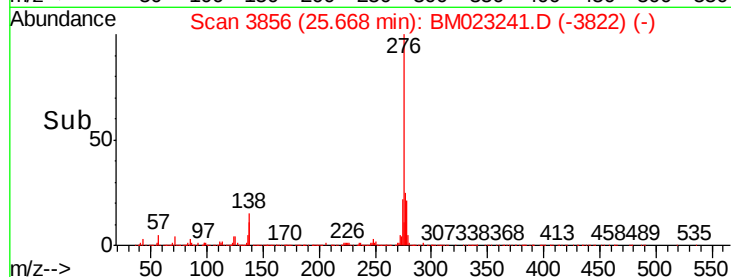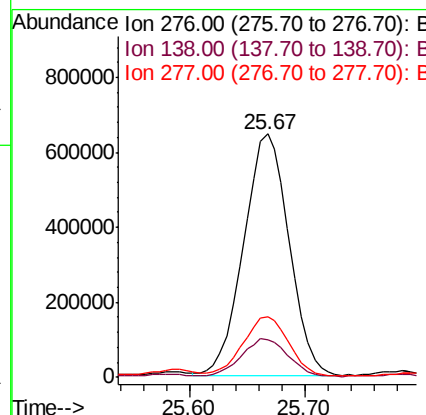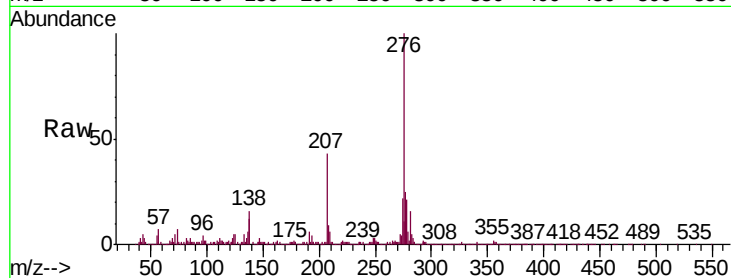


#93

Dibenzo(a,h)anthracene
Concen: 2.567 ng/ul
RT: 25.67 min Scan# 3857
Delta R.T. -0.01 min
Lab File: BM023241.D
Acq: 18 Oct 2019 04:41

Tgt Ion:278 Resp: 447232
Ion Ratio Lower Upper
278 100
139 17.0 10.0 15.0#
279 27.7 19.4 29.0

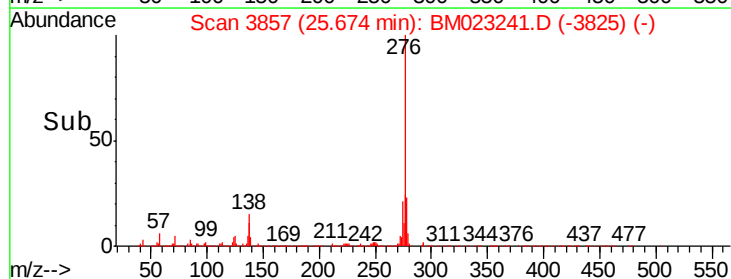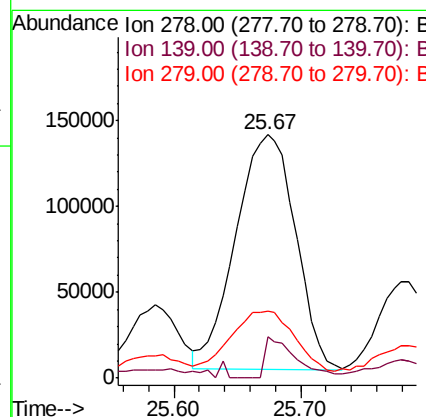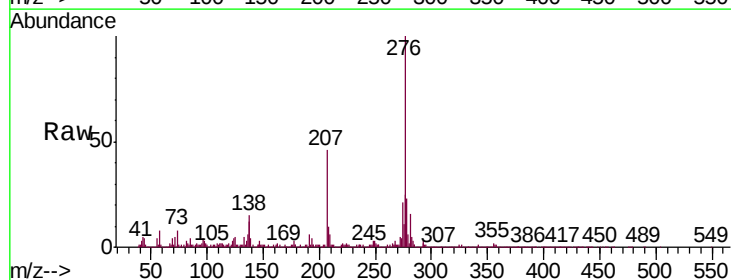

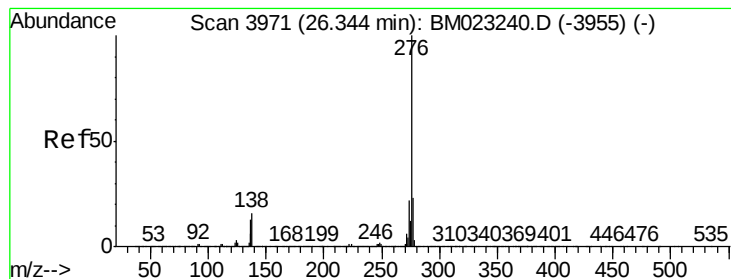

#94

Benzo(g,h,i)perylene

Concen: 7.137 ng/ul

RT: 26.34 min Scan# 3970

Delta R.T. -0.01 min

Lab File: BM023241.D

Acq: 18 Oct 2019 04:41

Instrument :

BNA_M

ClientSampleId :

BFB79DL


Tgt Ion: 276 Resp: 1224340

Ion Ratio Lower Upper

276 100

138 17.3 14.4 21.6

277 24.3 19.4 29.2

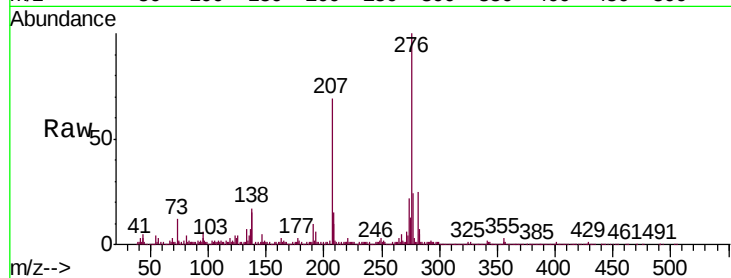

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

